


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090424\
Data File : BF139233.D
Acq On : 04 Sep 2024 11:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 04 16:11:43 2024

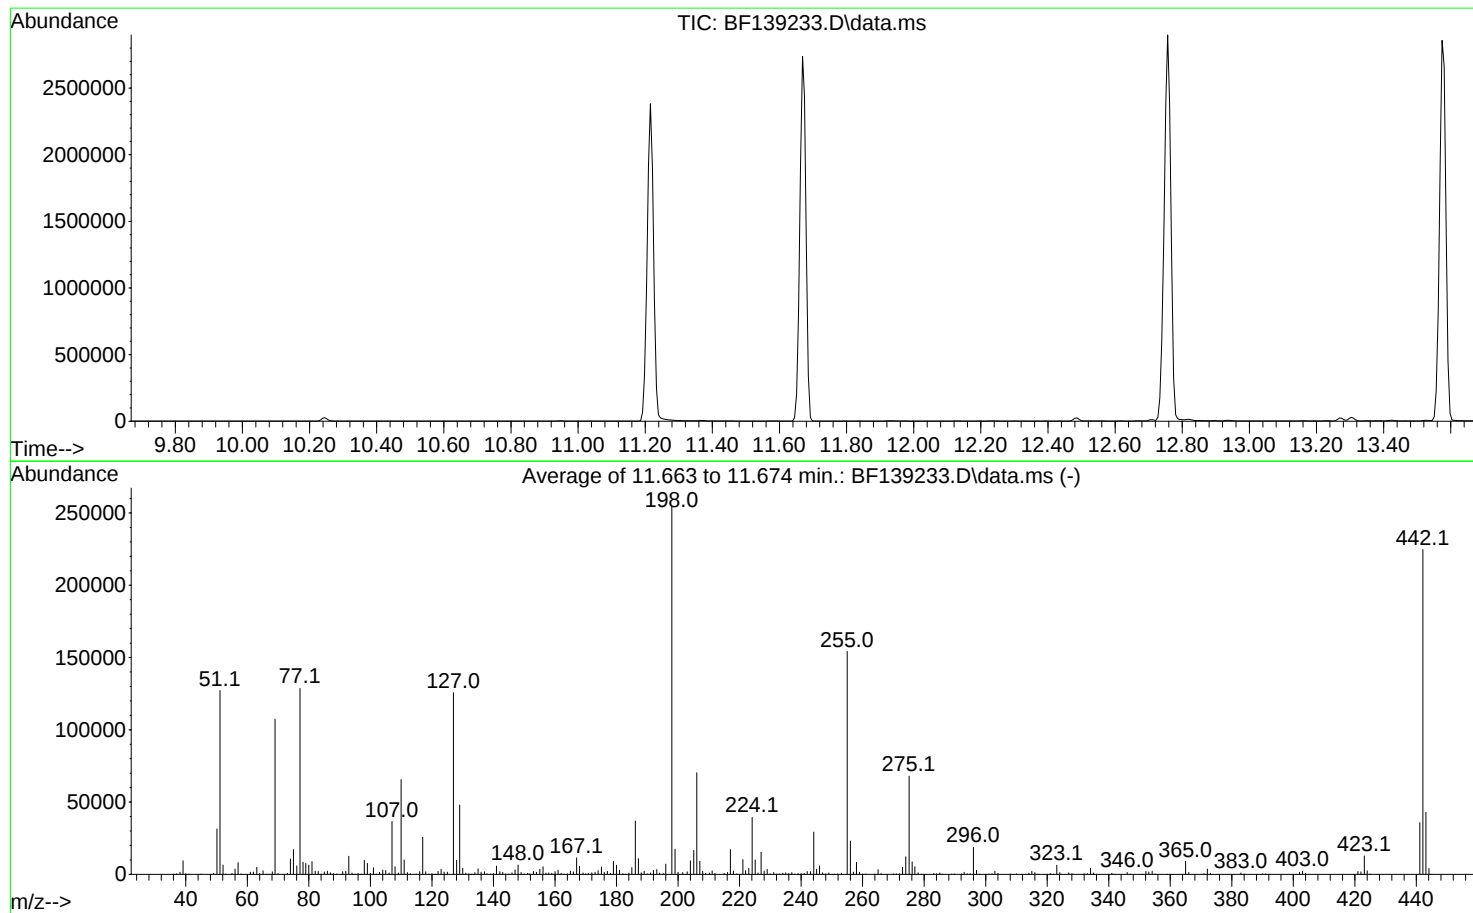




AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.0	127155	PASS
68	69	0.00	2	1.7	1798	PASS
69	198	0.00	100	42.2	107411	PASS
70	69	0.00	2	0.6	595	PASS
127	198	10	80	49.4	125733	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	254485	PASS
199	198	5	9	6.8	17414	PASS
275	198	10	60	26.7	67939	PASS
365	198	1	100	3.5	8972	PASS
441	198	0.01	100	14.1	35781	PASS
442	442	50	100	100.0	224683	PASS
443	442	15	24	19.1	42923	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090424\
Data File : BF139233.D
Acq On : 04 Sep 2024 11:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 04 13:35:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 13:35:04 2024
Response via : Initial Calibration

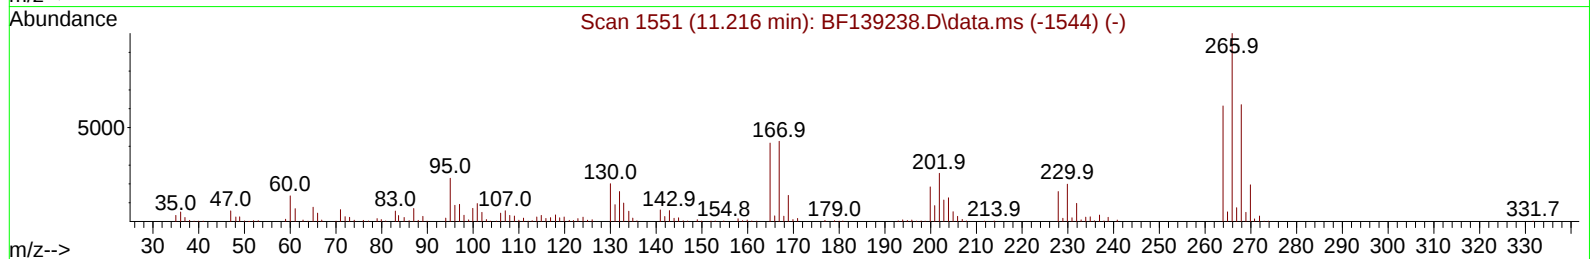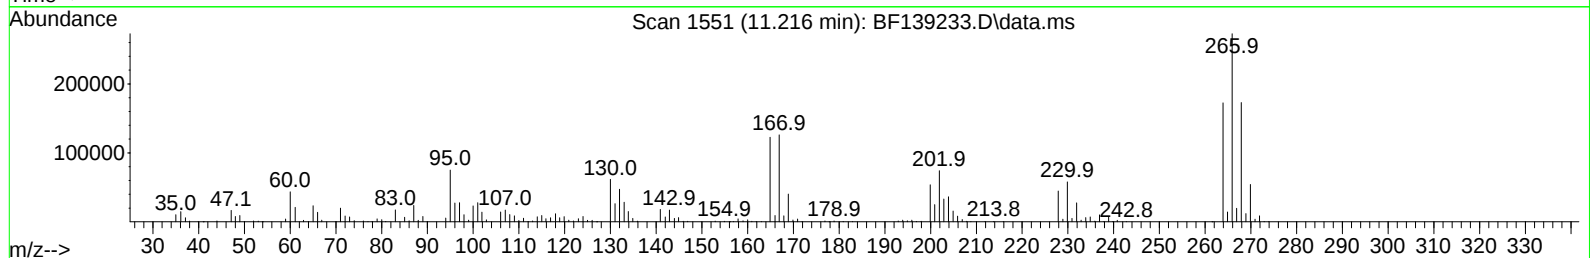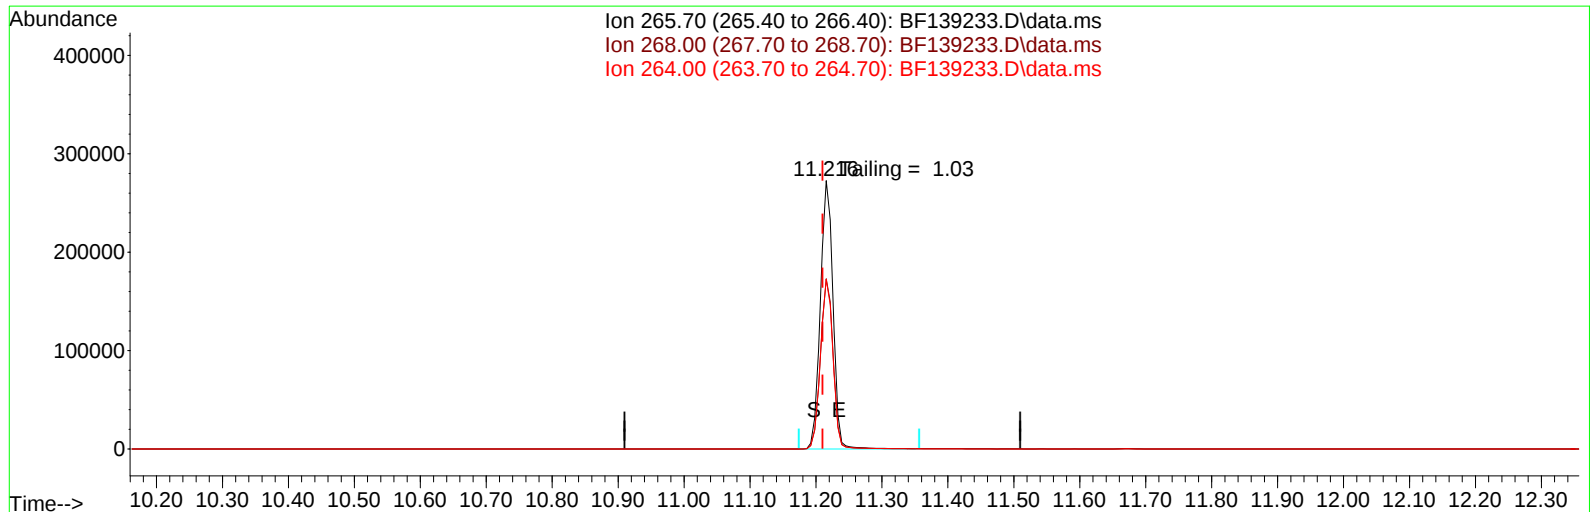

TIC: BF139233.D\data.ms

(70) Pentachlorophenol (C)

11.216min (+ 0.006) 32762.20 ng




response 363720

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.42
264.00	62.80	63.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090424\
Data File : BF139233.D
Acq On : 04 Sep 2024 11:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 04 13:35:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 13:35:04 2024
Response via : Initial Calibration

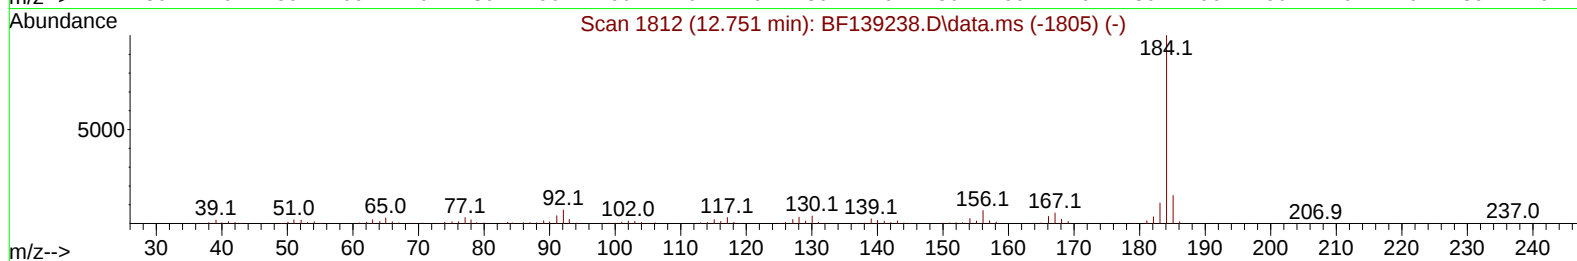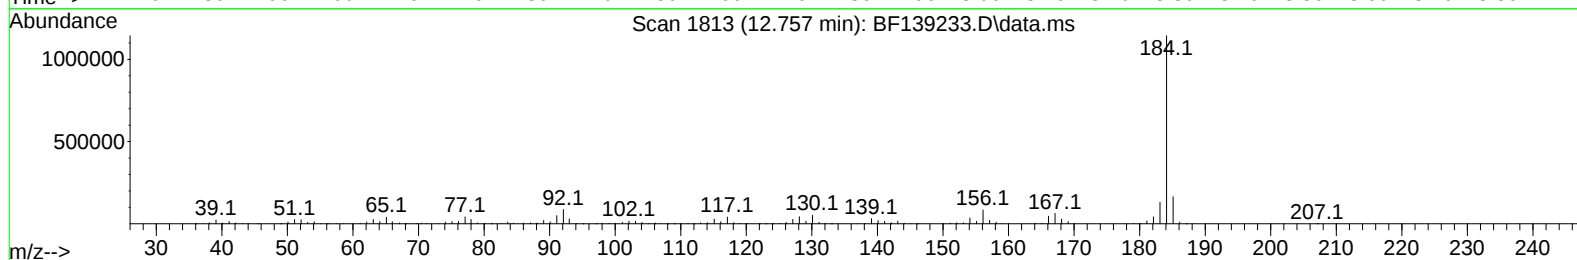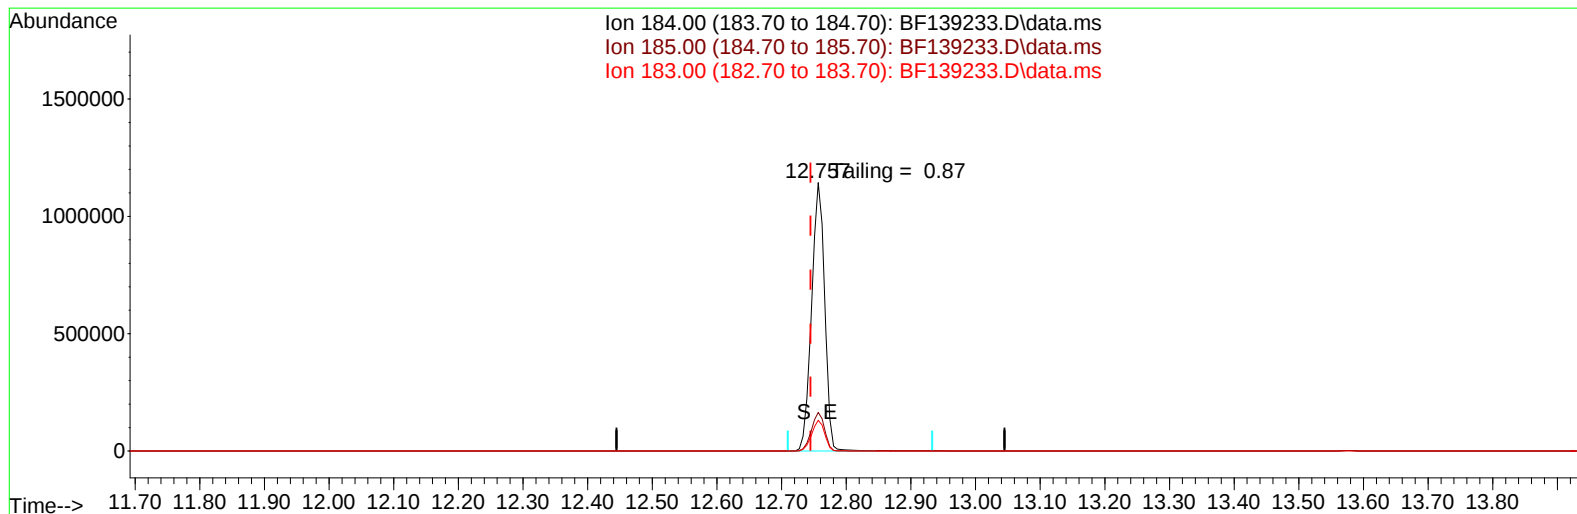

TIC: BF139233.D\data.ms

(77) Benzidine

12.757min (+ 0.012) 0.00 ng

response 1614907

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.39
183.00	11.90	11.45
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/4/2024	BNA_F	<u>BF139233.D</u>
Compound Name	Response	Retention Time
DDT	703410	13.574
DDD	12171	13.304
DDE	1008	12.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13179	716589	1.84

Instrument :
BNA_F
ClientSampleId :
DFTPP