


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090425\
Data File : BF143634.D
Acq On : 04 Sep 2025 07:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 03 18:35:49 2025

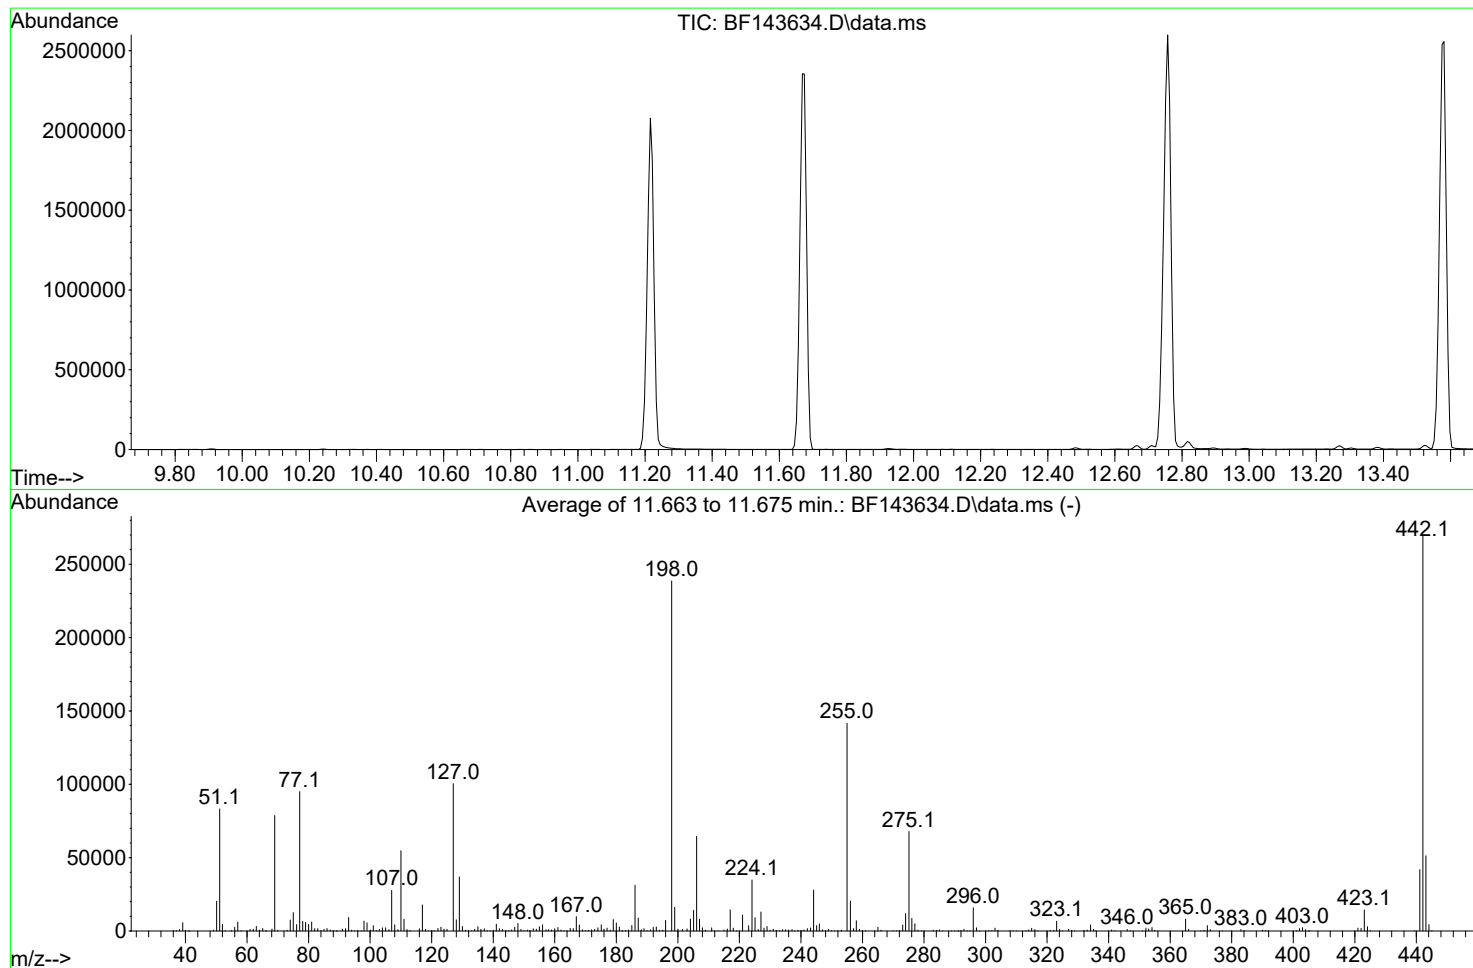

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1603

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.9	1473	PASS
69	69	100	100	100.0	78789	PASS
70	69	0.00	2	0.6	463	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	238635	PASS
199	198	5	9	6.8	16177	PASS
365	198	1	100	3.4	8100	PASS
441	443	0.01	150	81.8	41909	PASS
442	442	100	100	100.0	269163	PASS
443	442	15	24	19.0	51219	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/4/2025	BNA_F	<u>BF143634.D</u>
Compound Name	Response	Retention Time
DDT	721847	13.58
DDD	8465	13.269
DDE	495	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8960	730807	1.23

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090425\
Data File : BF143634.D
Acq On : 04 Sep 2025 07:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 04 08:41:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 03 18:35:49 2025
Response via : Initial Calibration

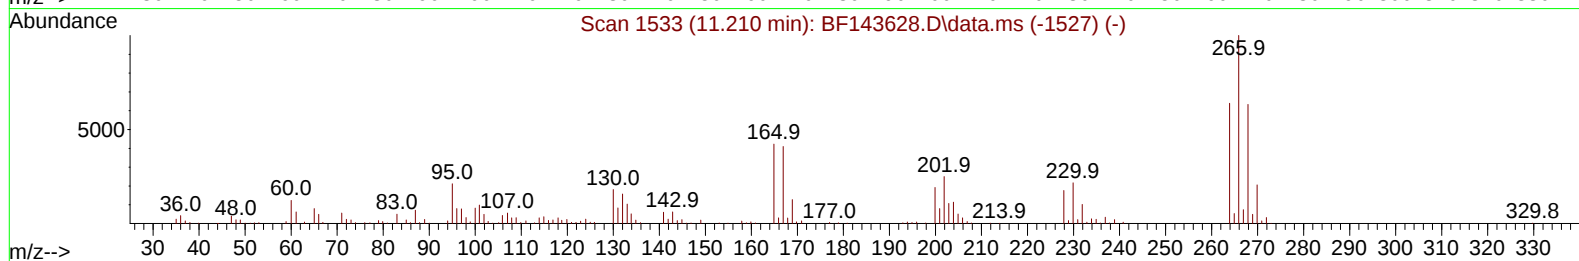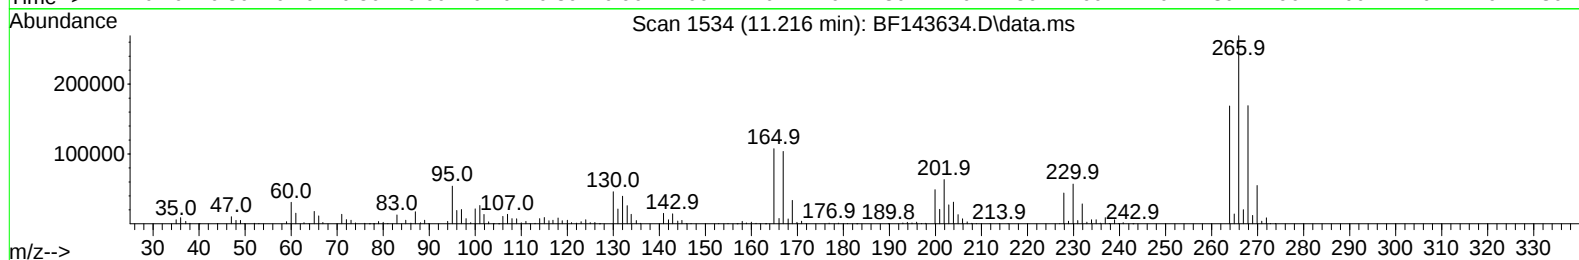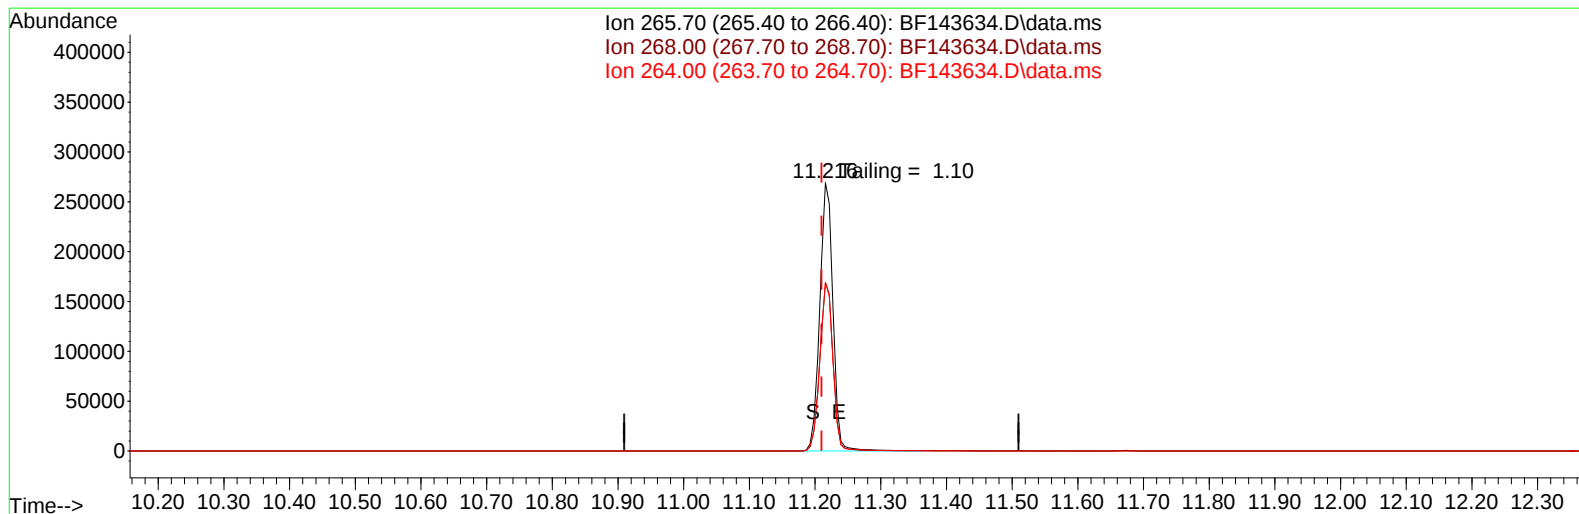

TIC: BF143634.D\data.ms

(70) Pentachlorophenol (C)

11.216min (+ 0.006) 233421.96 ng




response 375390

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	62.85
264.00	64.00	62.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090425\
Data File : BF143634.D
Acq On : 04 Sep 2025 07:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 04 08:41:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 03 18:35:49 2025
Response via : Initial Calibration

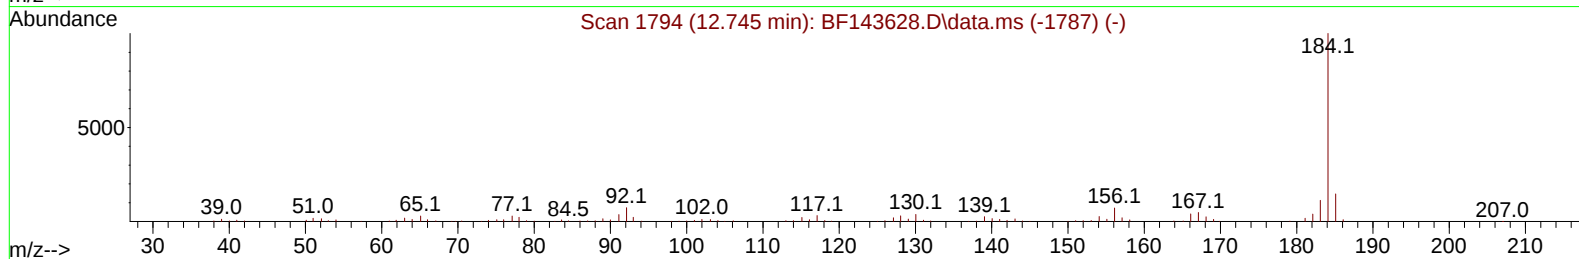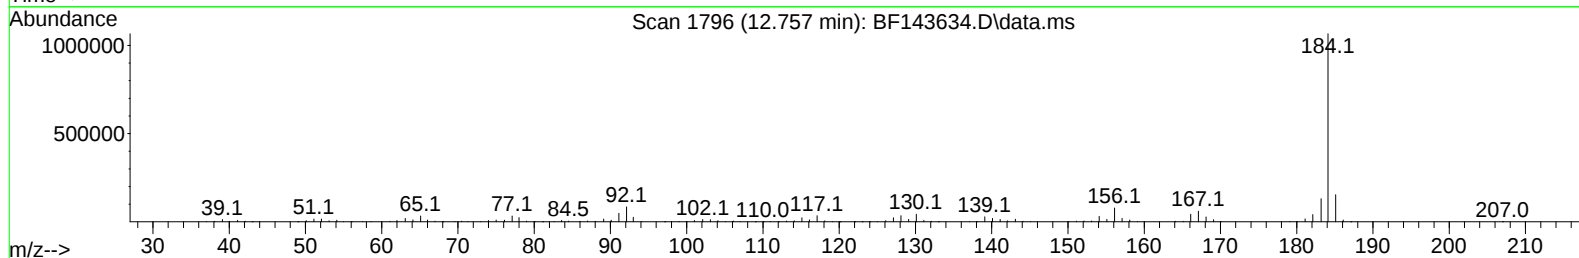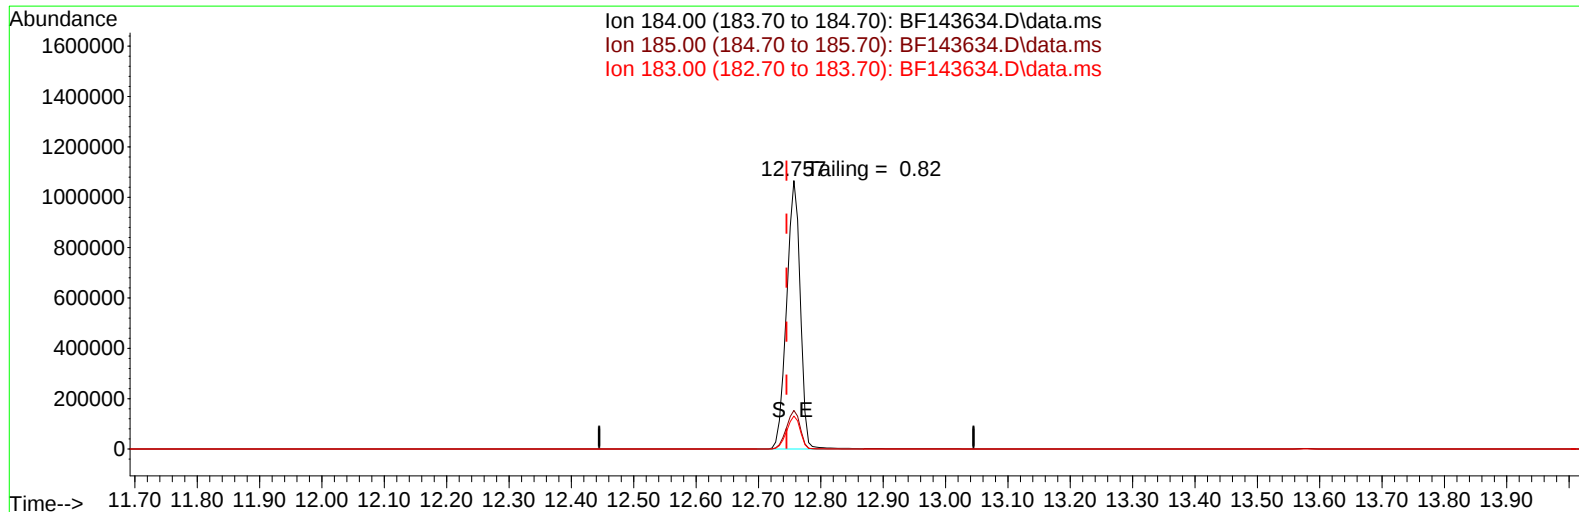

TIC: BF143634.D\data.ms

(77) Benzidine

12.757min (+ 0.012) 165192.76 ng

response 1628935

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.42
183.00	11.30	12.31
0.00	0.00	0.00