
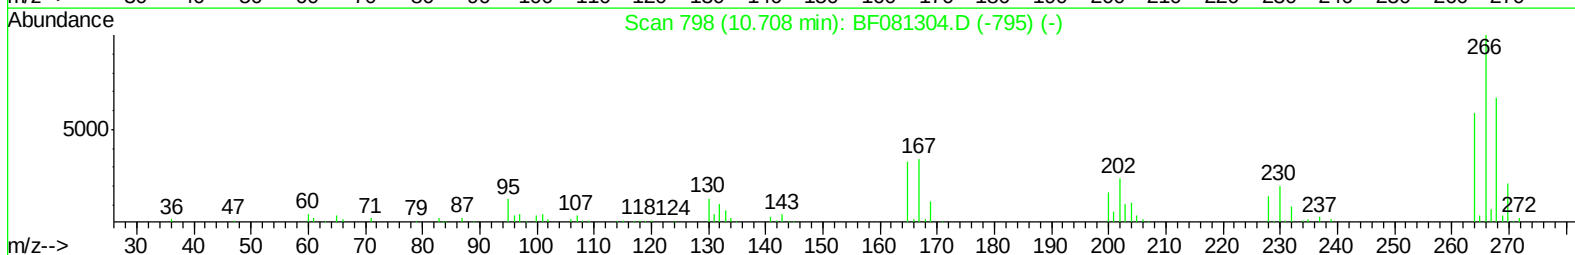
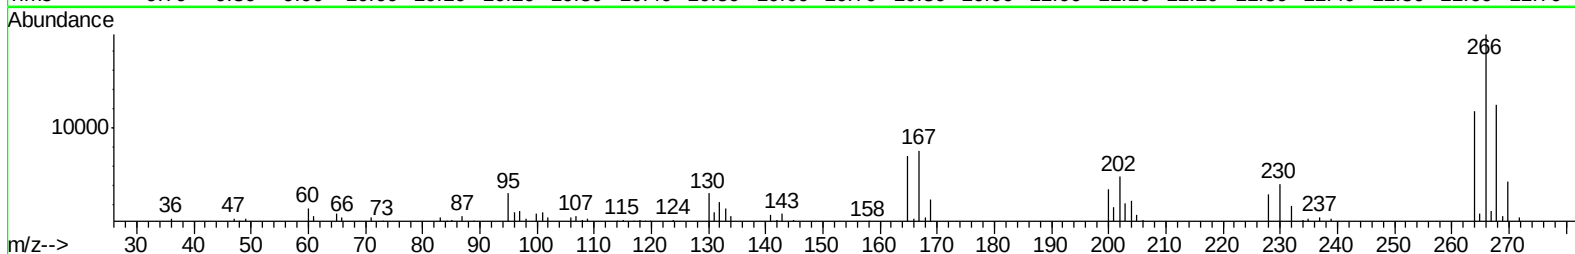


Data Path : Z:\HPCHEM1\BNA_F\Data\BF090515\
Data File : BF081474.D
Acq On : 5 Sep 2015 20:26
Operator : UM/IZ
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 07 04:08:17 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 07 02:47:26 2015
Response via : Initial Calibration

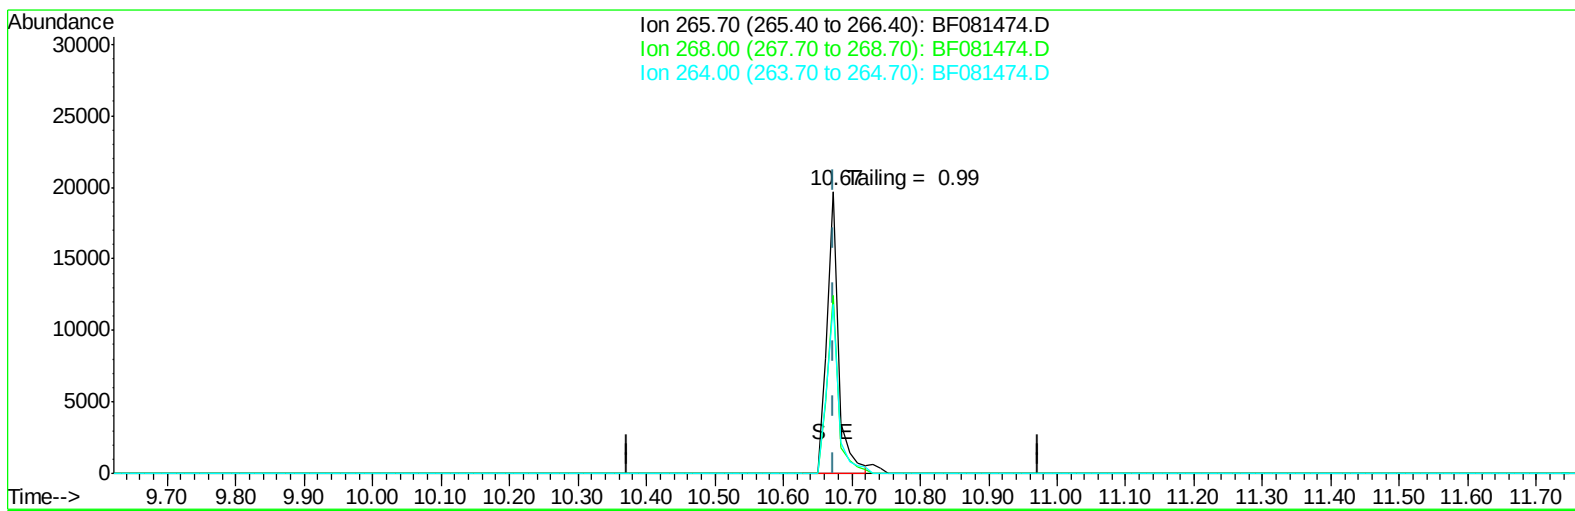

TIC: BF081474.D

(69) Pentachlorophenol (C)




10.673min (+0.000) 0.00ng

response 23861

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	63.00
264.00	62.70	59.84
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF090515\
Data File : BF081474.D
Acq On : 5 Sep 2015 20:26
Operator : UM/IZ
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 07 04:08:17 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 07 02:47:26 2015
Response via : Initial Calibration

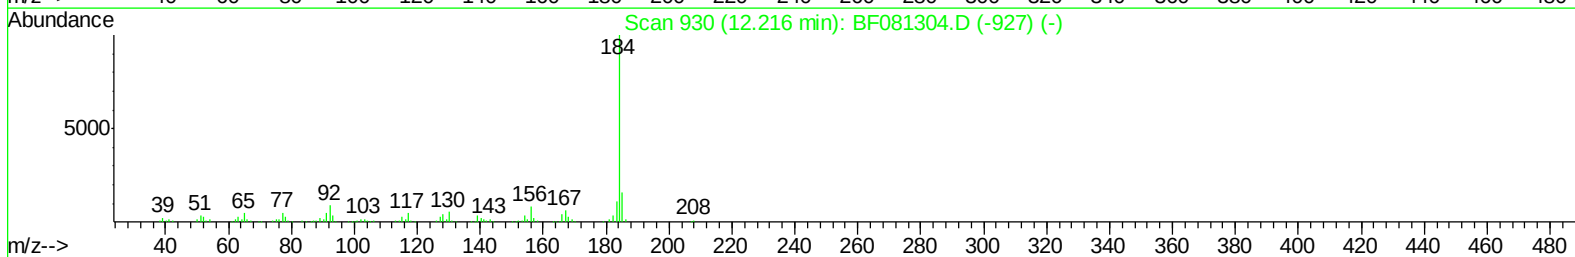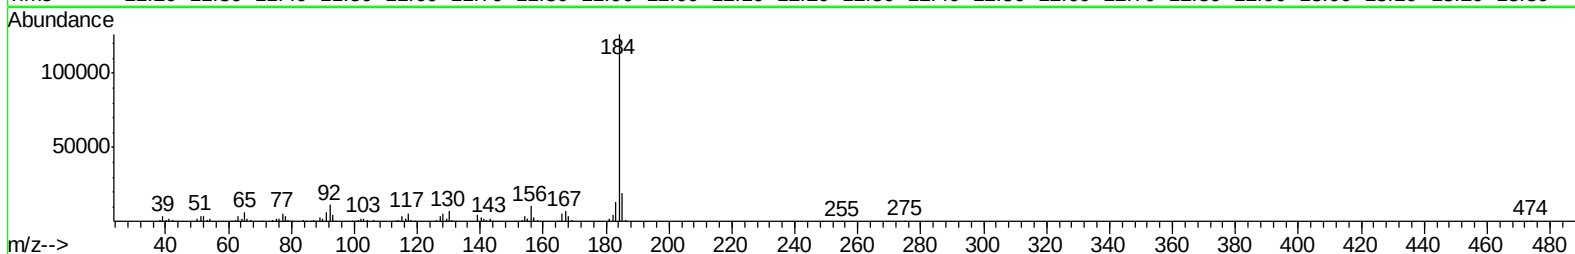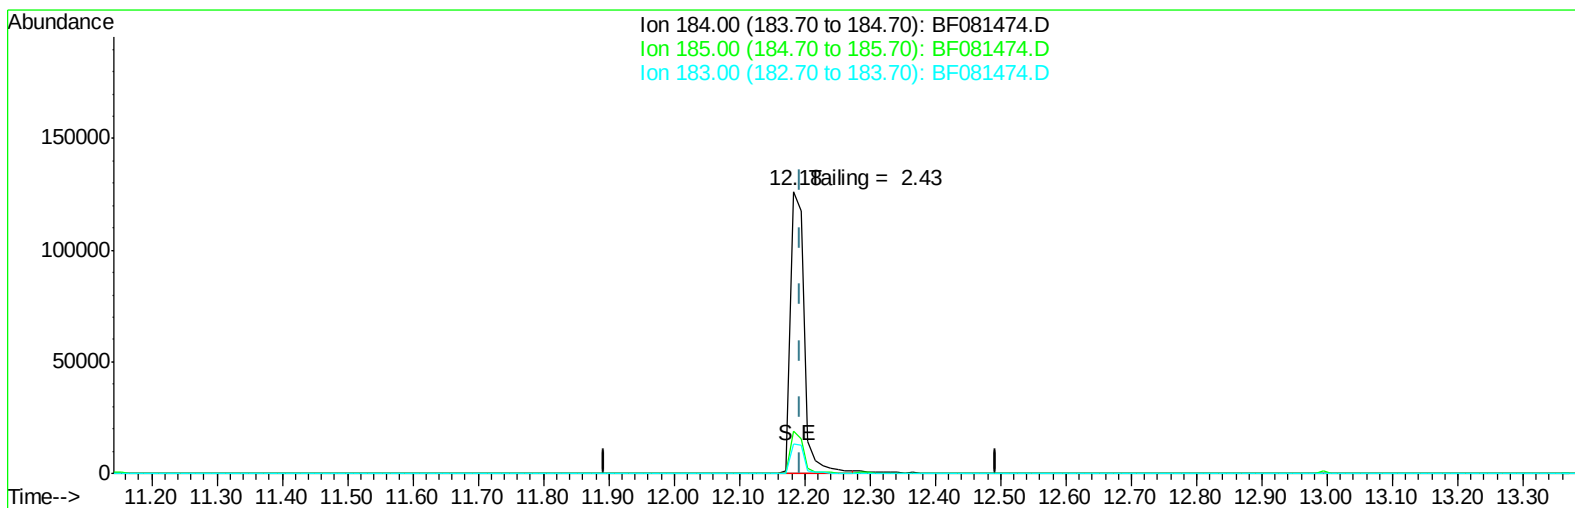

TIC: BF081474.D

(76) Benzidine

12.182min (-0.011) 0.00ng

response 190619

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	15.05
183.00	9.50	10.59
0.00	0.00	0.00