
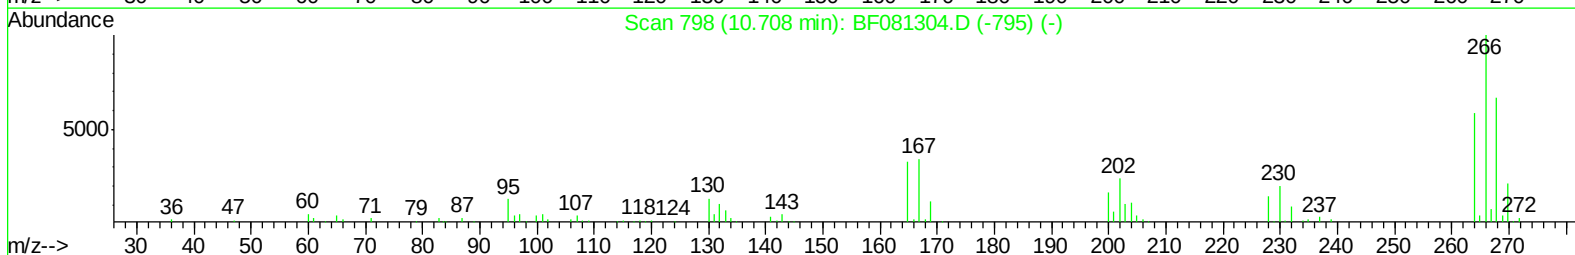
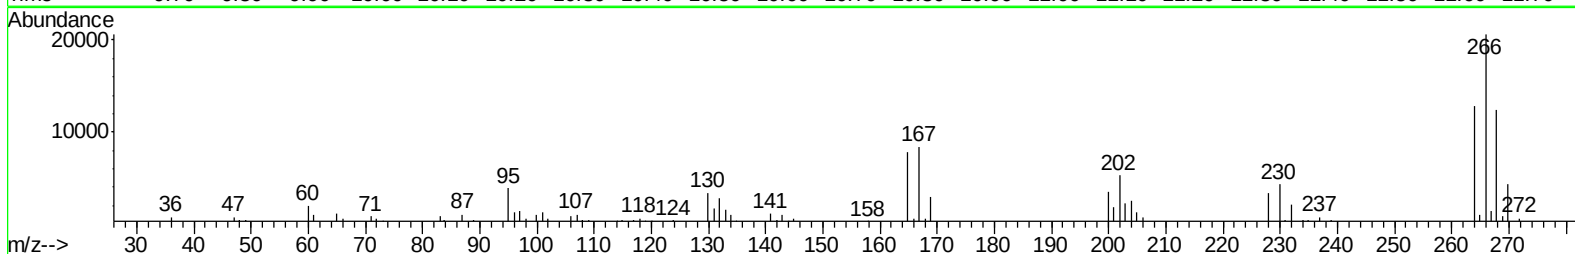


Data Path : Z:\HPCHEM1\BNA_F\Data\BF090515\
Data File : BF081497.D
Acq On : 6 Sep 2015 8:40
Operator : UM/IZ
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 08 17:20:12 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 08 15:49:53 2015
Response via : Initial Calibration

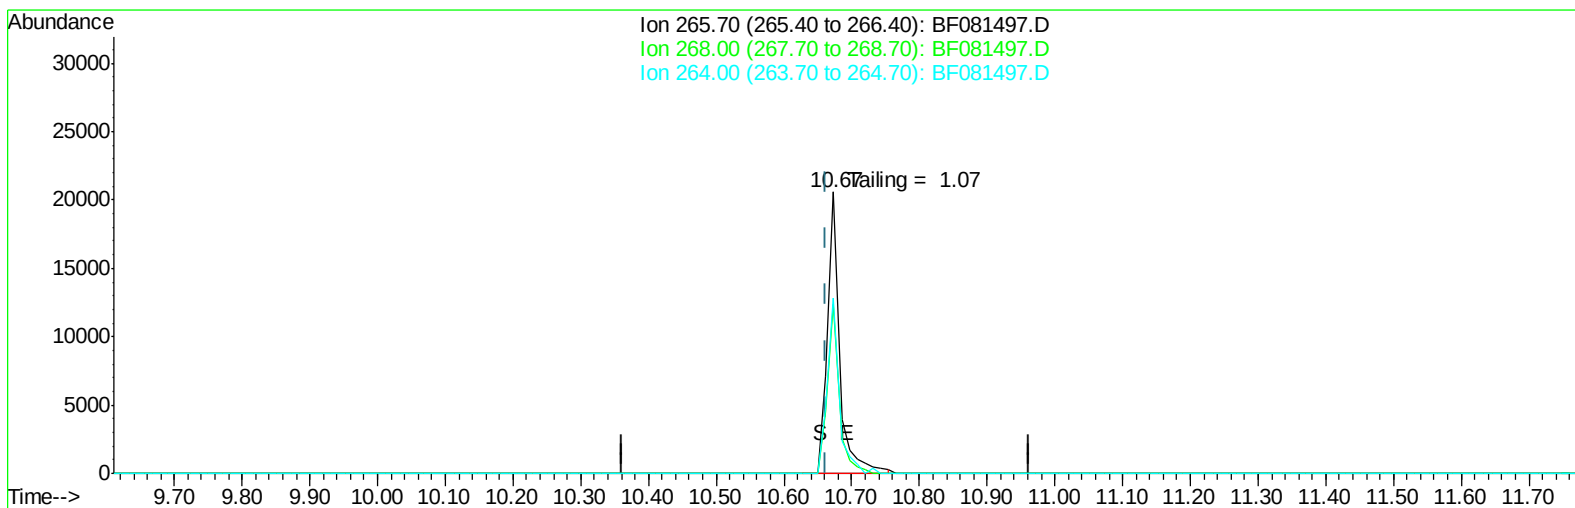

TIC: BF081497.D

(69) Pentachlorophenol (C)




10.674min (+0.012) 0.00ng

response 24832

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	60.17
264.00	62.70	62.23
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF090515\
Data File : BF081497.D
Acq On : 6 Sep 2015 8:40
Operator : UM/IZ
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 08 17:20:12 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 08 15:49:53 2015
Response via : Initial Calibration

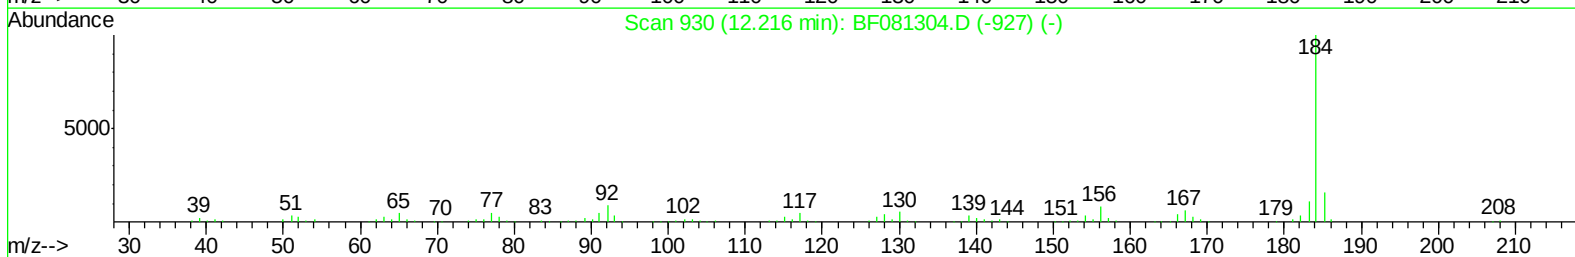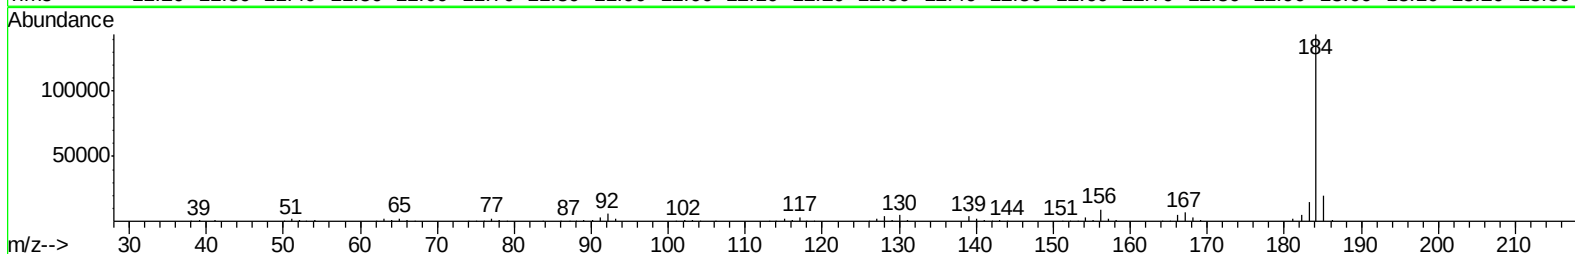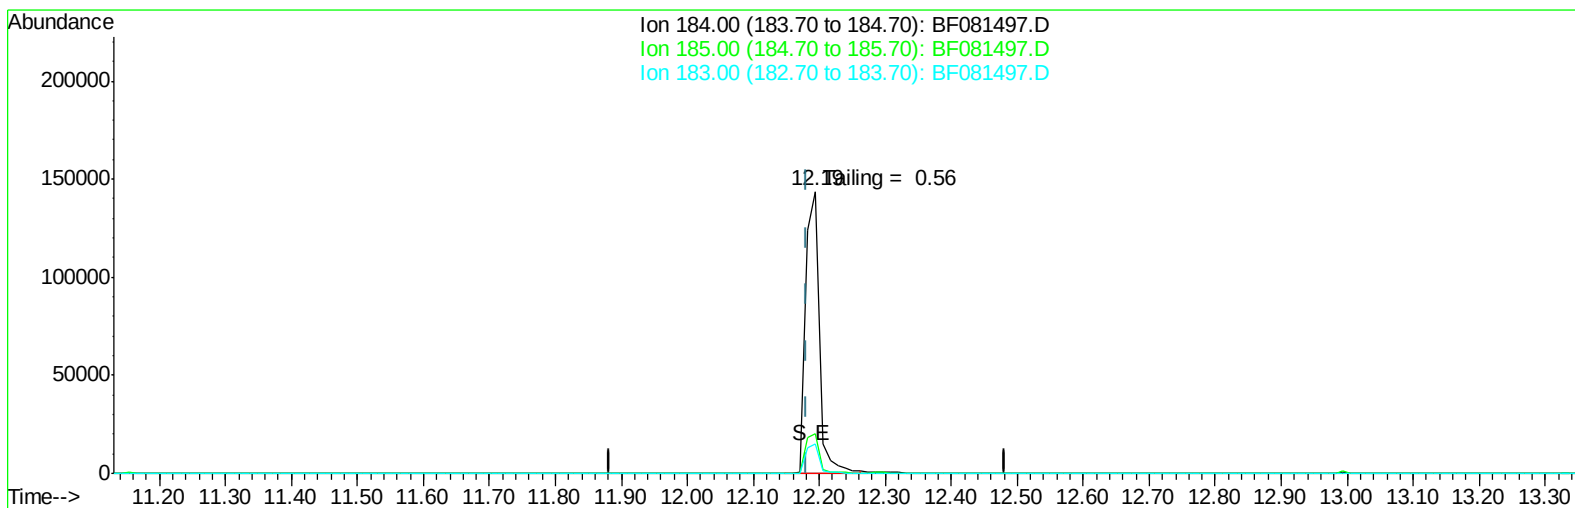

TIC: BF081497.D

(76) Benzidine

12.194min (+0.012) 0.00ng

response 208025

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.22
183.00	9.50	10.31
0.00	0.00	0.00