


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF090515\
 Data File : BF081474.D
 Acq On : 5 Sep 2015 20:26
 Operator : UM/IZ
 Sample : DFTTP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTTP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 08 15:49:53 2015

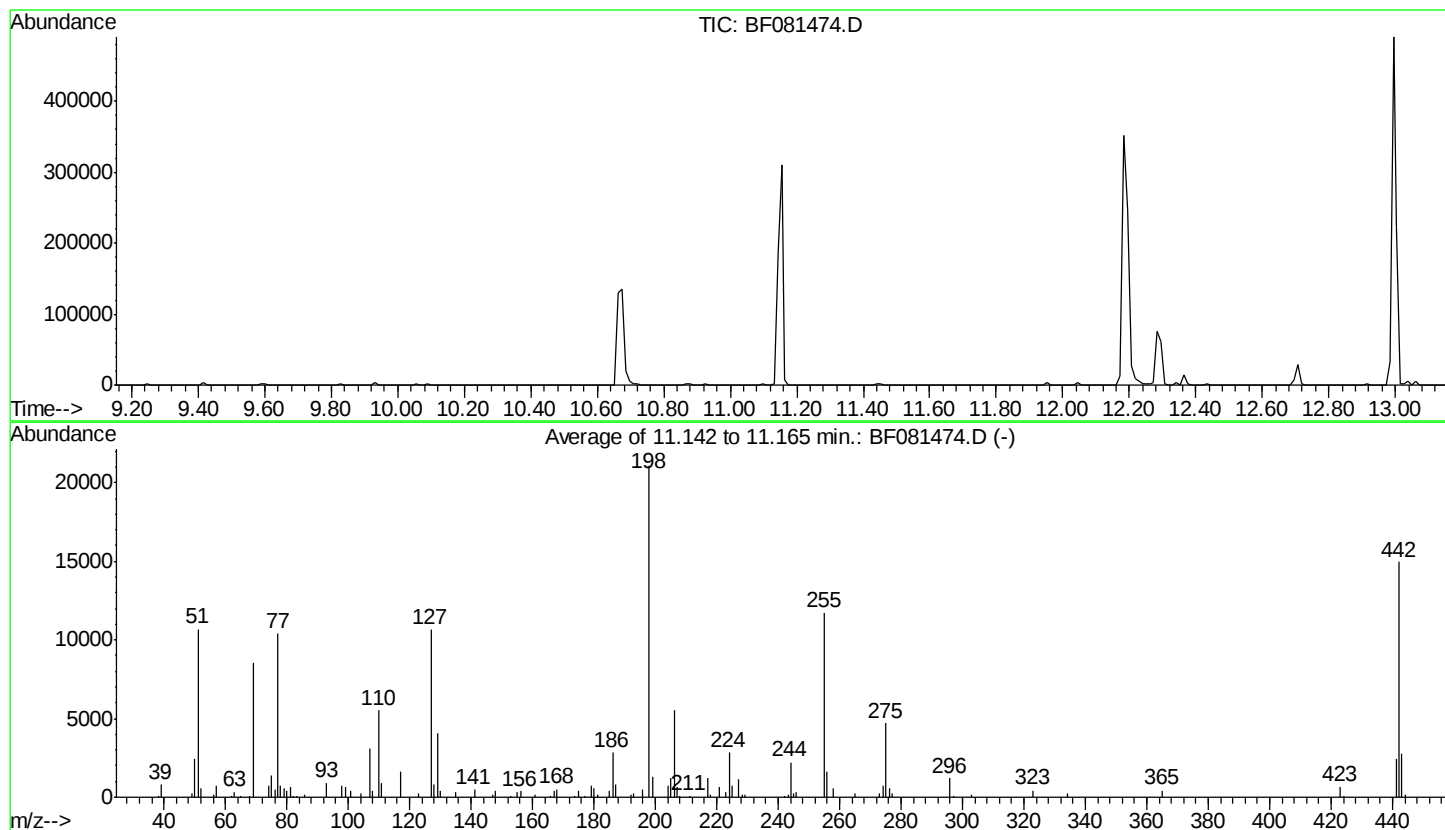

AutoFind: Scans 836, 837, 838; Background Corrected with Scan 833

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.7	10682	PASS
68	69	0.00	2	1.2	105	PASS
69	198	0.00	100	40.6	8571	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.5	10656	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	21088	PASS
199	198	5	9	6.1	1290	PASS
275	198	10	60	22.3	4700	PASS
365	198	1	100	2.1	446	PASS
441	442	0.01	24	16.4	2449	PASS
442	198	50	100	71.0	14973	PASS
443	442	15	24	18.5	2765	PASS