
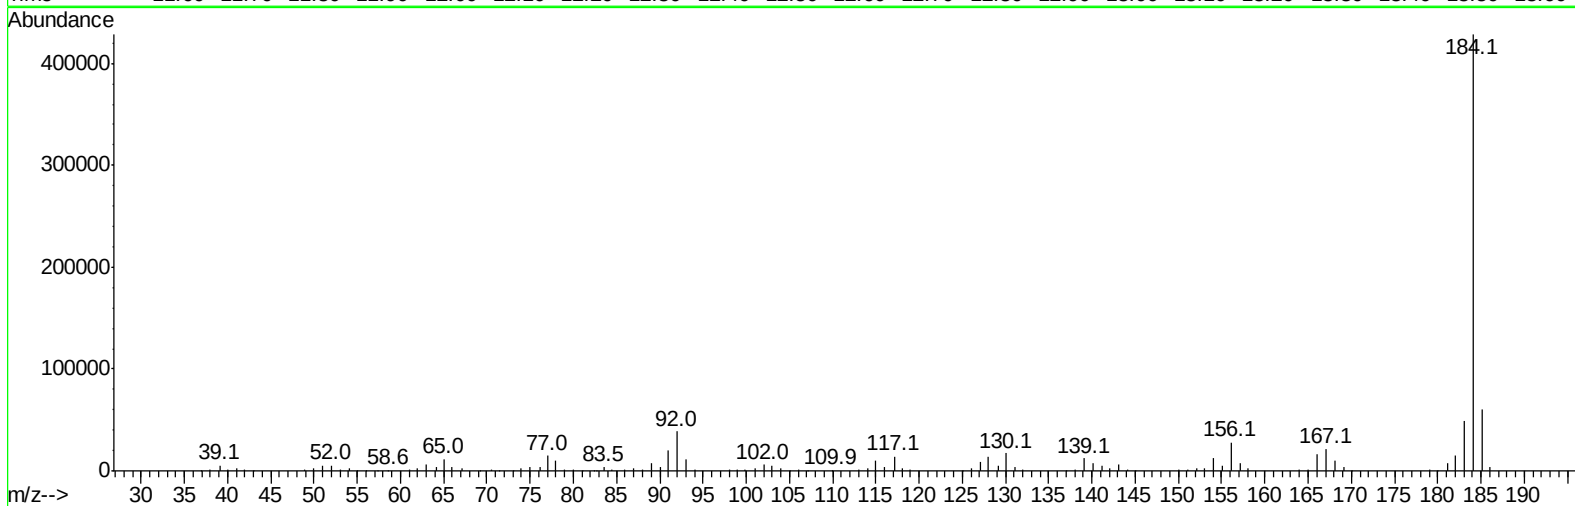


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF090517\
 Data File : BF098269.D
 Acq On : 5 Sep 2017 11:45
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 06 02:08:46 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 05 17:28:20 2017
 Response via : Initial Calibration

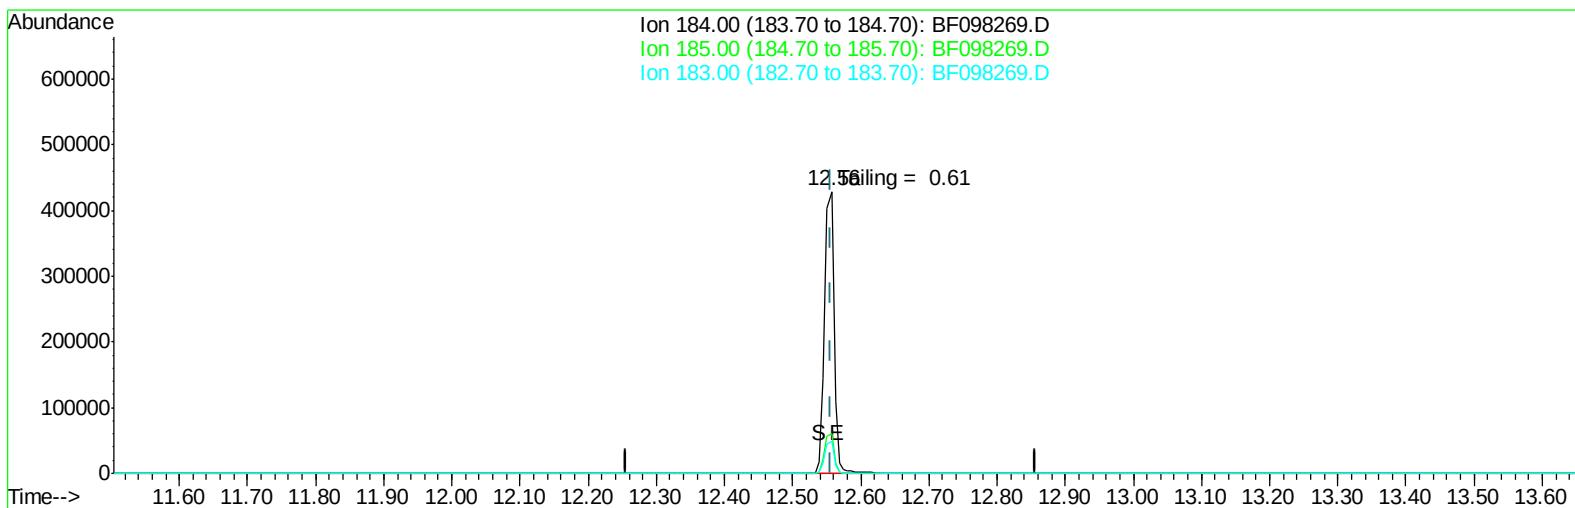

TIC: BF098269.D

(76) Benzidine



12.557min (+0.000) 0.00ng

response 404247

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.11#
183.00	12.20	11.34
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF090517\
Data File : BF098269.D
Acq On : 5 Sep 2017 11:45
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 06 02:08:46 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 05 17:28:20 2017
Response via : Initial Calibration

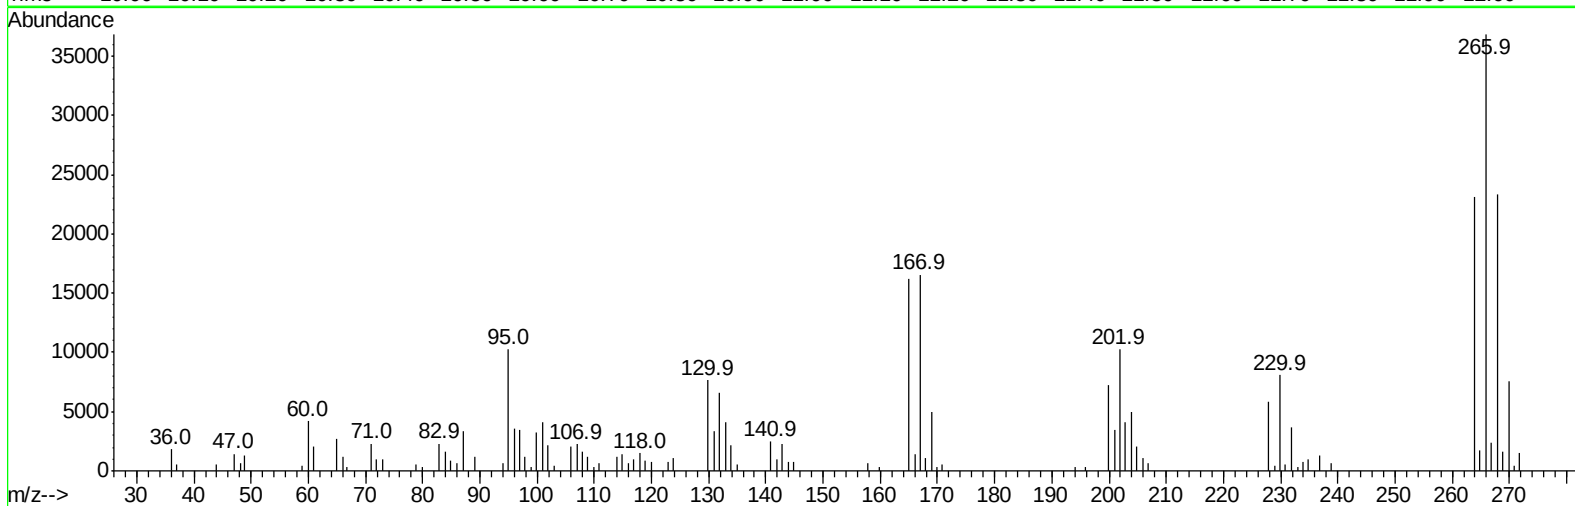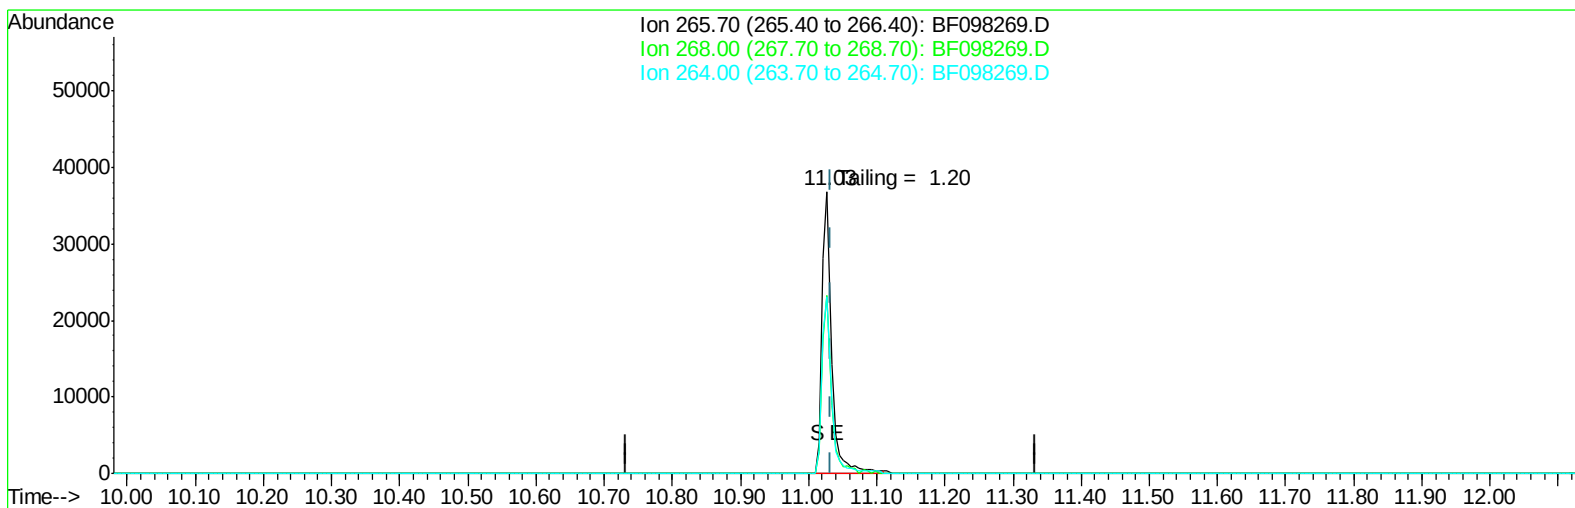

TIC: BF098269.D

(69) Pentachlorophenol (C)

11.027min (-0.006) 21998.54ng

response 35026

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.42
264.00	64.60	62.81
0.00	0.00	0.00