

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF090517\
 Data File : BF098272.D
 Acq On : 5 Sep 2017 15:04
 Operator : SJ/JU
 Sample : I5073-08
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-3-4-COMP

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.034	160	161	186	rBV4	45444	107032	3.85%	0.407%
2	4.893	473	477	490	rVB	166592	231863	8.34%	0.881%
3	5.310	543	548	551	rBV	2499352	2566147	92.34%	9.752%
4	6.346	719	724	727	rBV	2523215	2777118	99.93%	10.554%
5	6.475	741	746	749	rBV	2518735	2597774	93.47%	9.873%
6	6.698	781	784	788	rBV	770885	637435	22.94%	2.423%
7	6.857	807	811	814	rBV	2088346	1808751	65.08%	6.874%
8	7.269	876	881	884	rBV	1764573	1669002	60.05%	6.343%
9	7.987	998	1003	1006	rBV	883679	834486	30.03%	3.171%
10	9.063	1181	1186	1189	rBV	3044667	2779155	100.00%	10.562%
11	9.457	1249	1253	1256	rBV	368789	285492	10.27%	1.085%
12	9.734	1296	1300	1304	rBV	968382	867353	31.21%	3.296%
13	10.528	1430	1435	1438	rBV	1661111	1632444	58.74%	6.204%
14	10.645	1451	1455	1462	rVB2	38858	50316	1.81%	0.191%
15	11.216	1548	1552	1555	rBV	1008329	926986	33.35%	3.523%
16	11.239	1555	1556	1559	rVV	145225	87619	3.15%	0.333%
17	11.292	1560	1565	1569	rVB	37062	35965	1.29%	0.137%
18	11.828	1653	1656	1659	rBV	35872	38974	1.40%	0.148%
19	12.269	1727	1731	1734	rBV	22134	29593	1.06%	0.112%
20	12.427	1754	1758	1761	rBV	248368	212965	7.66%	0.809%
21	12.651	1791	1796	1800	rBV	233184	257991	9.28%	0.980%
22	12.804	1818	1822	1826	rVB	2540170	2613544	94.04%	9.933%
23	12.880	1829	1835	1838	rBV3	25886	43572	1.57%	0.166%
24	13.086	1866	1870	1873	rBV2	44807	51647	1.86%	0.196%
25	13.492	1936	1939	1943	rBV	48169	46831	1.69%	0.178%
26	13.598	1952	1957	1960	rBV3	30220	54920	1.98%	0.209%
27	13.704	1972	1975	1983	rVB3	246530	277621	9.99%	1.055%
28	13.851	1992	2000	2003	rBV2	819836	916985	33.00%	3.485%
29	13.874	2003	2004	2007	rVB	119489	71855	2.59%	0.273%
30	14.027	2027	2030	2034	rVB6	28698	34753	1.25%	0.132%
31	14.239	2064	2066	2069	rVB	37516	32507	1.17%	0.124%
32	14.274	2069	2072	2075	rBV3	22923	30177	1.09%	0.115%
33	14.339	2079	2083	2089	rVV4	85371	144471	5.20%	0.549%
34	14.863	2168	2172	2175	rBV	128794	190212	6.84%	0.723%

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF090517\
Data File : BF098272.D
Acq On : 5 Sep 2017 15:04
Operator : SJ/JU
Sample : I5073-08
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-3-4-COMP

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	14.963	2187	2189	2192	rVB3	32216	30202	1.09%	0.115%
36	15.145	2217	2220	2225	rVB	82365	106593	3.84%	0.405%
37	15.204	2226	2230	2236	rVB	106816	154458	5.56%	0.587%
38	15.263	2236	2240	2244	rBV	474712	574750	20.68%	2.184%
39	15.910	2346	2350	2358	rVB2	77150	146102	5.26%	0.555%
40	16.310	2414	2418	2424	rVB2	81339	137160	4.94%	0.521%
41	16.621	2468	2471	2476	rVB2	39236	59467	2.14%	0.226%
42	16.839	2504	2508	2513	rBV7	32545	63368	2.28%	0.241%
43	18.098	2717	2722	2733	rBV7	30212	97241	3.50%	0.370%


Sum of corrected areas: 26312897

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA_F\DATA\BF090517\
Data File : BF098272.D
Acq On : 5 Sep 2017 15:04
Operator : SJ/JU
Sample : I5073-08
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-3-4-COMP

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

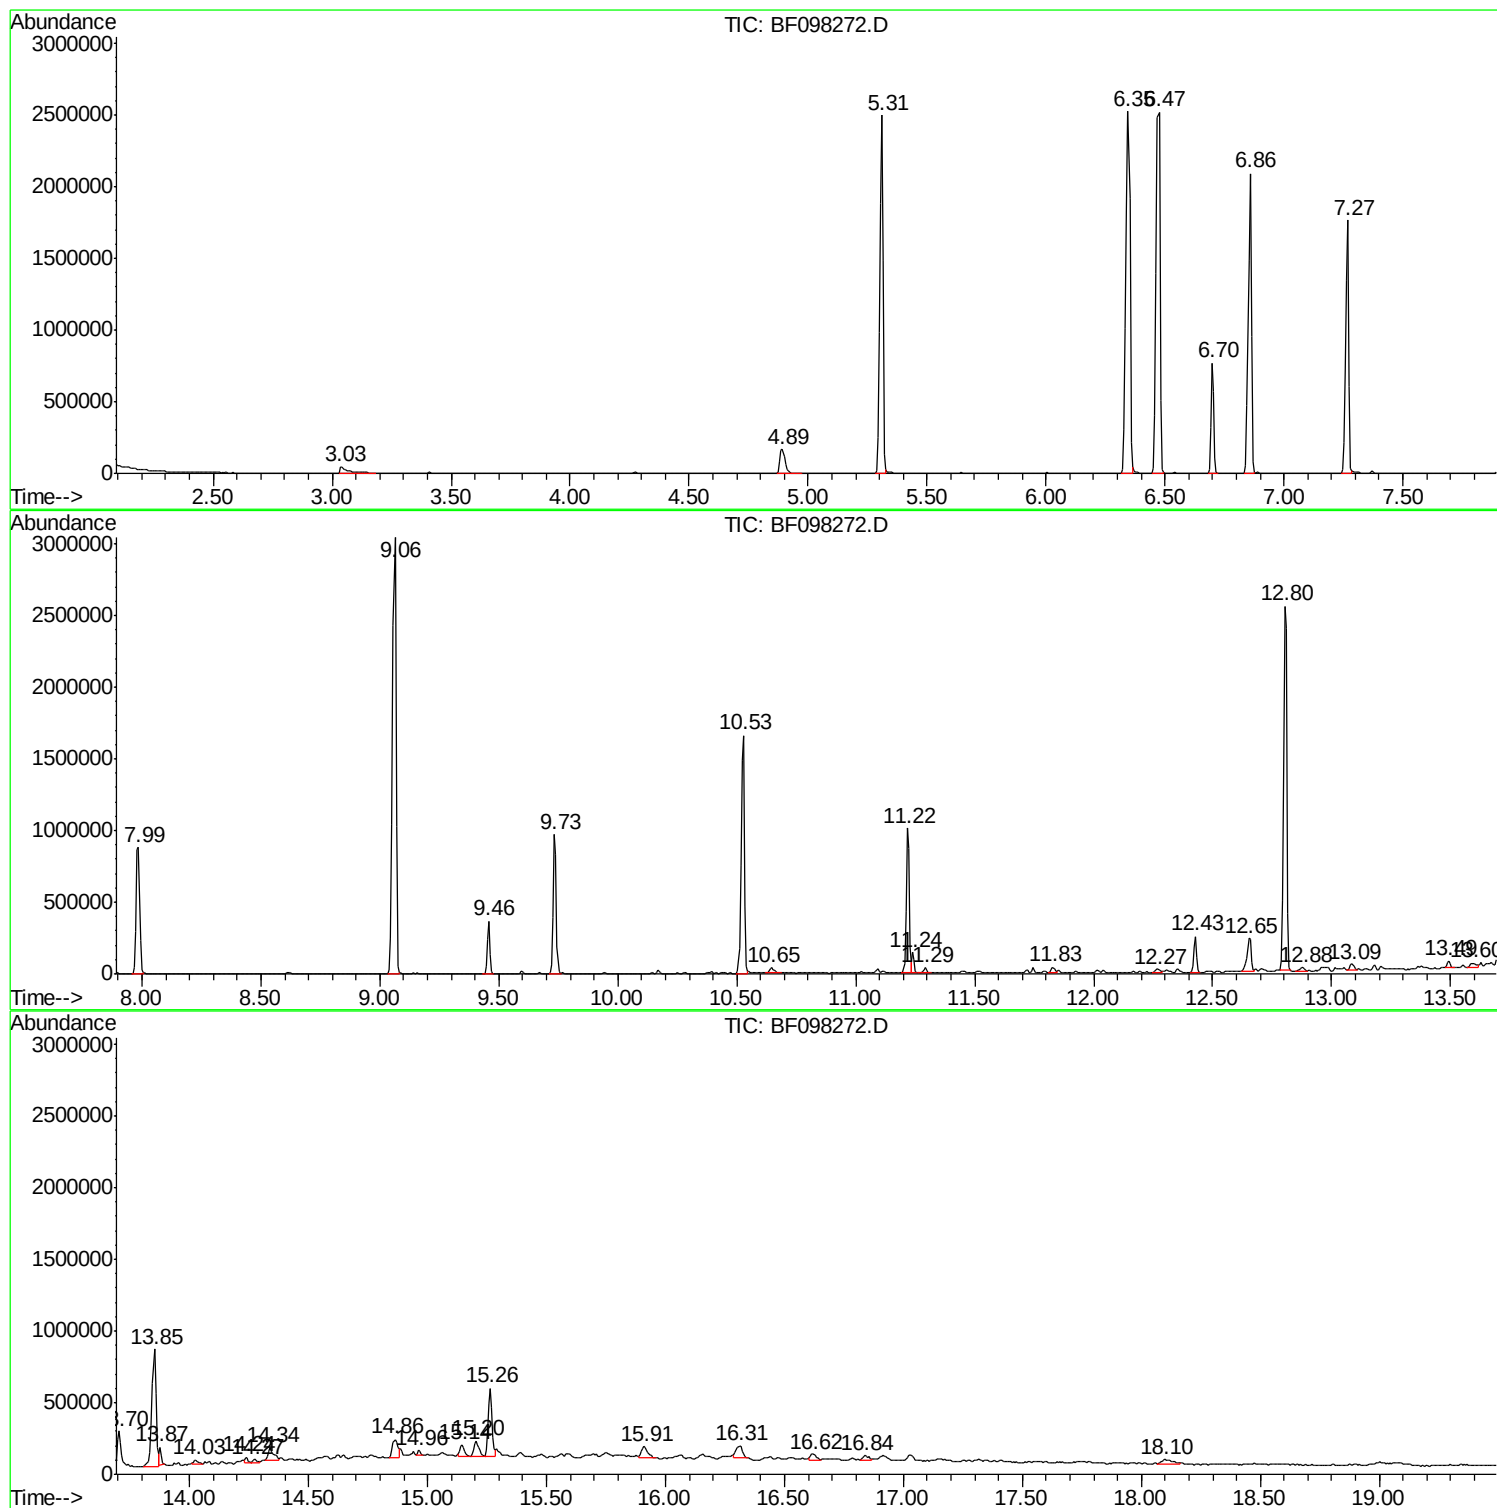

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF090517\
Data File : BF098272.D
Acq On : 5 Sep 2017 15:04
Operator : SJ/JU
Sample : I5073-08
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-3-4-COMP

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown3.03 Concentration Rank 9

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.03	3.36 ng	107032	1,4-Dichlorobenzene-d4	6.70

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	R-(-)-1,2-propanediol	76	C3H8O2	004254-14-2	43
2		(S)-(+)-1,2-Propanediol	76	C3H8O2	004254-15-3	43
3		2-Pentanol	88	C5H12O	006032-29-7	9
4		Propylene Glycol	76	C3H8O2	000057-55-6	9
5		2-Heptanol	116	C7H16O	000543-49-7	9

