


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF090517\
 Data File : BF098269.D
 Acq On : 5 Sep 2017 11:45
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 05 17:28:20 2017

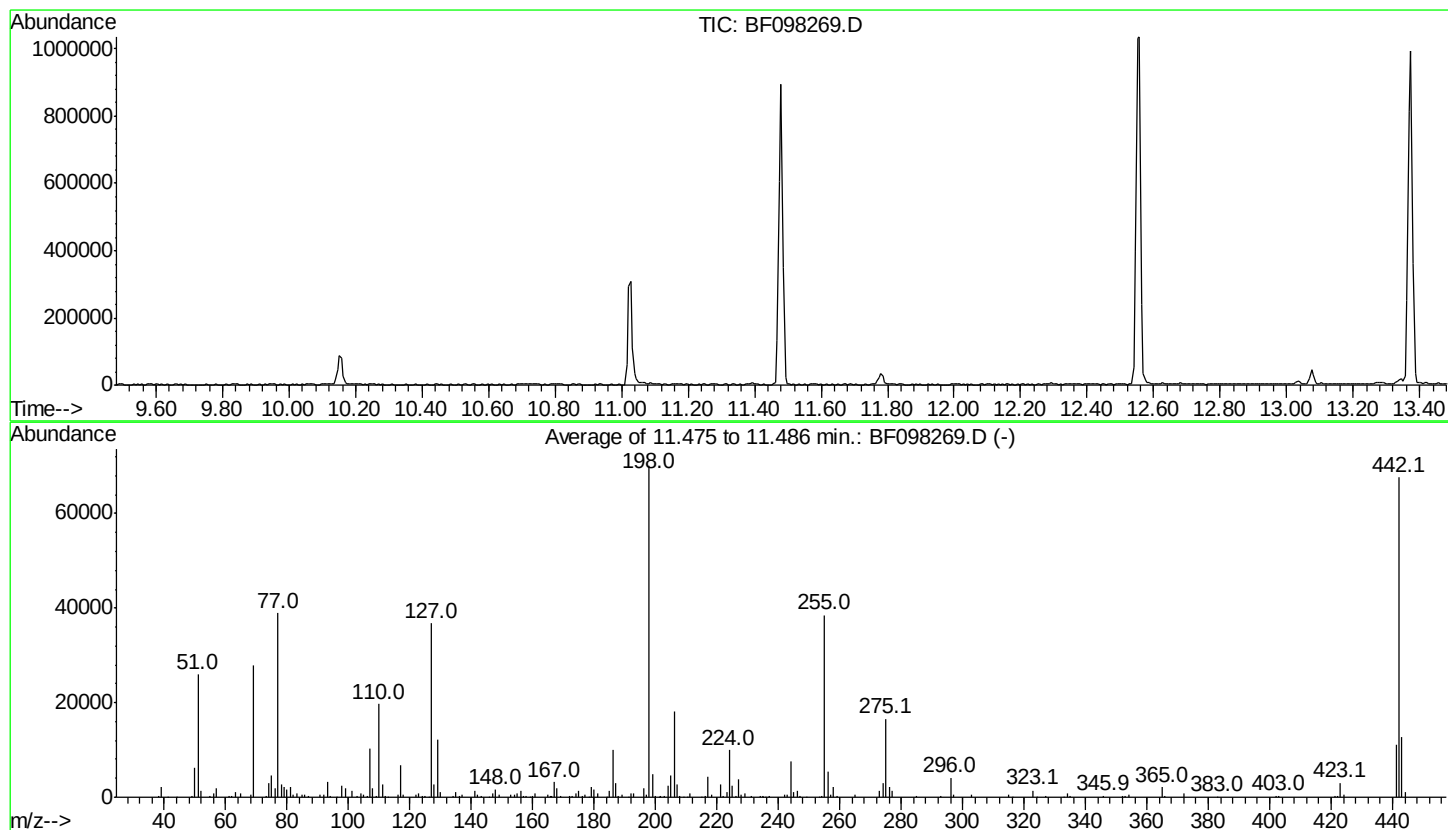

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	25919	PASS
68	69	0.00	2	1.9	540	PASS
69	198	0.00	100	39.9	27993	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.3	36718	PASS
197	198	0.00	2	0.7	481	PASS
198	198	100	100	100.0	70154	PASS
199	198	5	9	7.1	4963	PASS
275	198	10	60	23.6	16531	PASS
365	198	1	100	3.0	2081	PASS
441	442	0.01	24	16.3	11041	PASS
442	198	50	100	96.3	67592	PASS
443	442	15	24	18.9	12798	PASS