
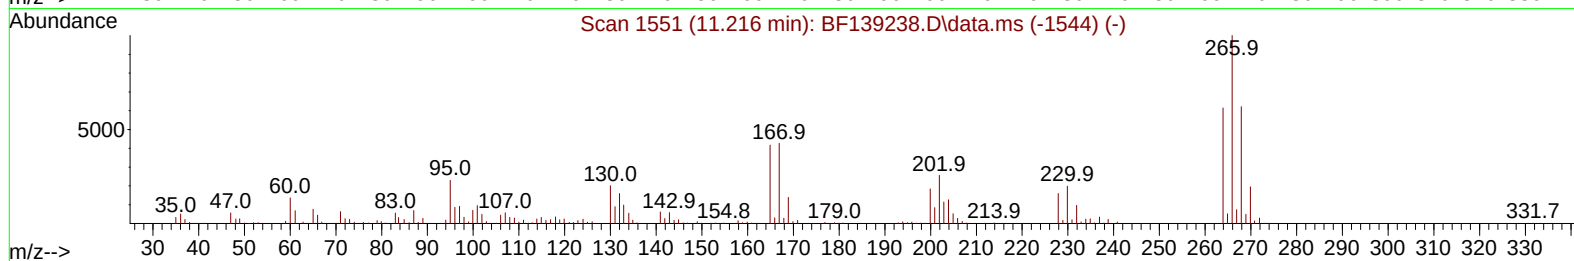
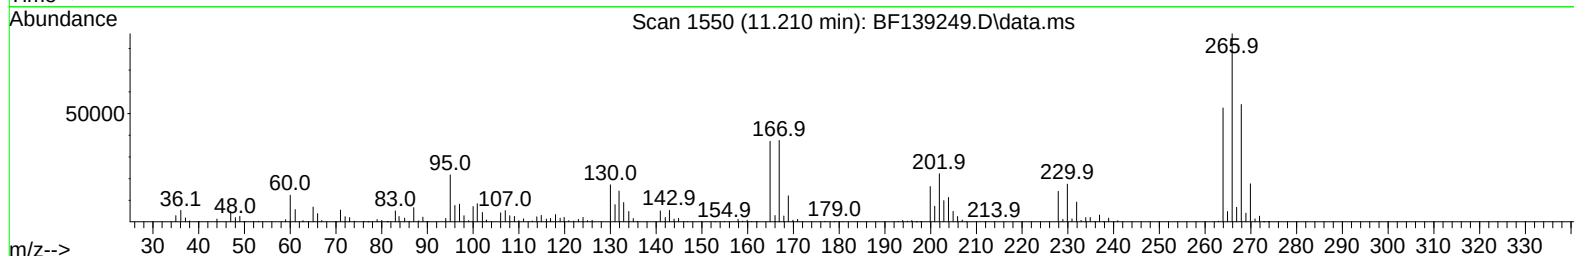


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090524\
Data File : BF139249.D
Acq On : 05 Sep 2024 08:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 05 10:58:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 16:11:43 2024
Response via : Initial Calibration

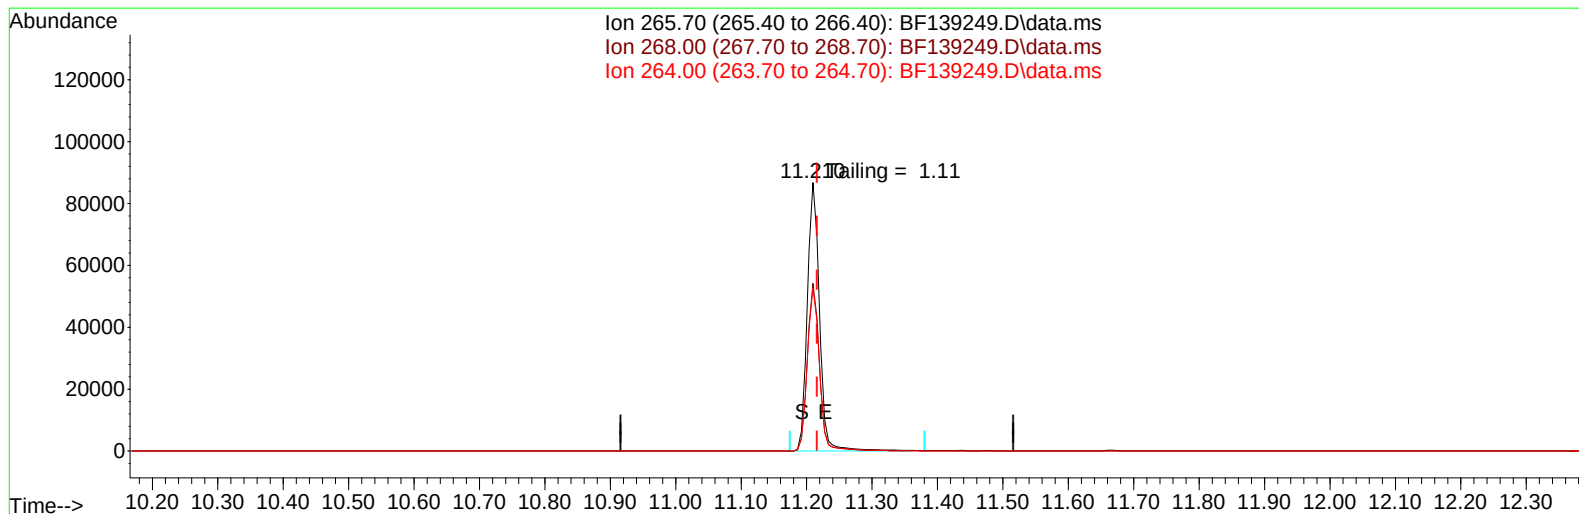

TIC: BF139249.D\data.ms

(70) Pentachlorophenol (C)




11.210min (-0.006) 33360.18 ng

response 112156

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.10	62.43
264.00	61.50	60.62
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090524\  
Data File : BF139249.D  
Acq On    : 05 Sep 2024  08:14  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Sep 05 10:58:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 16:11:43 2024
Response via : Initial Calibration

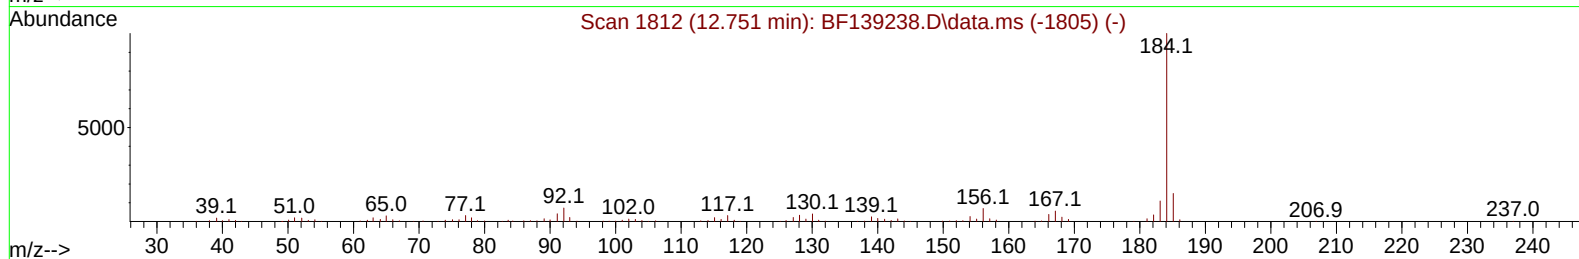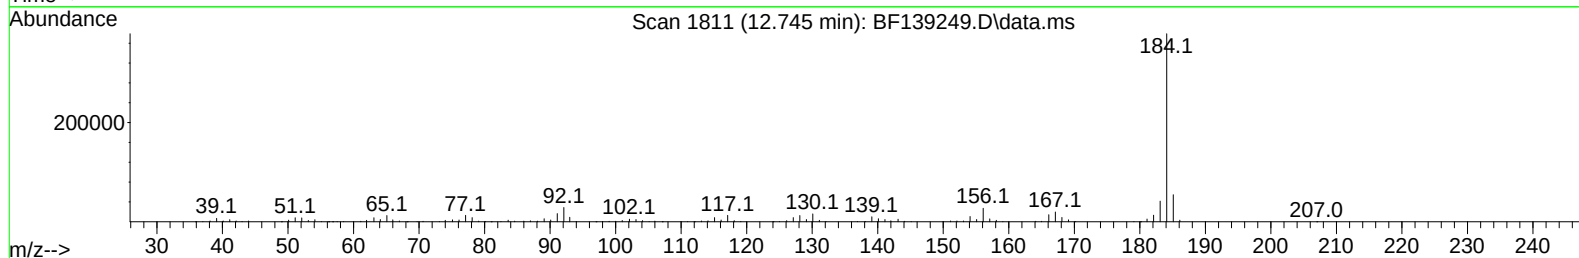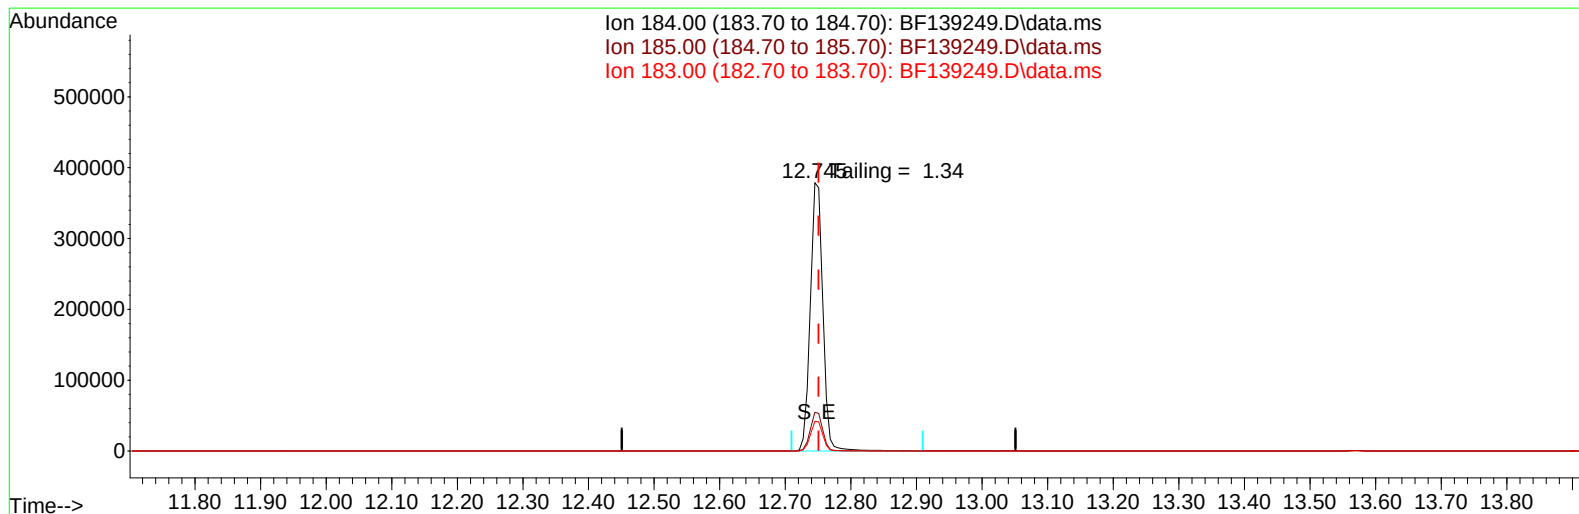

TIC: BF139249.D\data.ms

(77) Benzidine

12.745min (-0.006) 0.00 ng

response **506939**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.44
183.00	11.00	11.02
0.00	0.00	0.00