
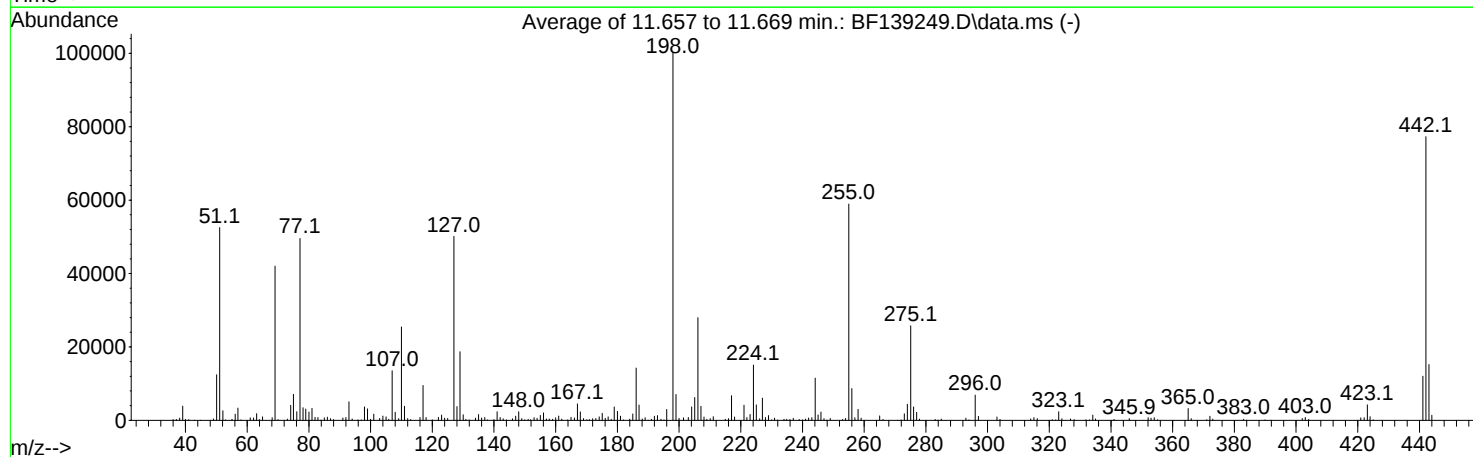


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090524\
Data File : BF139249.D
Acq On : 05 Sep 2024 08:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 04 16:11:43 2024

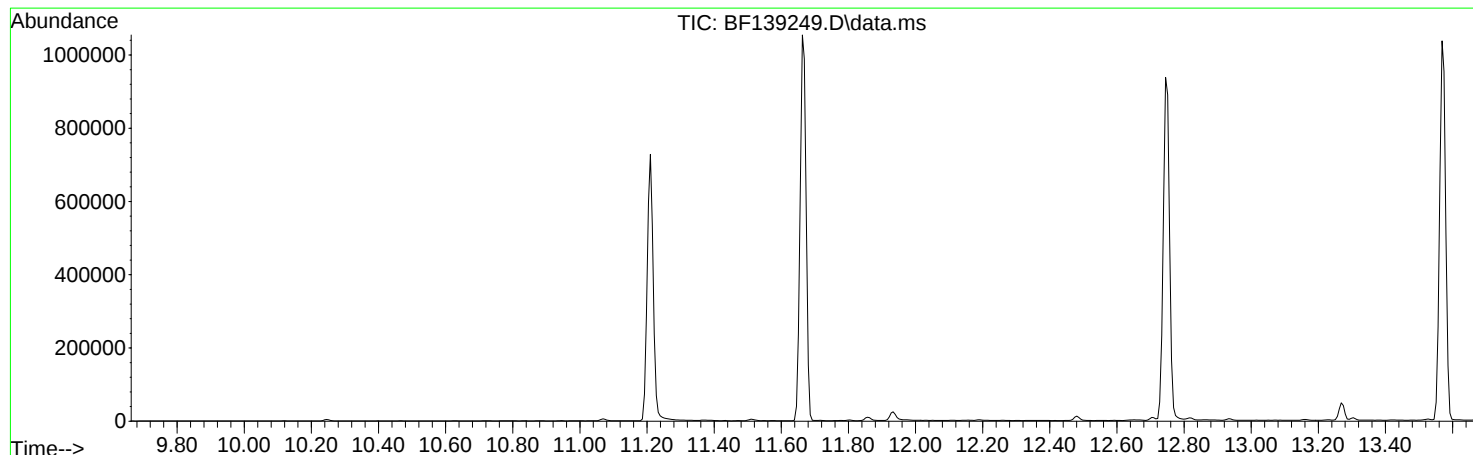




AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.4	52536	PASS
68	69	0.00	2	1.8	747	PASS
69	198	0.00	100	41.9	42003	PASS
70	69	0.00	2	0.5	231	PASS
127	198	10	80	50.0	50109	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	100216	PASS
199	198	5	9	7.1	7072	PASS
275	198	10	60	25.7	25752	PASS
365	198	1	100	3.2	3240	PASS
441	198	0.01	100	12.0	12054	PASS
442	442	50	100	100.0	77267	PASS
443	442	15	24	19.7	15196	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090524\
Data File : BF139249.D
Acq On : 05 Sep 2024 08:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 05 10:58:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 16:11:43 2024
Response via : Initial Calibration

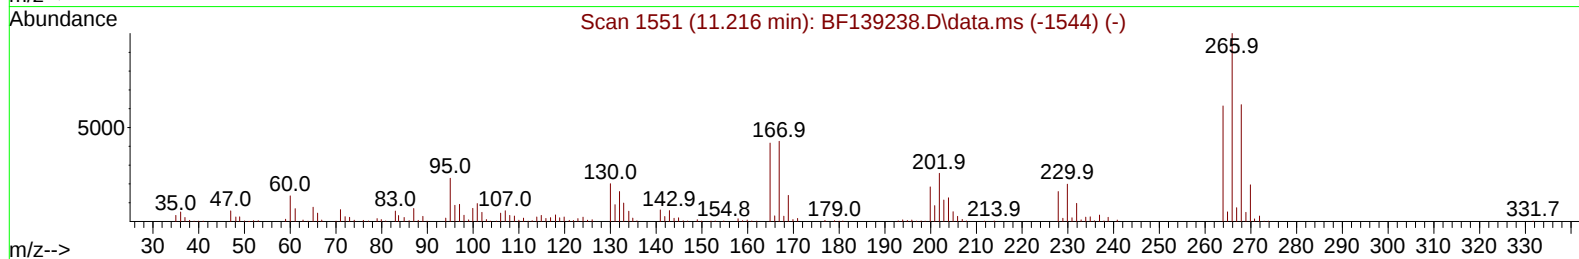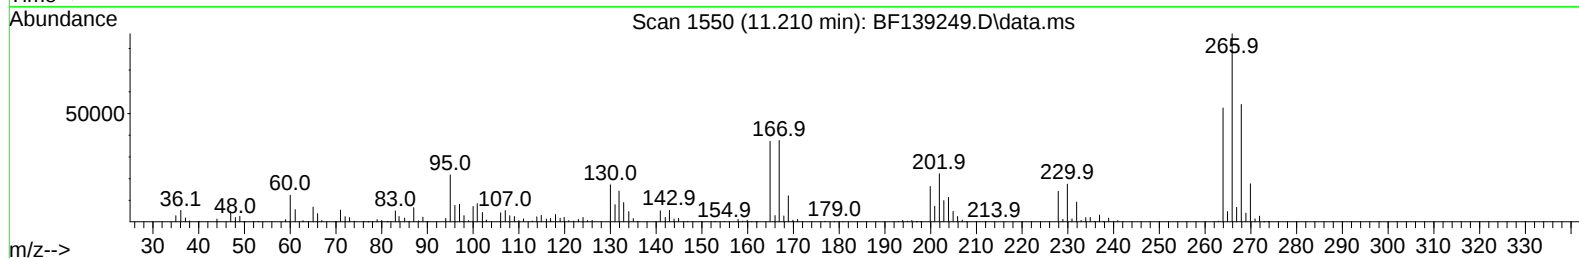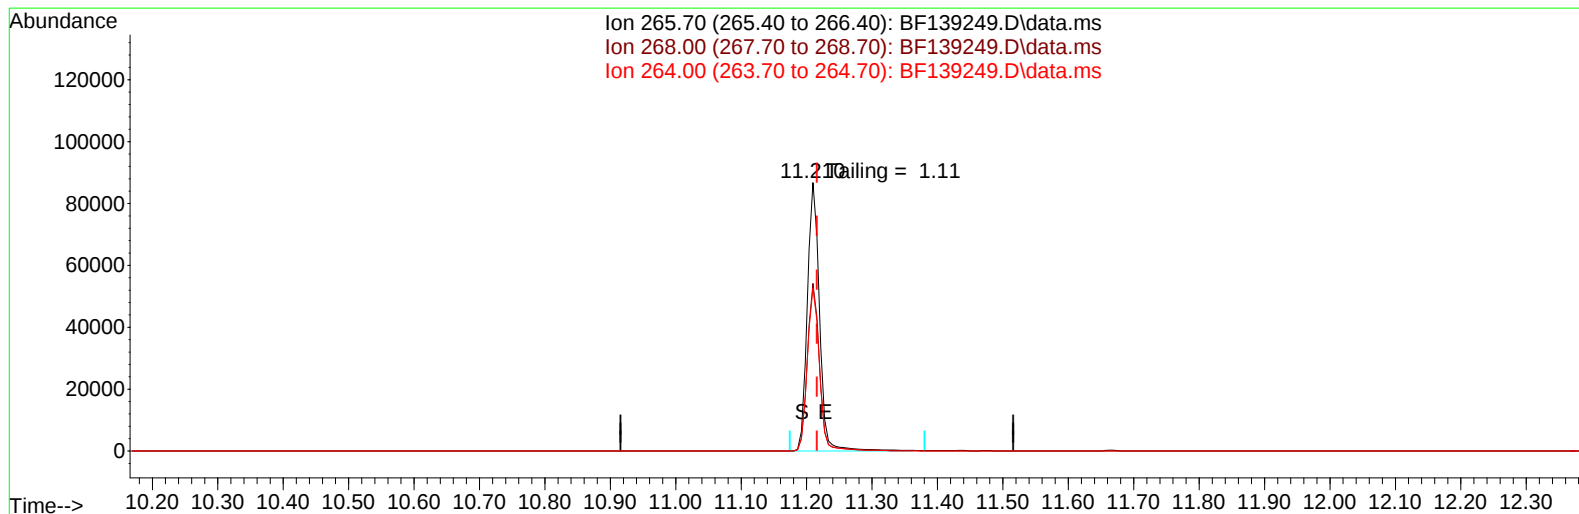

TIC: BF139249.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.006) 33360.18 ng




response 112156

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.10	62.43
264.00	61.50	60.62
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090524\  
Data File : BF139249.D  
Acq On    : 05 Sep 2024  08:14  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 05 10:58:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 16:11:43 2024
Response via : Initial Calibration

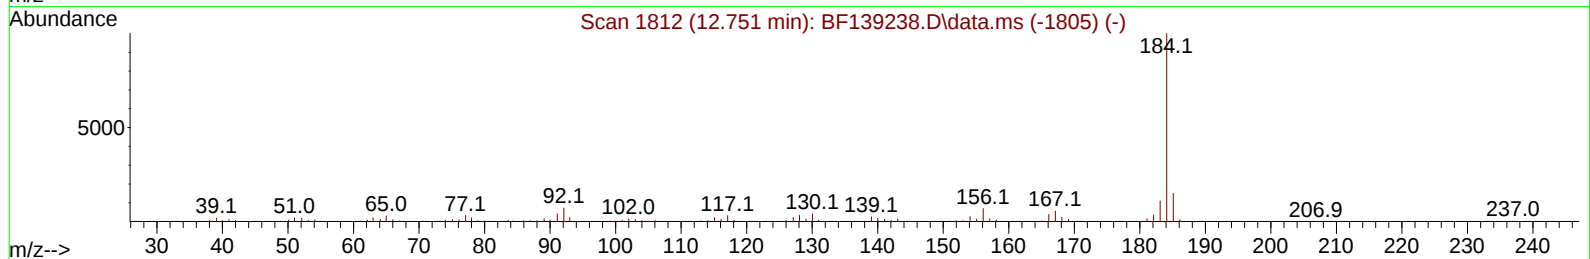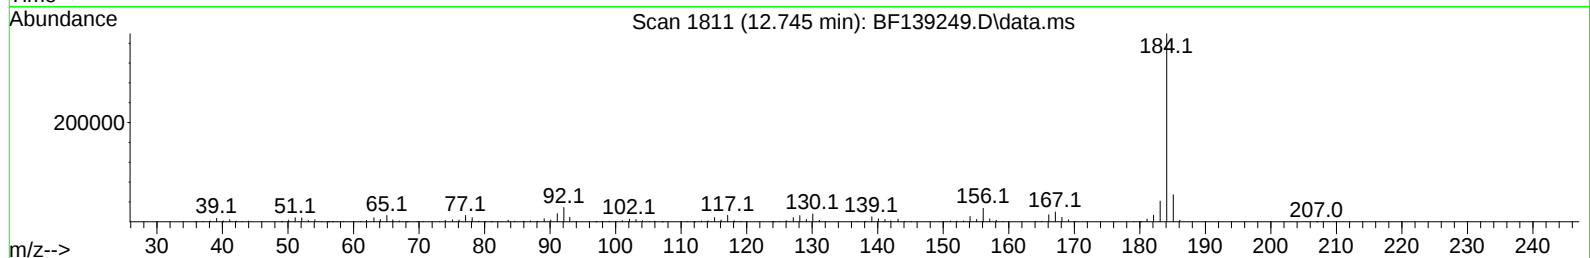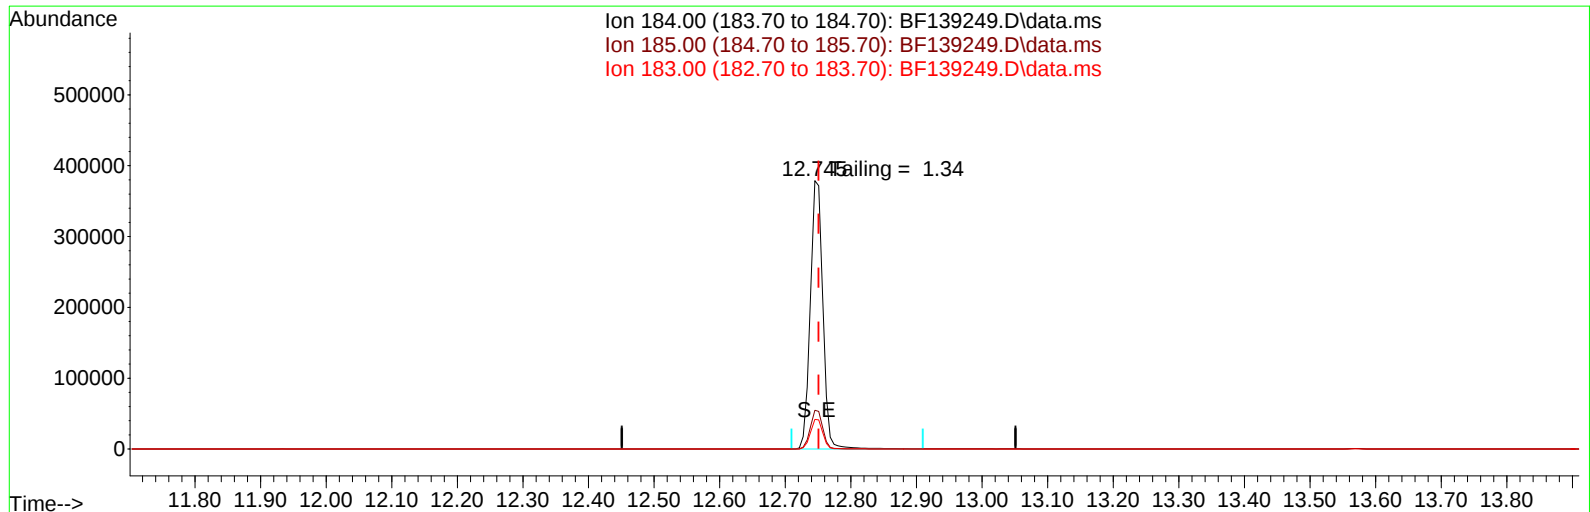

TIC: BF139249.D\data.ms

(77) Benzidine

12.745min (-0.006) 0.00 ng

response **506939**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.44
183.00	11.00	11.02
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/5/2024	BNA_F	<u>BF139249.D</u>
Compound Name	Response	Retention Time
DDT	249735	13.569
DDD	14015	13.269
DDE	1297	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15312	265047	5.78

Instrument :
BNA_F
ClientSampleId :
DFTPP