
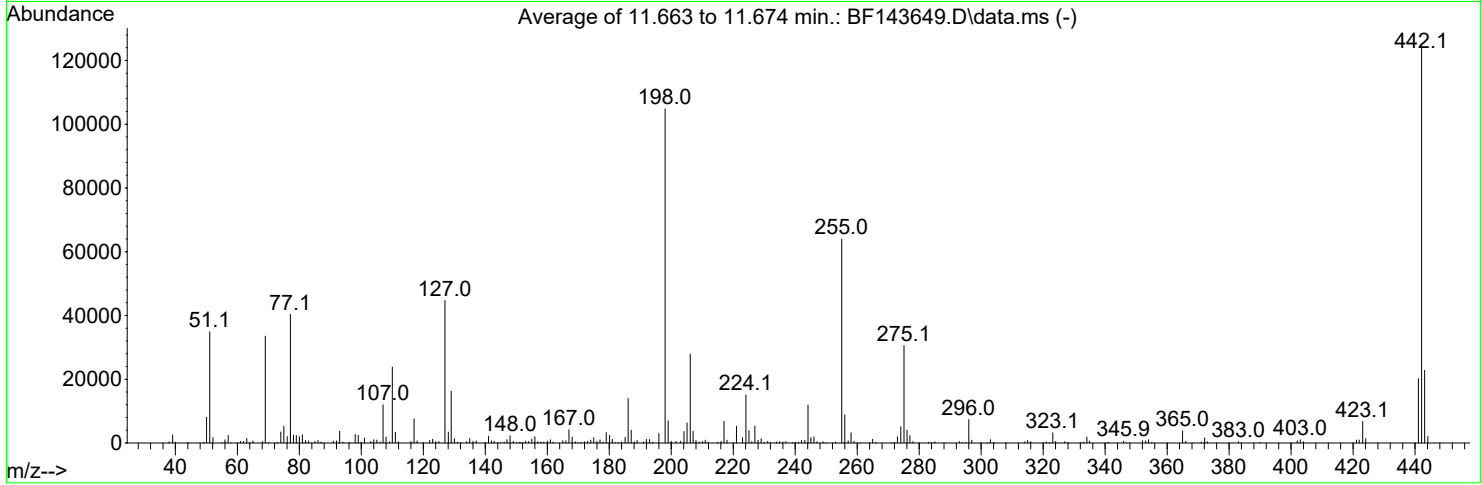


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF090525\  
 Data File : BF143649.D  
 Acq On : 05 Sep 2025 08:25  
 Operator : RC/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

**Instrument :**  
 BNA\_F  
**ClientSampleId :**  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF090325.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Sep 03 18:35:49 2025

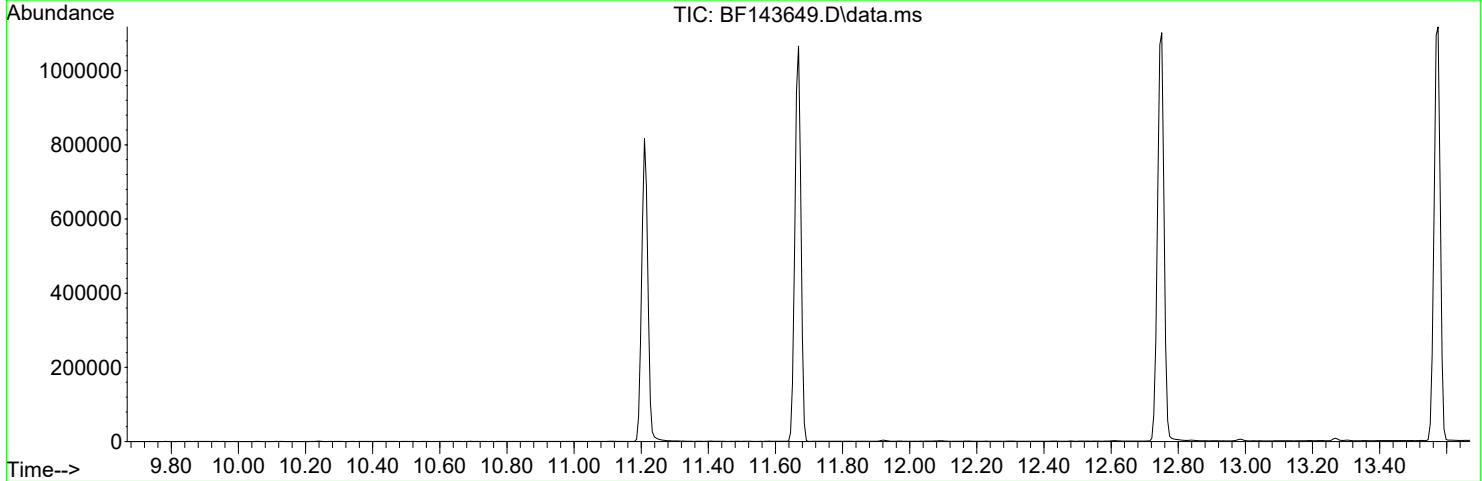

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.2	412	PASS
69	69	100	100	100.0	33517	PASS
70	69	0.00	2	0.3	111	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	104784	PASS
199	198	5	9	6.6	6967	PASS
365	198	1	100	3.6	3796	PASS
441	443	0.01	150	88.4	20160	PASS
442	442	100	100	100.0	123851	PASS
443	442	15	24	18.4	22803	PASS

**DDT Breakdown**




Date	Instrument Name	DFTPP Data File
9/5/2025	BNA_F	<u>BF143649.D</u>
Compound Name	Response	Retention Time
DDT	286563	13.574
DDD	3273	13.268
DDE	0	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3273	289836	1.13

Instrument :  
 BNA\_F  
 ClientSampled :  
 DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF090525\  
 Data File : BF143649.D  
 Acq On : 05 Sep 2025 08:25  
 Operator : RC/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

**Instrument :**  
 BNA\_F  
**ClientSampleId :**  
 DFTPP

Quant Time: Sep 05 12:03:17 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF090325.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Sep 03 18:35:49 2025  
 Response via : Initial Calibration

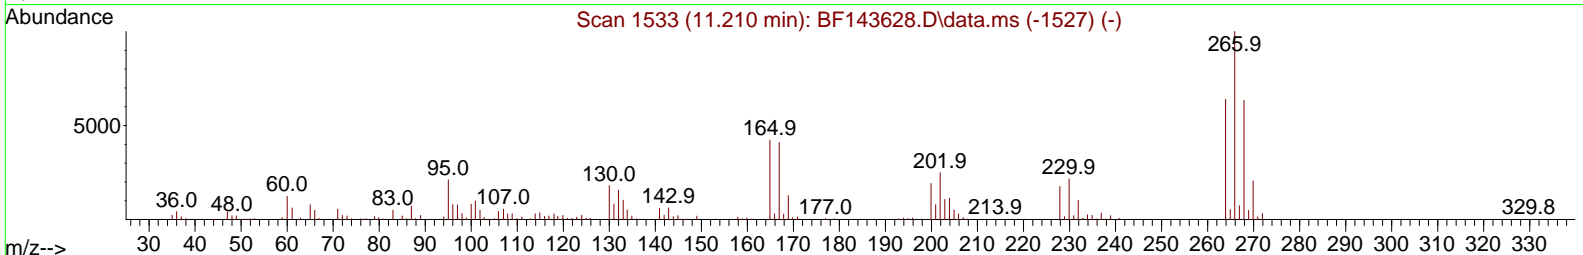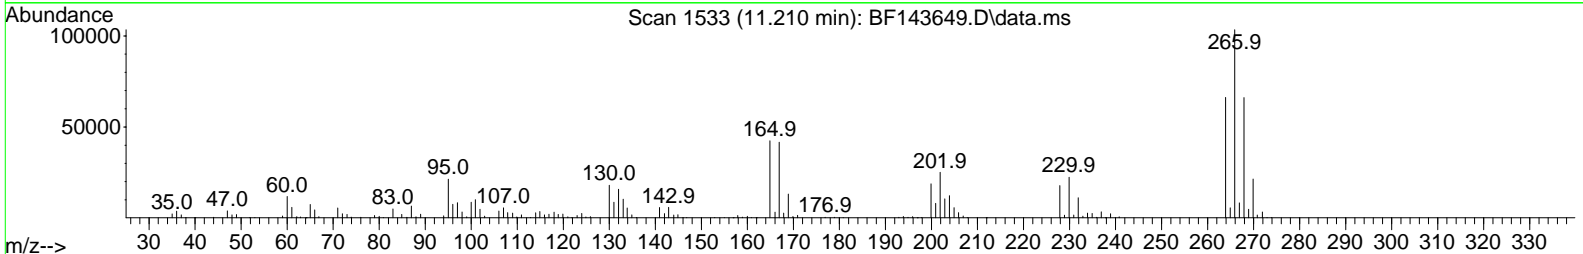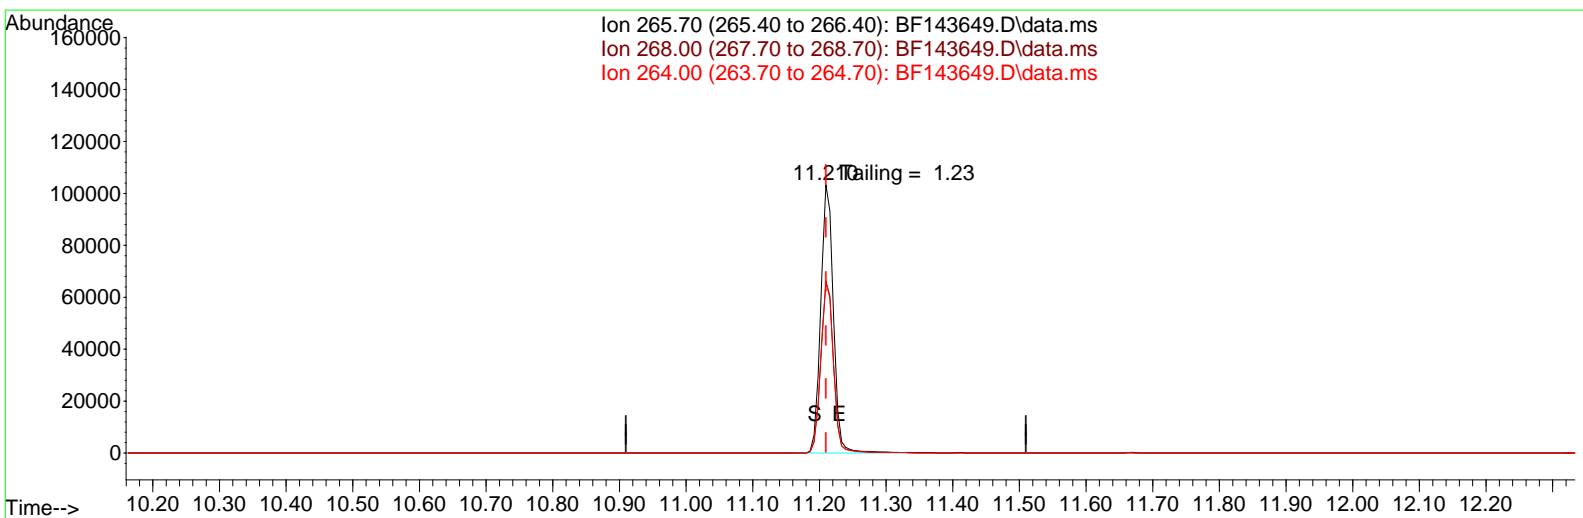

TIC: BF143649.D\data.ms

(70) Pentachlorophenol (C)




11.210min (-0.000) 131147.90 ng

response	136420
Ion	Exp% Act%
265.70	100.00 100.00
268.00	63.30 63.94
264.00	64.00 64.05
0.00	0.00 0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF090525\  
 Data File : BF143649.D  
 Acq On : 05 Sep 2025 08:25  
 Operator : RC/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Quant Time: Sep 05 12:03:17 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF090325.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Sep 03 18:35:49 2025  
 Response via : Initial Calibration

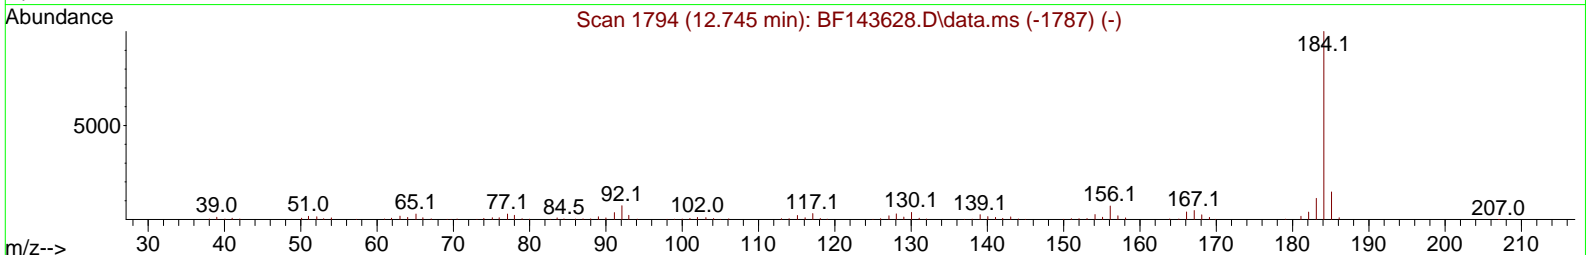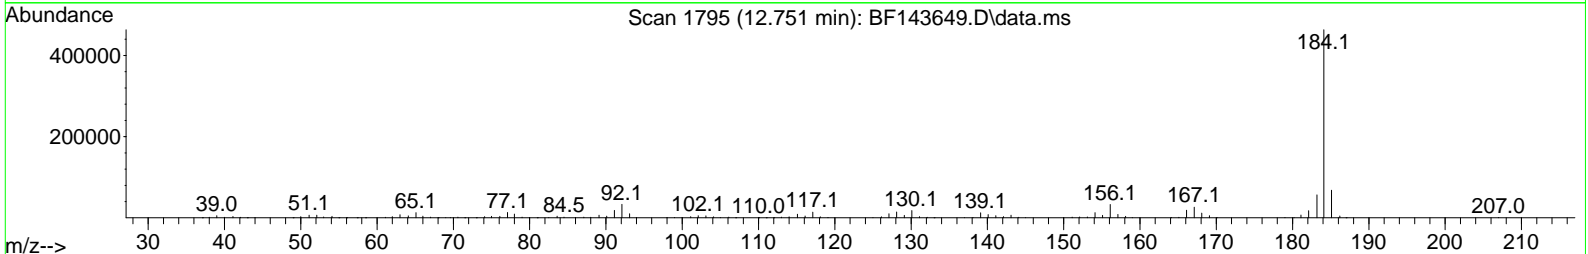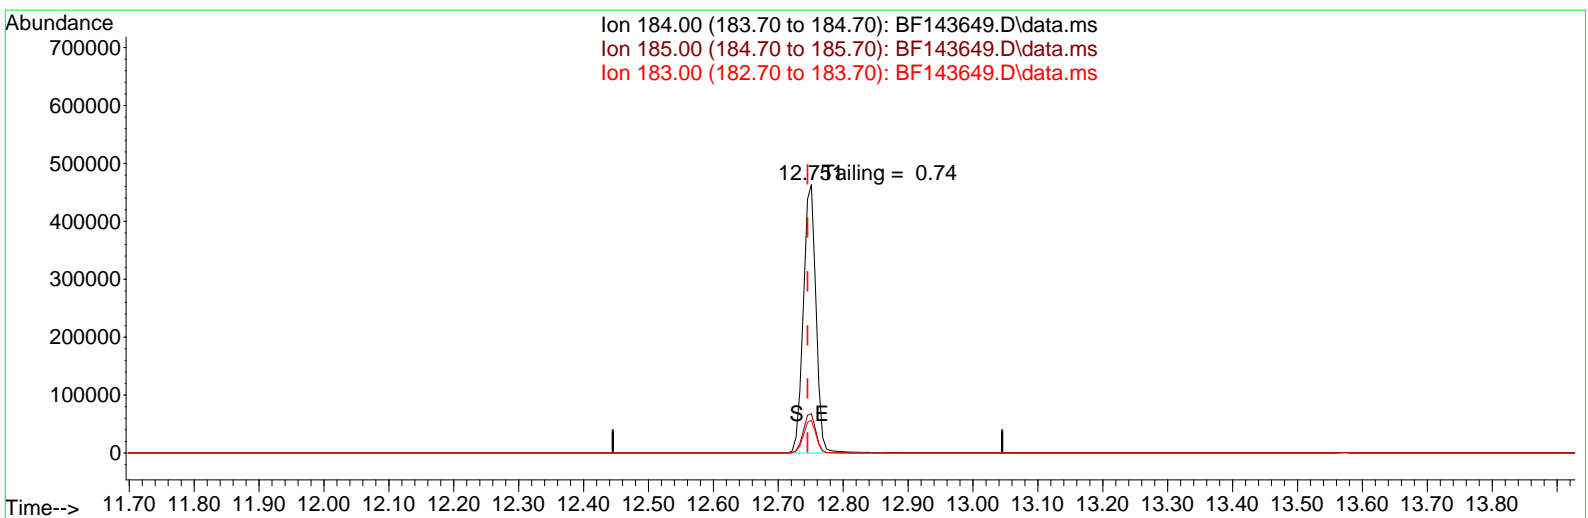

TIC: BF143649.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 34283.21 ng

response 633765

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.68
183.00	11.30	12.17
0.00	0.00	0.00