
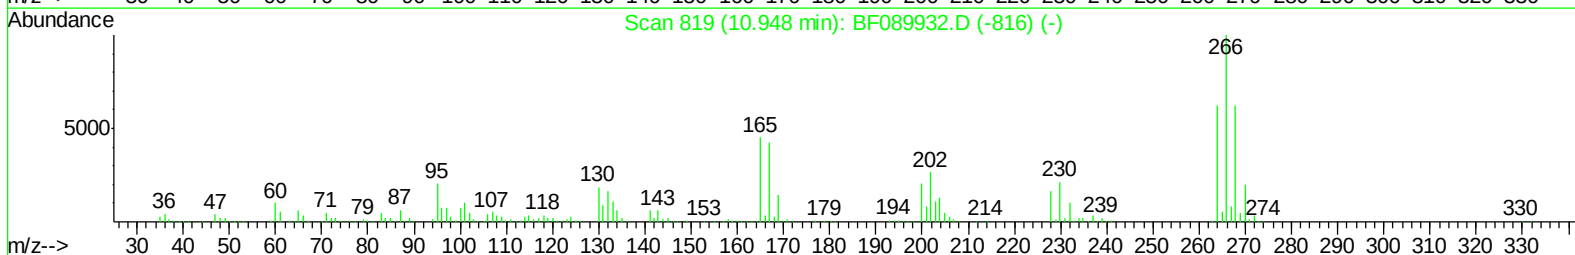
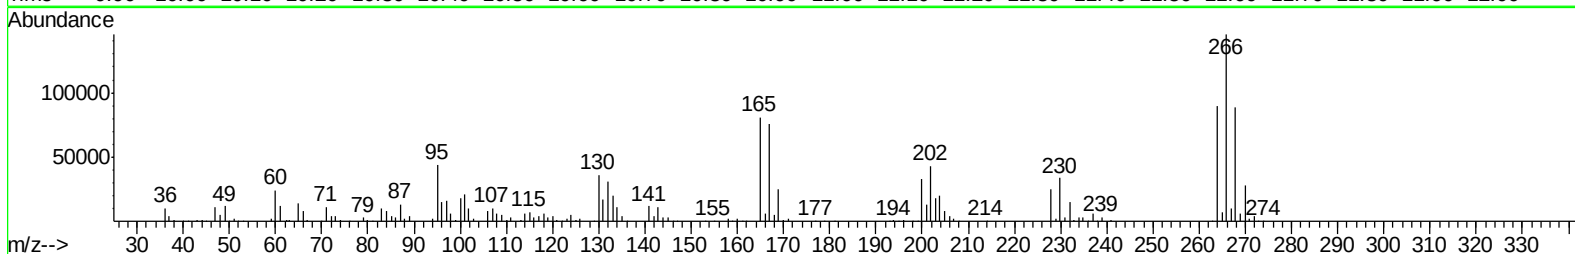


Data Path : Z:\HPCHEM1\BNA_F\Data\BF090616\
Data File : BF089989.D
Acq On : 6 Sep 2016 13:58
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 07 07:39:21 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 02 13:29:08 2016
Response via : Initial Calibration

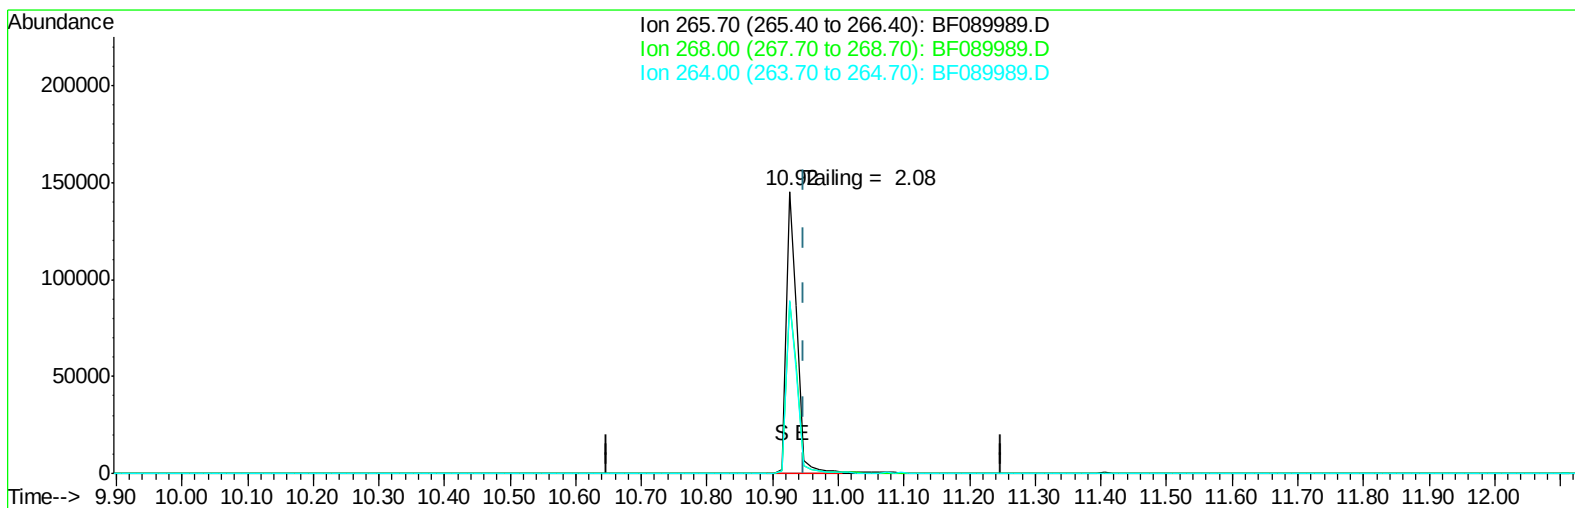

TIC: BF089989.D

(69) Pentachlorophenol (C)




10.925min (-0.023) 33936.29ng

response 173418

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	60.97
264.00	63.20	61.43
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF090616\
 Data File : BF089989.D
 Acq On : 6 Sep 2016 13:58
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 07 07:39:21 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF083116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 02 13:29:08 2016
 Response via : Initial Calibration

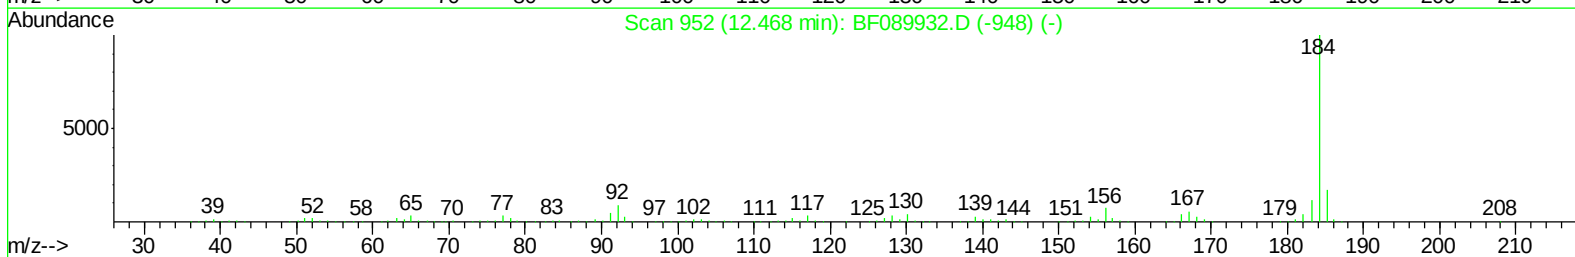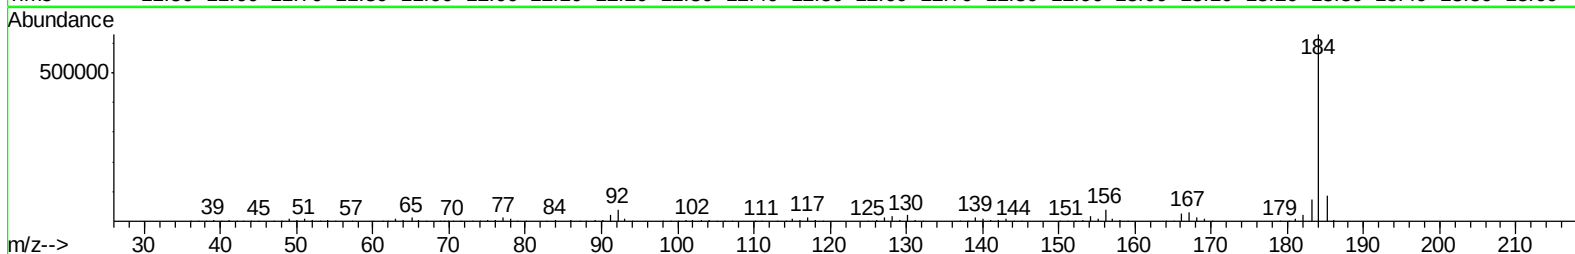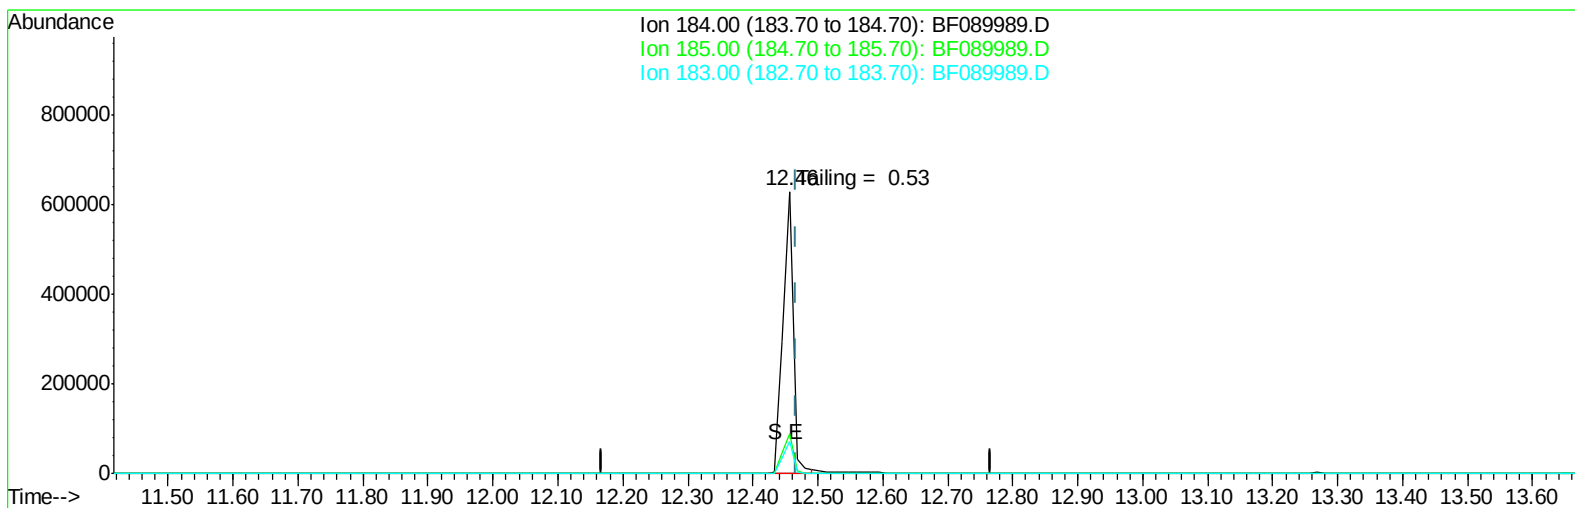

TIC: BF089989.D

(76) Benzidine

12.457min (-0.011) 26093.41ng

response 688984

Ion	Exp%	Act%
184.00	100	100
185.00	17.30	14.09
183.00	12.00	11.47
0.00	0.00	0.00