

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF090617\
 Data File : BF098285.D
 Acq On : 6 Sep 2017 21:06
 Operator : SJ/JU
 Sample : I5093-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 AU-06-090117-A

Quant Time: Sep 07 05:56:37 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 05 17:28:20 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.70	152	106897	20.00	ng	0.00
21) Naphthalene-d8	7.98	136	382342	20.00	ng	0.00
38) Acenaphthene-d10	9.73	164	142465	20.00	ng	-0.01
63) Phenanthrene-d10	11.21	188	239887	20.00	ng	-0.01
75) Chrysene-d12	13.85	240	253365	20.00	ng	-0.01
86) Perylene-d12	15.26	264	178279	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.30	112	535898	76.25	ng	0.00
7) Phenol-d6	6.34	99	707767	74.12	ng	-0.01
23) Nitrobenzene-d5	7.26	82	413862	58.80	ng	-0.01
41) 2,4,6-Tribromophenol	10.52	330	90799	73.46	ng	-0.01
44) 2-Fluorobiphenyl	9.06	172	580284	59.84	ng	-0.01
78) Terphenyl-d14	12.80	244	438829	36.12	ng	0.00
Target Compounds						Qvalue
49) Dimethylphthalate	9.45	163	23494	2.256	ng	# 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF090617\
Data File : BF098285.D
Acq On : 6 Sep 2017 21:06
Operator : SJ/JU
Sample : I5093-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
AU-06-090117-A

Quant Time: Sep 07 05:56:37 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 05 17:28:20 2017
Response via : Initial Calibration

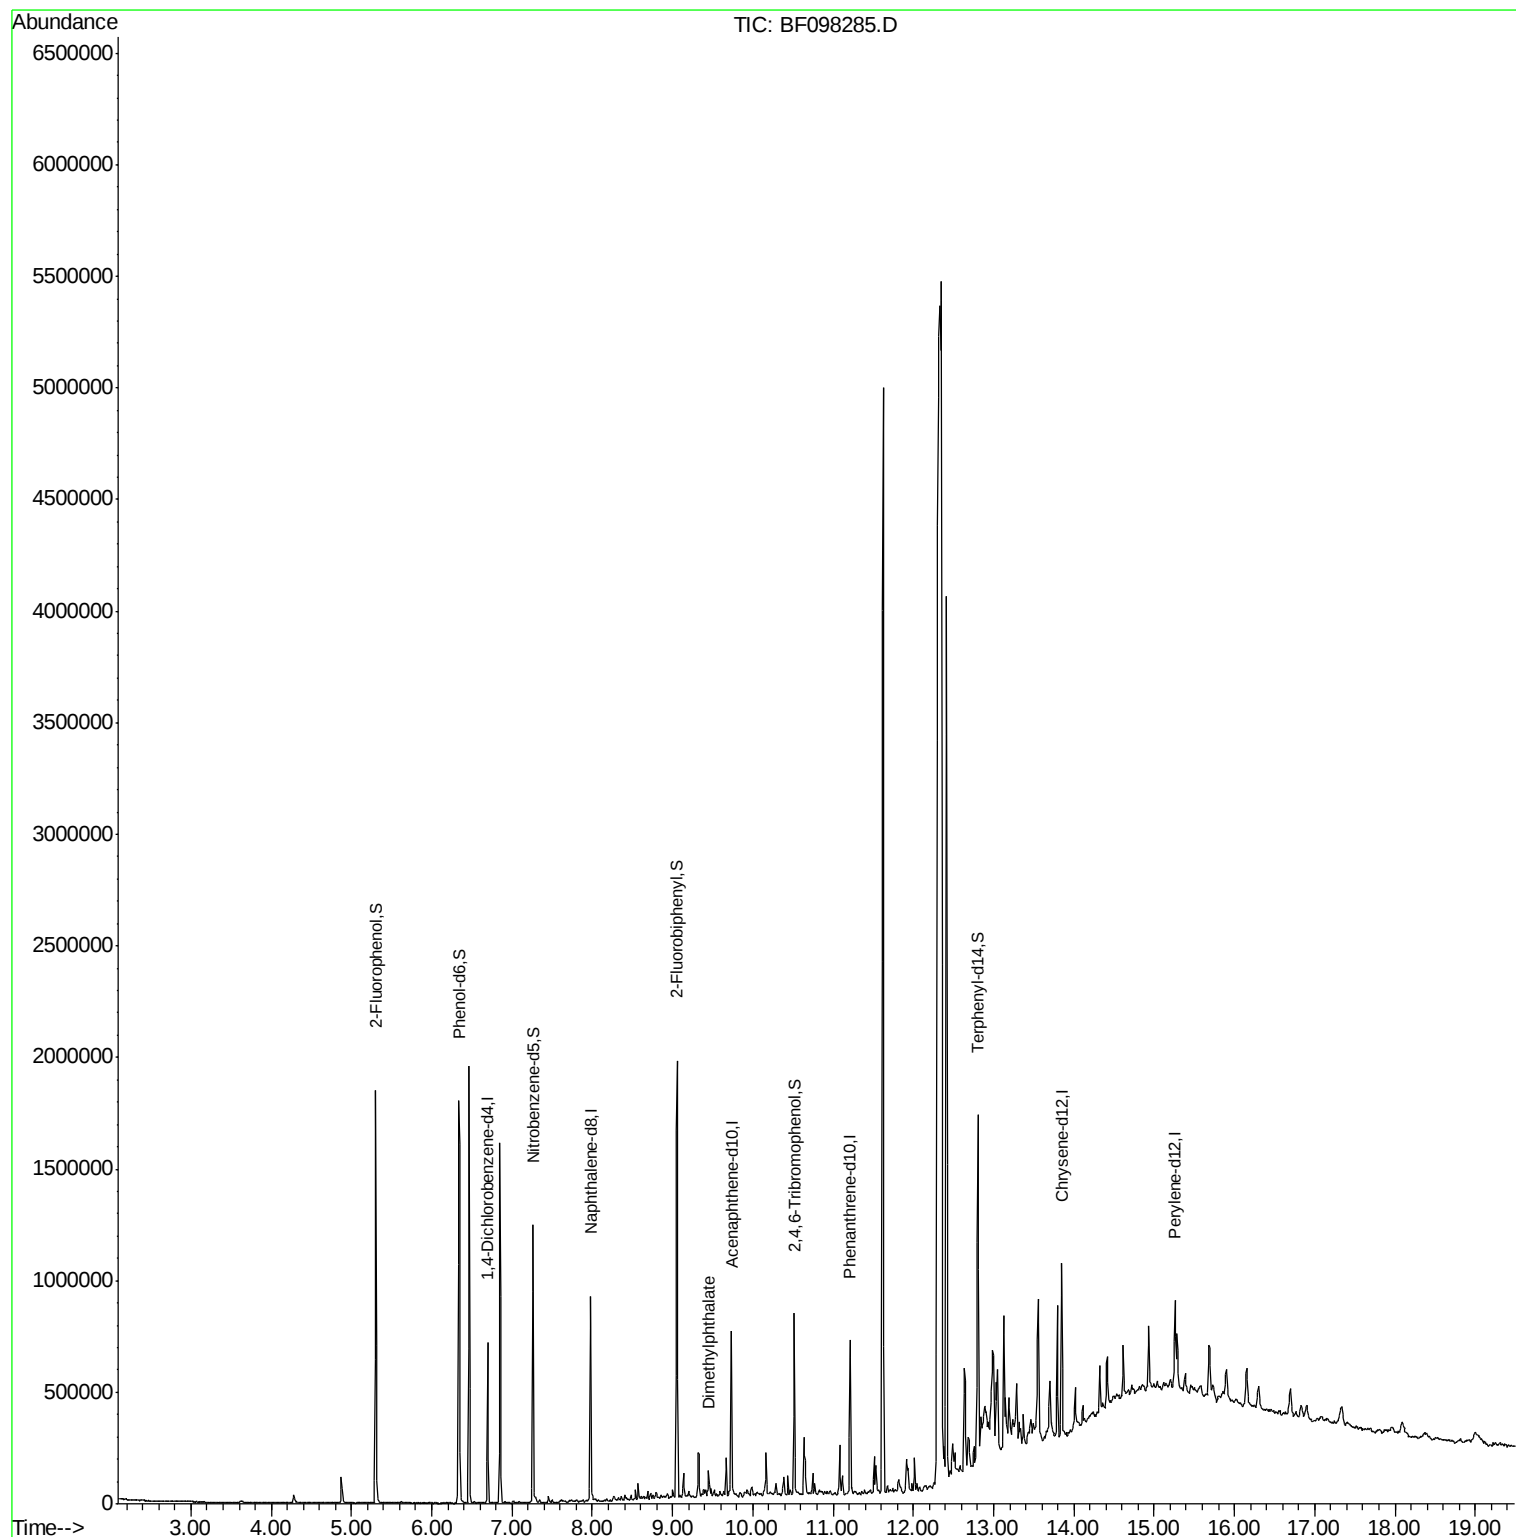




#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.70 min Scan# 784
 Delta R.T. -0.01 min
 Lab File: BF098285.D
 Acq: 6 Sep 2017 21:06

Instrument :
 BNA_F
 ClientSampleId :
 AU-06-090117-A

Tot Ion:152 Resp: 106897
 Ion Ratio Lower Upper
 152 100
 150 158.4 126.2 189.2
 115 61.4 52.2 78.2

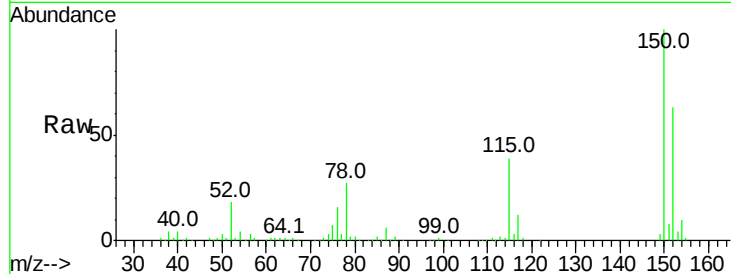


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

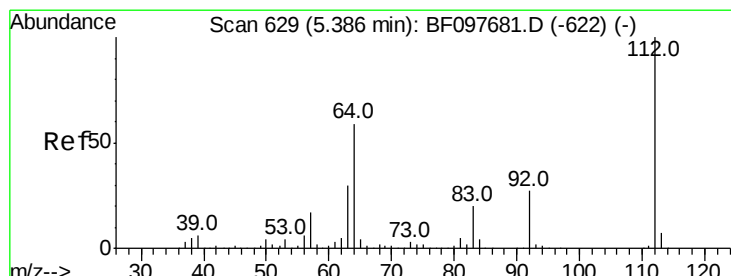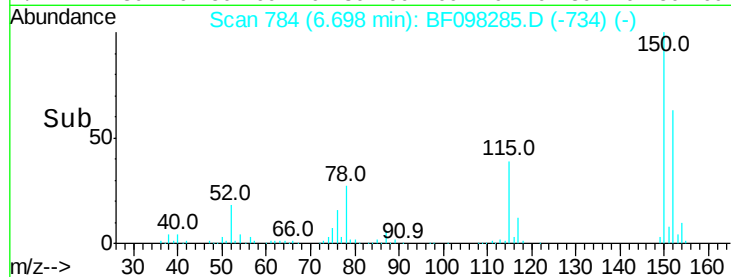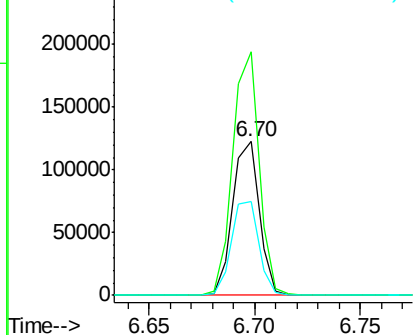



#5


2-Fluorophenol
 Concen: 76.255 ng
 RT: 5.30 min Scan# 547
 Delta R.T. 0.00 min
 Lab File: BF098285.D
 Acq: 6 Sep 2017 21:06

Tgt Ion:112 Resp: 535898
 Ion Ratio Lower Upper
 112 100
 64 57.1 46.0 69.0
 63 28.2 23.4 35.0

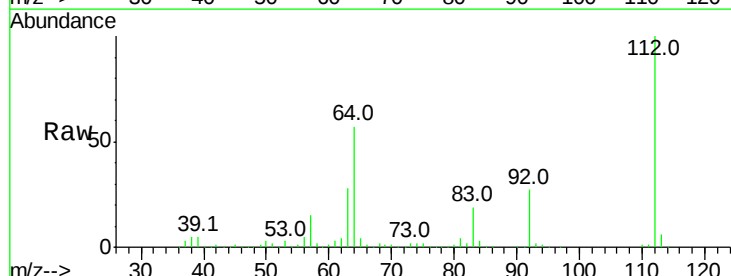

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

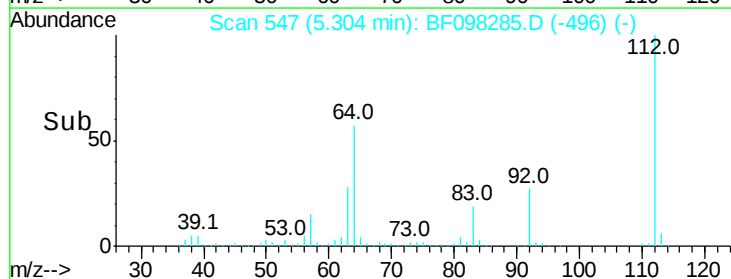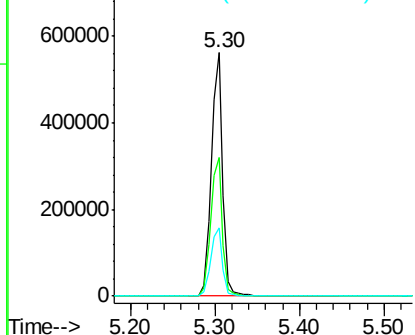

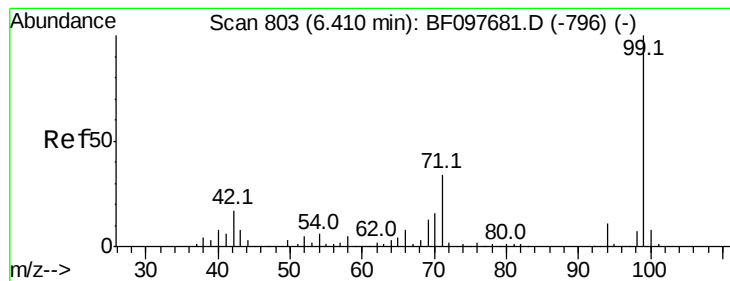

#7

Phenol-d6

Concen: 74.122 ng

RT: 6.34 min Scan# 723

Delta R.T. -0.01 min

Lab File: BF098285.D

Acq: 6 Sep 2017 21:06

Instrument :

BNA_F

ClientSampleId :

AU-06-090117-A


Tot Ion: 99 Resp: 707767

Ion Ratio Lower Upper

99 100

42 14.4 13.5 20.3

71 32.3 24.5 36.7

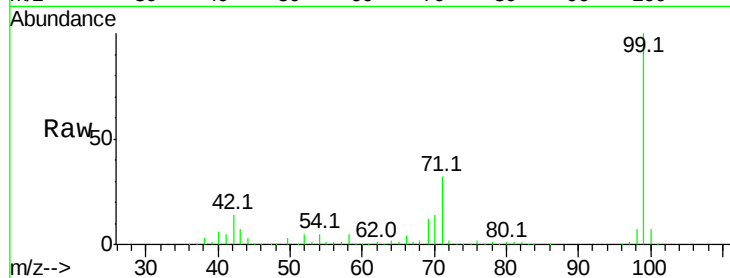

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

6.34

800000



600000

400000

200000

0

Time-->

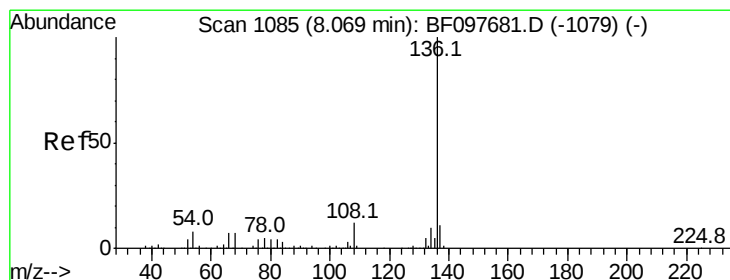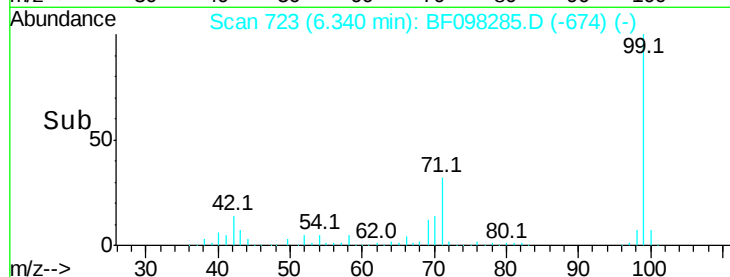

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.98 min Scan# 1002

Delta R.T. -0.01 min

Lab File: BF098285.D

Acq: 6 Sep 2017 21:06

Tgt Ion: 136 Resp: 382342


Ion Ratio Lower Upper

136 100

137 10.9 8.5 12.7

54 7.4 4.9 7.3#

68 7.3 4.1 6.1#

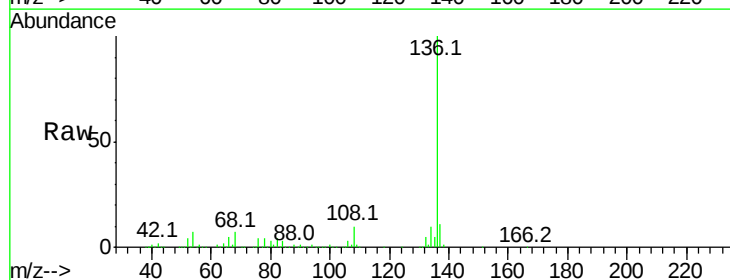

Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

7.98


600000

400000

200000

0

Time-->




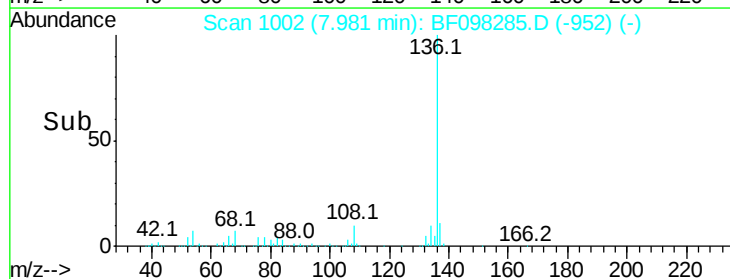




#23
 Nitrobenzene-d5
 Concen: 58.803 ng
 RT: 7.26 min Scan# 880
 Delta R.T. -0.01 min
 Lab File: BF098285.D
 Acq: 6 Sep 2017 21:06




Instrument :
 BNA_F
 ClientSampleId :
 AU-06-090117-A

Tot Ion: 82 Resp: 413862
 Ion Ratio Lower Upper
 82 100
 128 39.5 34.0 51.0
 54 38.4 42.2 63.2#

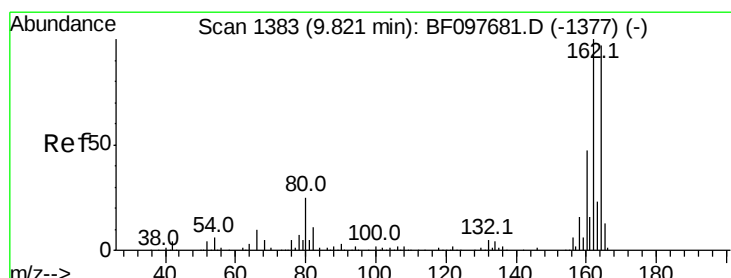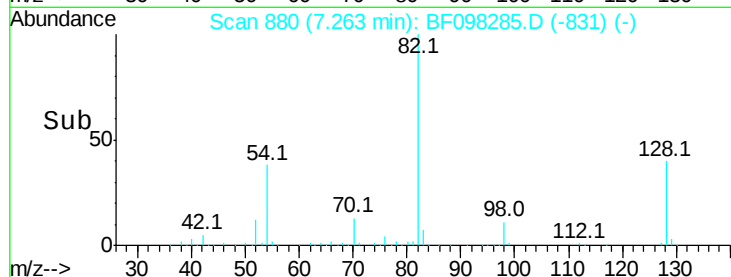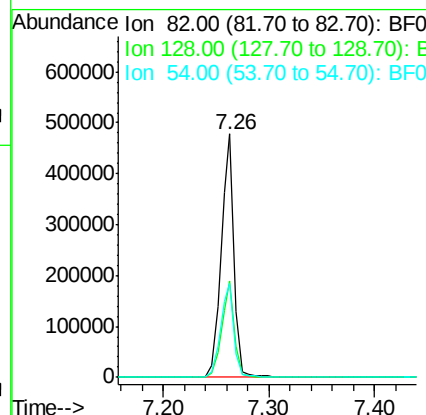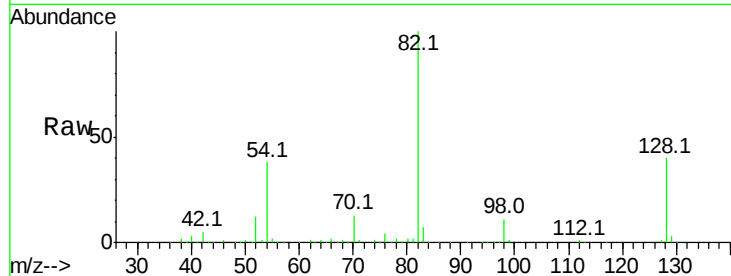

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.73 min Scan# 1299
 Delta R.T. -0.01 min
 Lab File: BF098285.D
 Acq: 6 Sep 2017 21:06

Tgt Ion:164 Resp: 142465
 Ion Ratio Lower Upper
 164 100
 162 101.9 82.6 123.8
 160 46.4 36.2 54.2

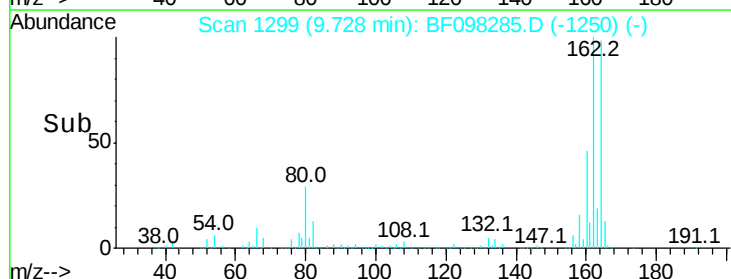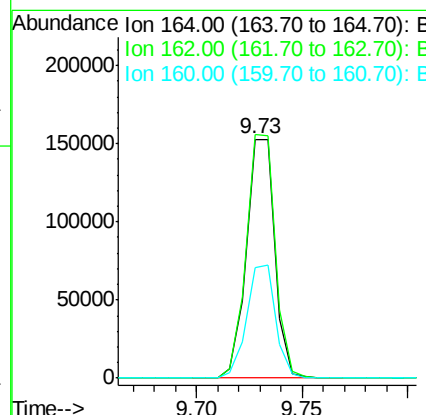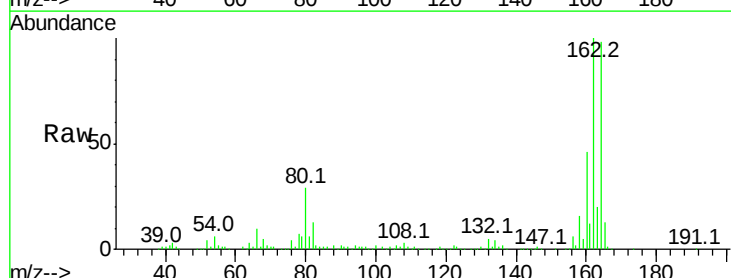







#41
 2,4,6-Tribromophenol
 Concen: 73.455 ng
 RT: 10.52 min Scan# 1434
 Delta R.T. -0.01 min
 Lab File: BF098285.D
 Acq: 6 Sep 2017 21:06

Instrument :
 BNA_F
 ClientSampleId :
 AU-06-090117-A

Tot Ion	Ratio	Lower	Upper
330	100		
332	94.9	76.6	115.0
141	36.7	31.4	47.2

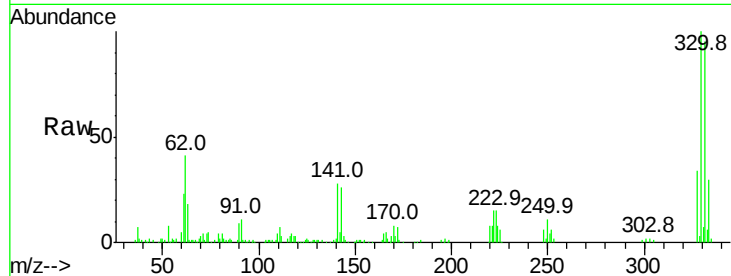


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

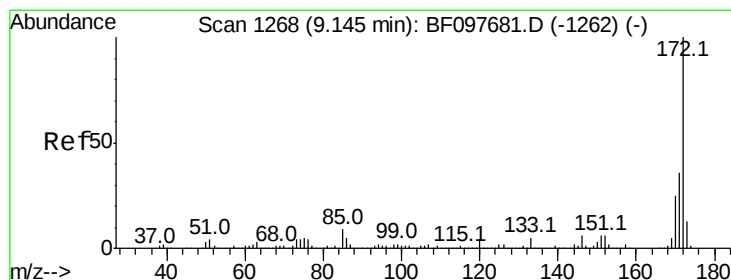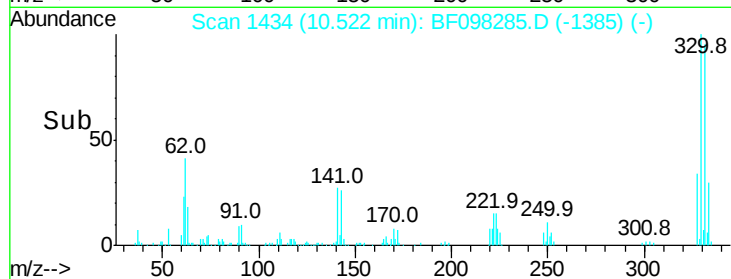
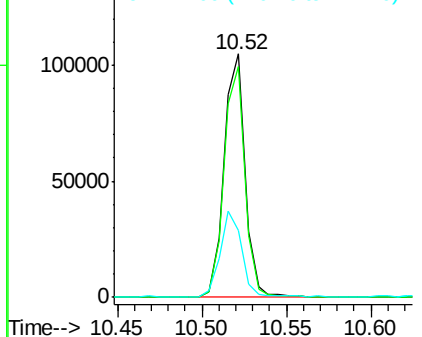



#44
 2-Fluorobiphenyl
 Concen: 59.843 ng
 RT: 9.06 min Scan# 1185
 Delta R.T. -0.01 min
 Lab File: BF098285.D
 Acq: 6 Sep 2017 21:06

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.5	29.6	44.4
170	24.2	19.8	29.8

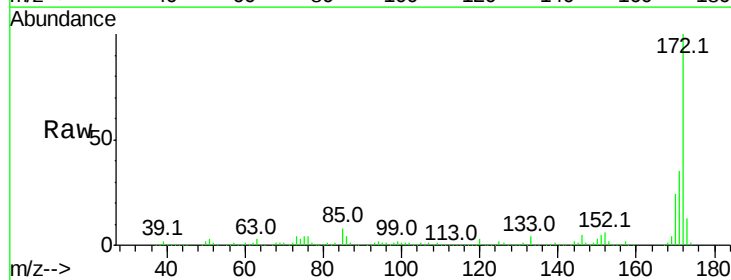

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



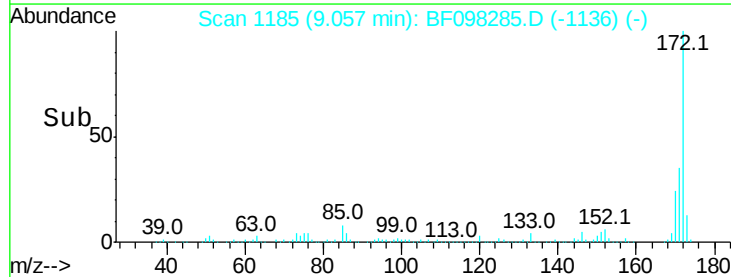
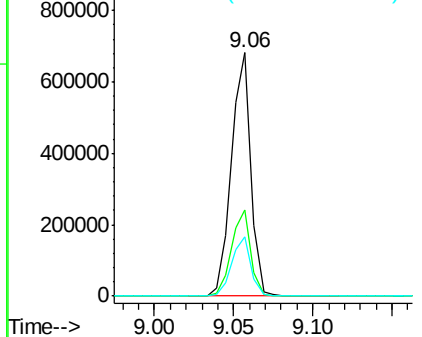


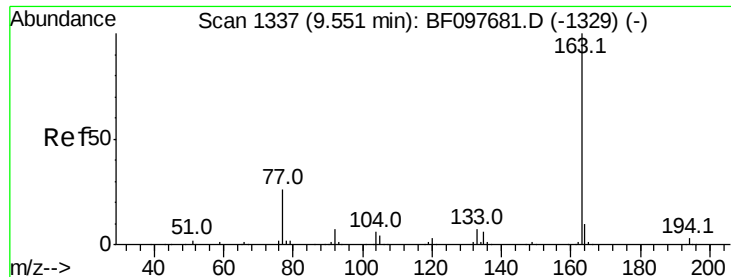

#49
Dimethylphthalate
Concen: 2.256 ng
RT: 9.45 min Scan# 1252
Delta R.T. -0.02 min
Lab File: BF098285.D
Acq: 6 Sep 2017 21:06




Instrument :
BNA_F
ClientSampleId :
AU-06-090117-A


Tot Ion:163 Resp: 23494
Ion Ratio Lower Upper
163 100
194 4.1 2.6 4.0#
164 10.4 8.4 12.6

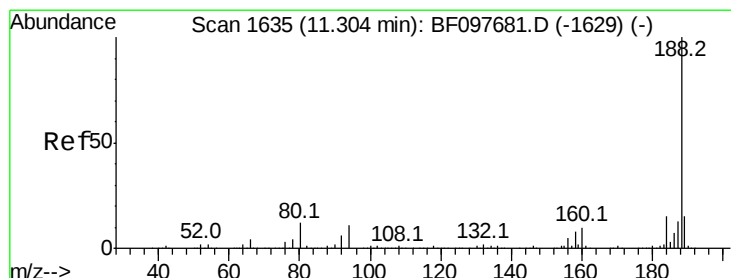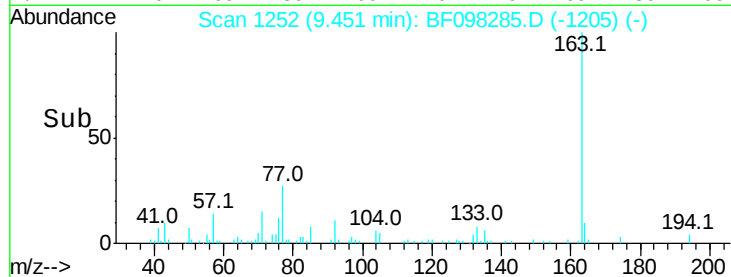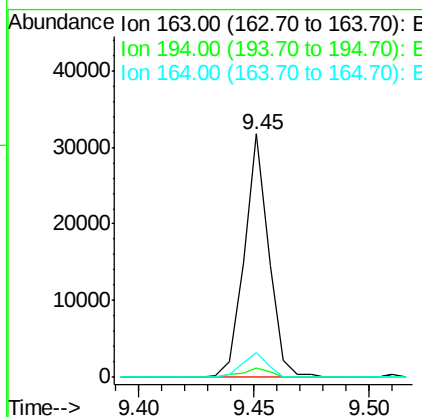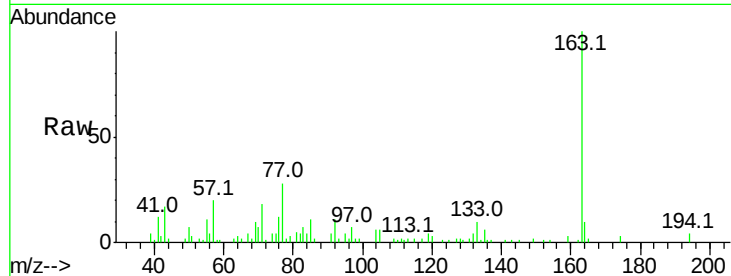

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.21 min Scan# 1551
Delta R.T. -0.01 min
Lab File: BF098285.D
Acq: 6 Sep 2017 21:06

Tgt Ion:188 Resp: 239887
Ion Ratio Lower Upper
188 100
94 12.7 9.4 14.2
80 13.7 10.2 15.2

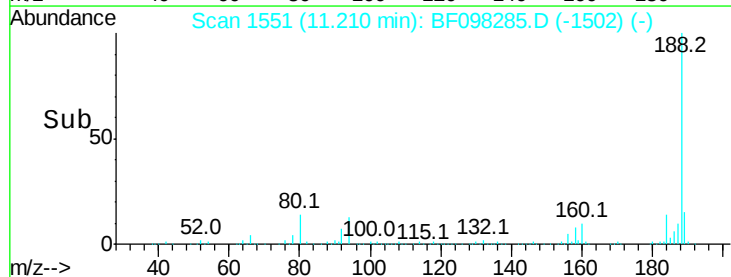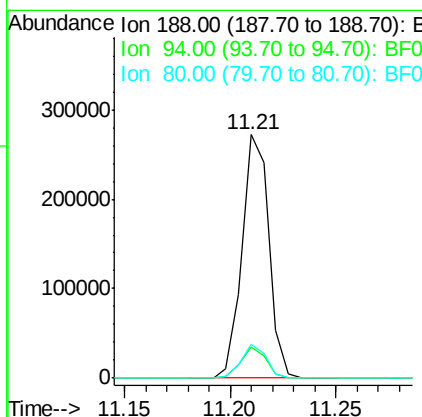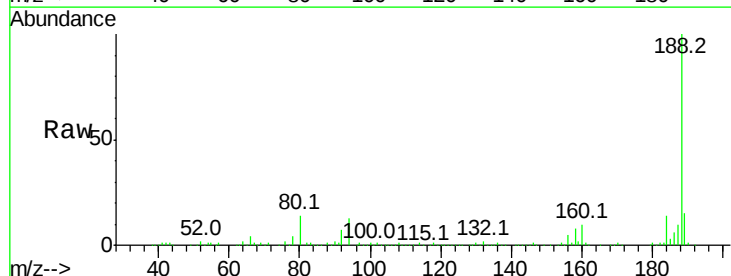

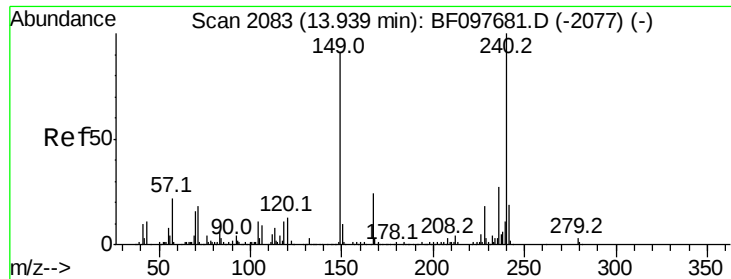

#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.85 min Scan# 2000

Delta R.T. -0.01 min

Lab File: BF098285.D

Acq: 6 Sep 2017 21:06

Instrument :

BNA_F

ClientSampleId :

AU-06-090117-A


Tot Ion:240 Resp: 253365

Ion Ratio Lower Upper

240 100

120 13.4 5.8 8.8#




236 26.3 20.5 30.7

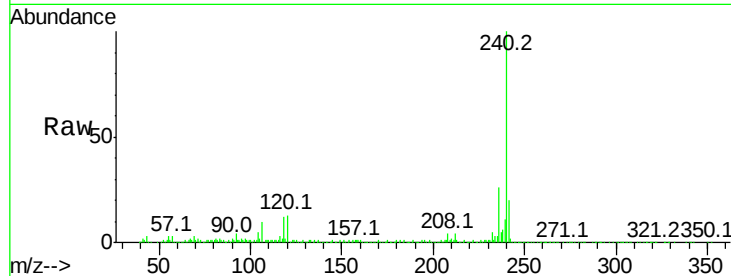

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

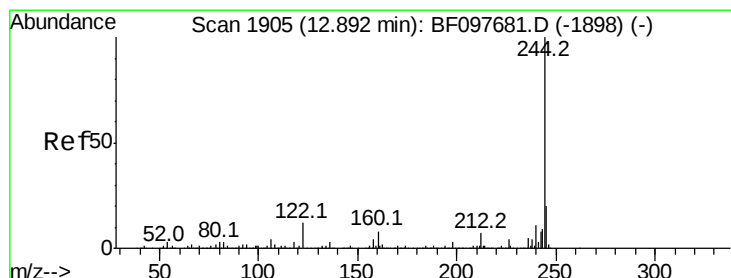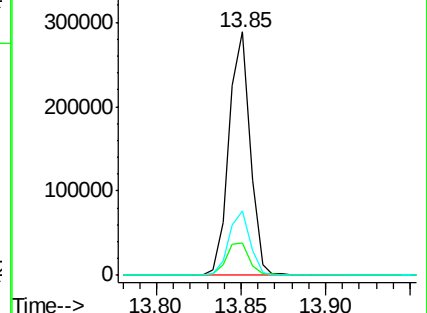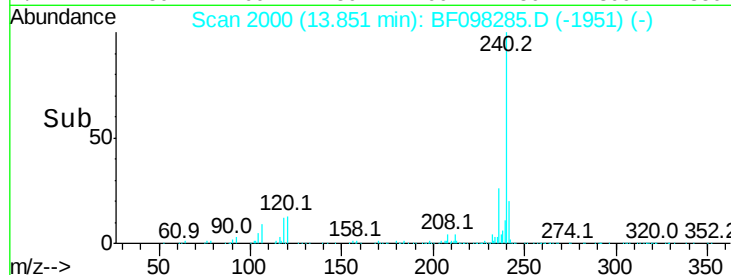

#78

Terphenyl-d14

Concen: 36.118 ng

RT: 12.80 min Scan# 1822

Delta R.T. -0.01 min

Lab File: BF098285.D

Acq: 6 Sep 2017 21:06


Tgt Ion:244 Resp: 438829

Ion Ratio Lower Upper

244 100

212 7.3 6.0 9.0



122 14.0 10.3 15.5

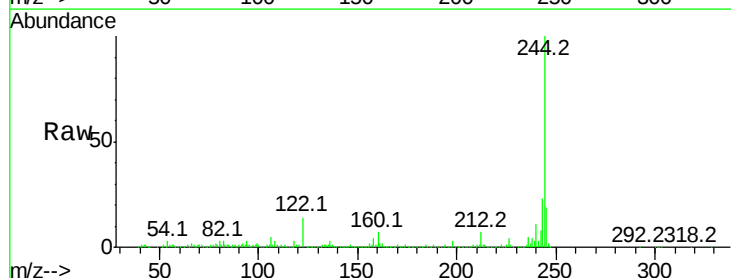


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

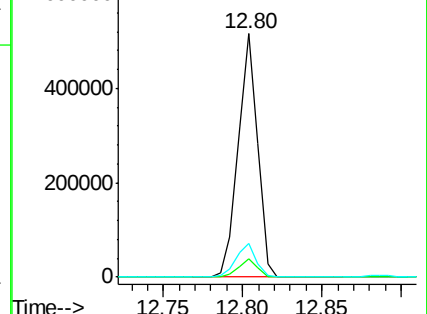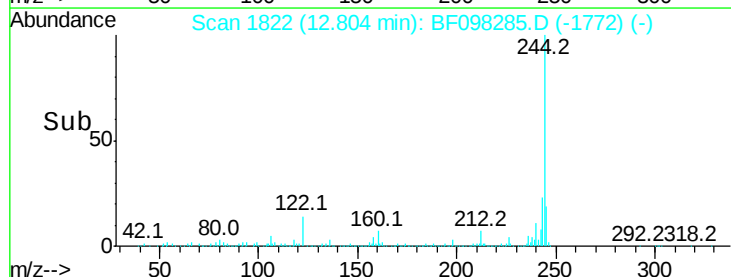


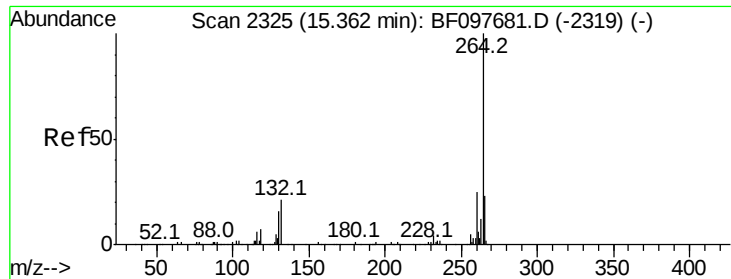

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.26 min Scan# 2240
Delta R.T. 0.00 min
Lab File: BF098285.D
Acq: 6 Sep 2017 21:06

Instrument :
BNA_F
ClientSampleId :
AU-06-090117-A

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.9	19.5	29.3
265	22.8	17.2	25.8

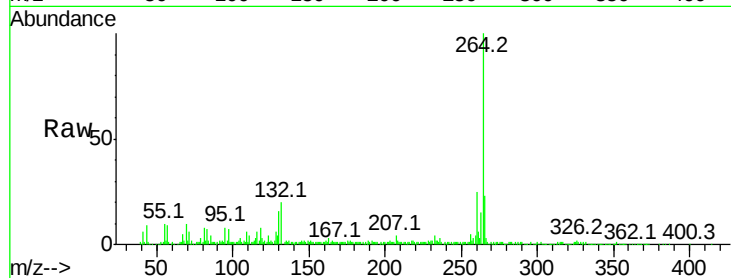

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

