

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF090617\
 Data File : BF098303.D
 Acq On : 7 Sep 2017 6:00
 Operator : SJ/JU
 Sample : I5083-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CLEAN-SAND-8

Quant Time: Sep 07 07:43:29 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 05 17:28:20 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.70	152	188908	20.00	ng	0.00
21) Naphthalene-d8	7.98	136	686810	20.00	ng	0.00
38) Acenaphthene-d10	9.73	164	262325	20.00	ng	0.00
63) Phenanthrene-d10	11.22	188	442655	20.00	ng	0.00
75) Chrysene-d12	13.84	240	414578	20.00	ng	-0.02
86) Perylene-d12	15.26	264	289015	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.31	112	877000	70.62	ng	0.00
7) Phenol-d6	6.35	99	1156521	68.54	ng	0.00
23) Nitrobenzene-d5	7.26	82	693569	54.86	ng	-0.01
41) 2,4,6-Tribromophenol	10.52	330	155259	68.21	ng	-0.01
44) 2-Fluorobiphenyl	9.06	172	912376	51.10	ng	-0.01
78) Terphenyl-d14	12.80	244	679906	34.20	ng	-0.01
Target Compounds						Qvalue
49) Dimethylphthalate	9.45	163	124838	6.510	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF090617\
Data File : BF098303.D
Acq On : 7 Sep 2017 6:00
Operator : SJ/JU
Sample : I5083-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CLEAN-SAND-8

Quant Time: Sep 07 07:43:29 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 05 17:28:20 2017
Response via : Initial Calibration

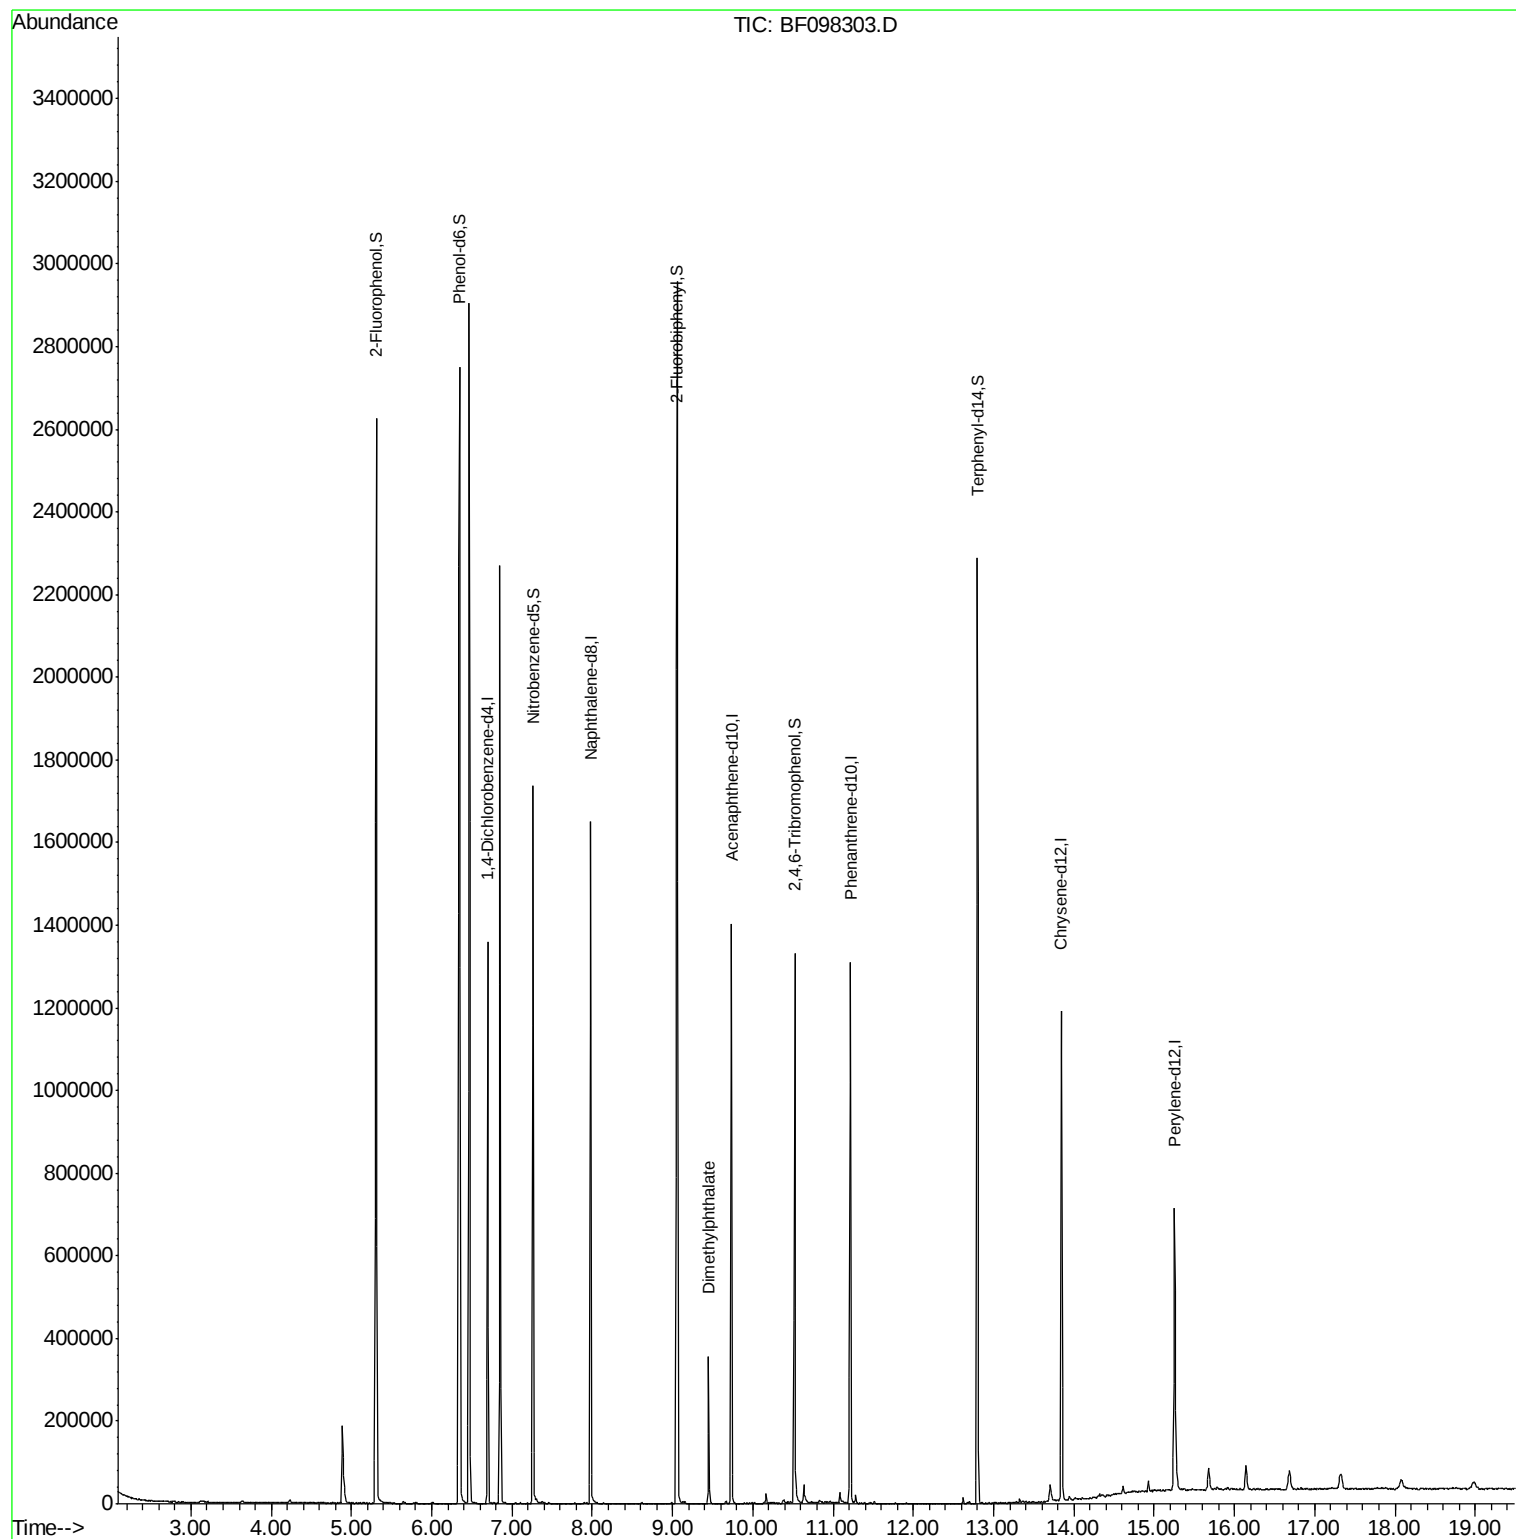

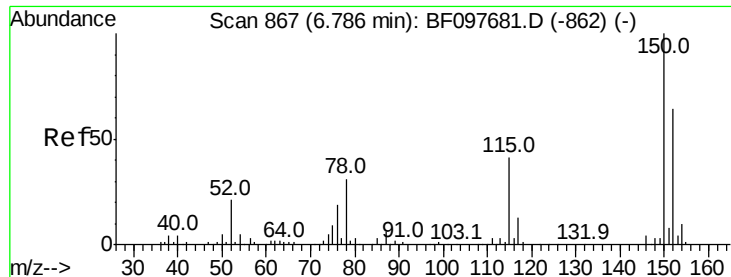


#1



1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.70 min Scan# 784
 Delta R.T. -0.01 min
 Lab File: BF098303.D
 Acq: 7 Sep 2017 6:00

Instrument :
 BNA_F
 ClientSampleId :
 CLEAN-SAND-8

Tot Ion:152 Resp: 188908
 Ion Ratio Lower Upper
 152 100
 150 155.0 126.2 189.2
 115 64.0 52.2 78.2

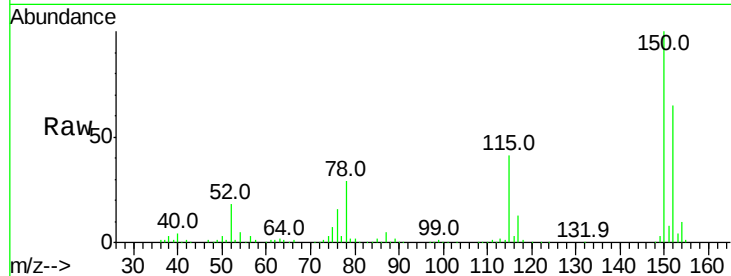


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

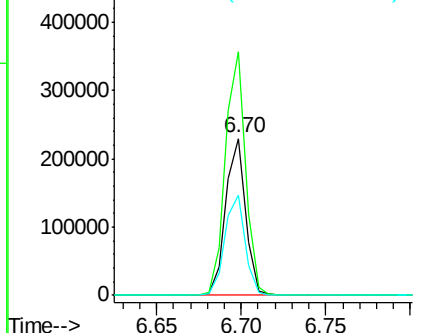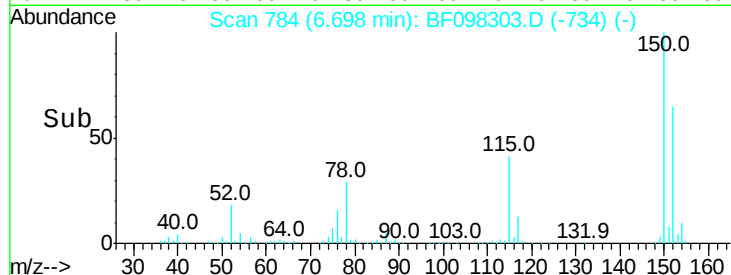



#5


2-Fluorophenol
 Concen: 70.615 ng
 RT: 5.31 min Scan# 548
 Delta R.T. 0.01 min
 Lab File: BF098303.D
 Acq: 7 Sep 2017 6:00

Tgt Ion:112 Resp: 877000
 Ion Ratio Lower Upper
 112 100
 64 55.0 46.0 69.0
 63 27.5 23.4 35.0

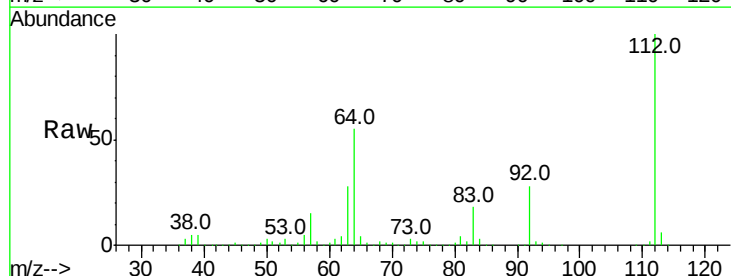

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

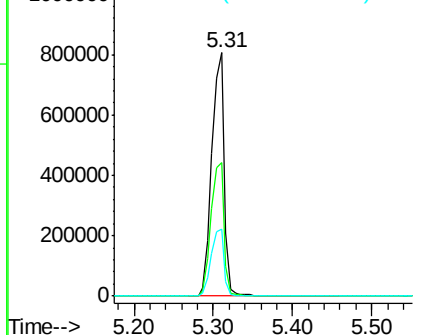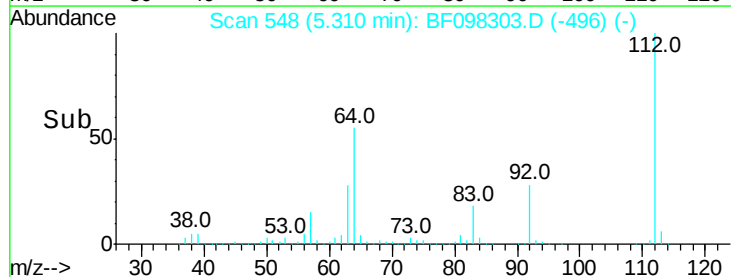

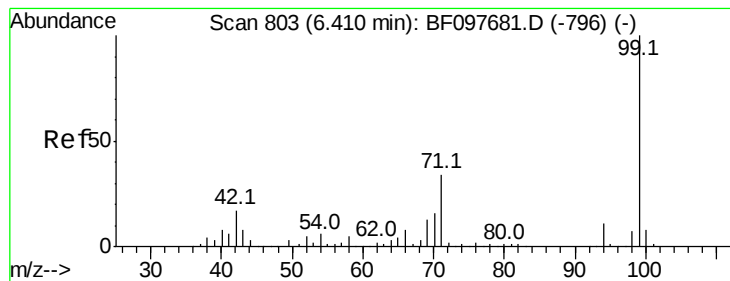

#7

Phenol-d6

Concen: 68.537 ng

RT: 6.35 min Scan# 724

Delta R.T. -0.01 min

Lab File: BF098303.D

Acq: 7 Sep 2017 6:00

Instrument :

BNA_F

ClientSampleId :

CLEAN-SAND-8


Tot Ion: 99 Resp: 1156521

Ion Ratio Lower Upper

99 100

42 14.5 13.5 20.3




71 32.4 24.5 36.7

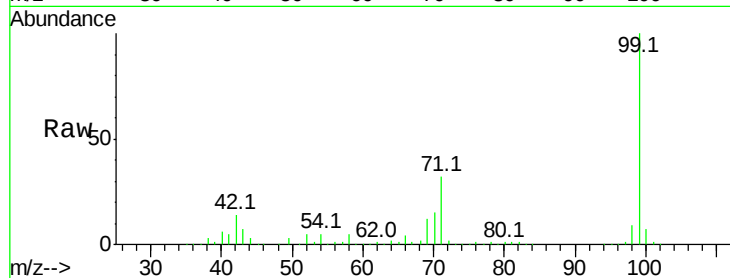

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

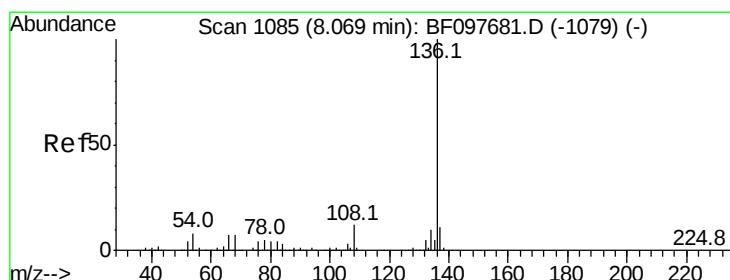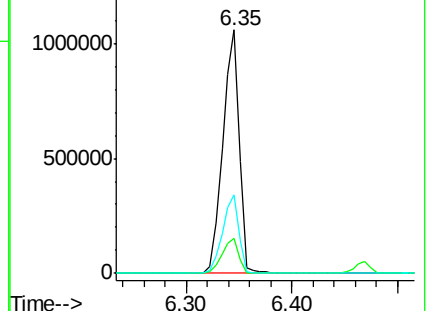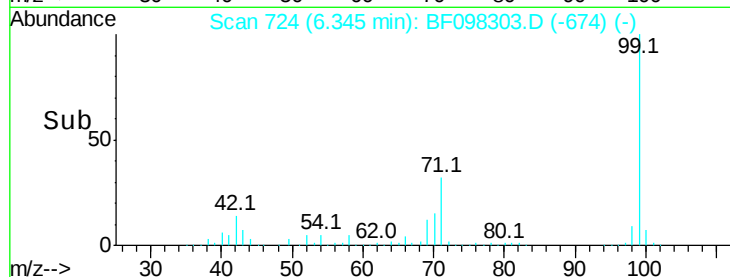

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.98 min Scan# 1002

Delta R.T. -0.01 min

Lab File: BF098303.D

Acq: 7 Sep 2017 6:00

Tgt Ion: 136 Resp: 686810


Ion Ratio Lower Upper

136 100

137 11.3 8.5 12.7

54 7.5 4.9 7.3#

68 7.4 4.1 6.1#


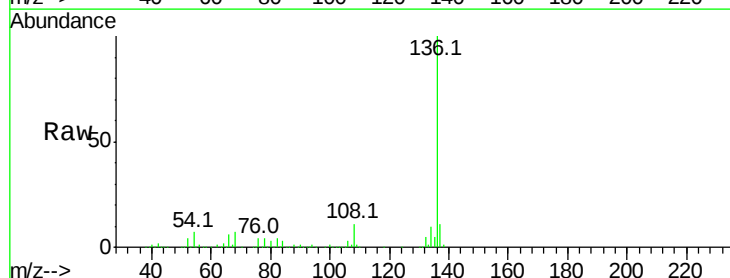


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



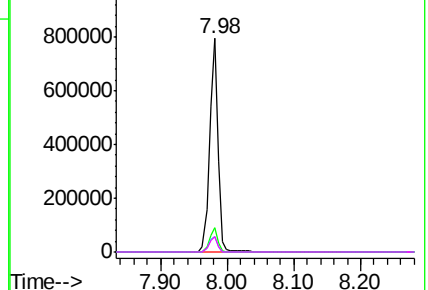
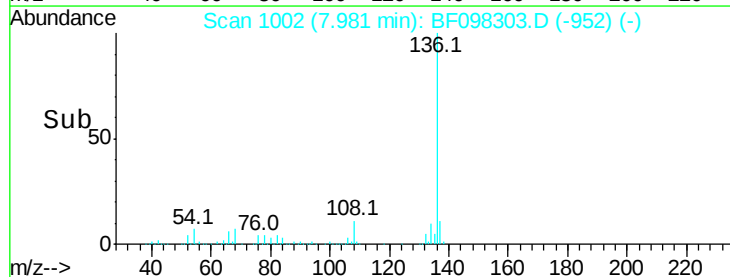




#23
 Nitrobenzene-d5
 Concen: 54.859 ng
 RT: 7.26 min Scan# 880
 Delta R.T. -0.01 min
 Lab File: BF098303.D
 Acq: 7 Sep 2017 6:00




Instrument :
 BNA_F
 ClientSampleId :
 CLEAN-SAND-8

Tot Ion: 82 Resp: 693569
 Ion Ratio Lower Upper
 82 100
 128 38.9 34.0 51.0
 54 39.8 42.2 63.2#

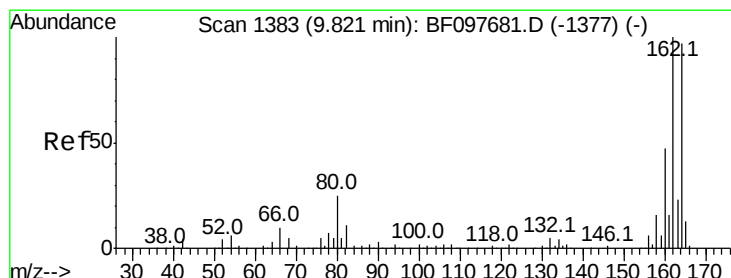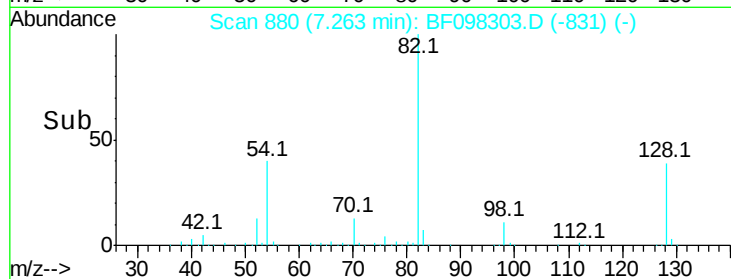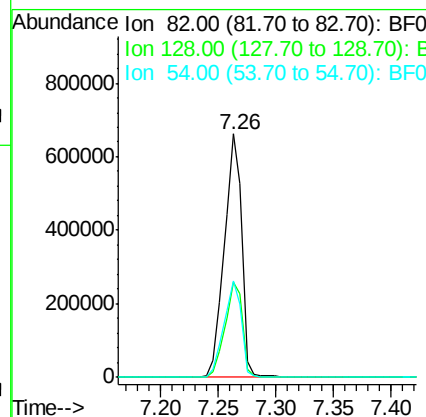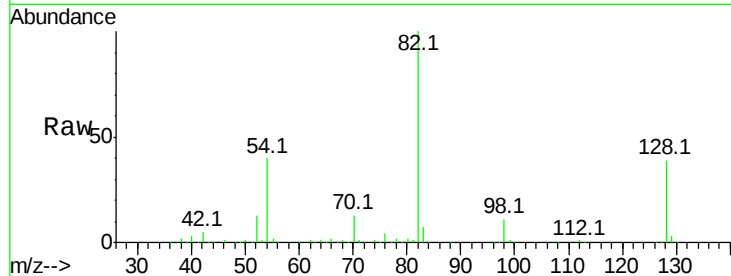

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.73 min Scan# 1300
 Delta R.T. -0.01 min
 Lab File: BF098303.D
 Acq: 7 Sep 2017 6:00

Tgt Ion:164 Resp: 262325
 Ion Ratio Lower Upper
 164 100
 162 103.3 82.6 123.8
 160 49.7 36.2 54.2


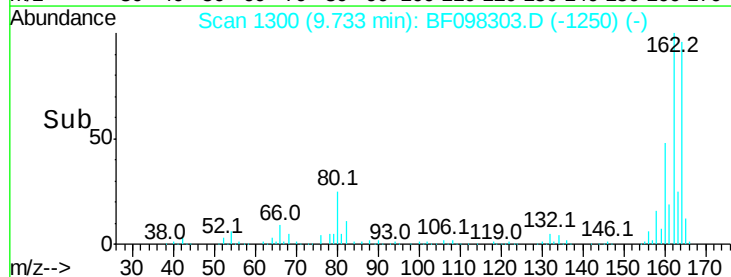
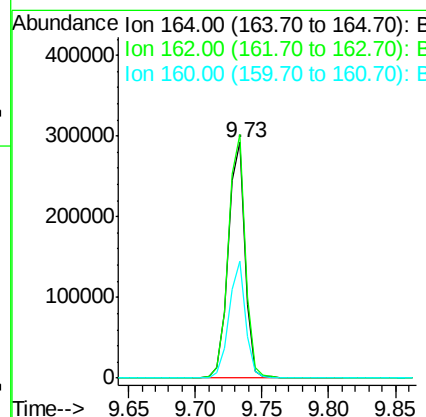
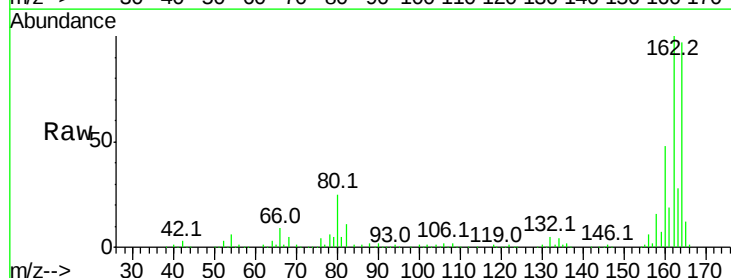




#41
 2,4,6-Tribromophenol
 Concen: 68.213 ng
 RT: 10.52 min Scan# 1434
 Delta R.T. -0.01 min
 Lab File: BF098303.D
 Acq: 7 Sep 2017 6:00




Instrument :
 BNA_F
 ClientSampleId :
 CLEAN-SAND-8


Tot Ion:330 Resp: 155259
 Ion Ratio Lower Upper
 330 100
 332 94.7 76.6 115.0
 141 36.5 31.4 47.2

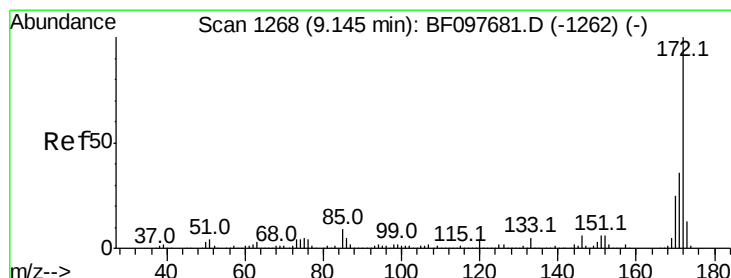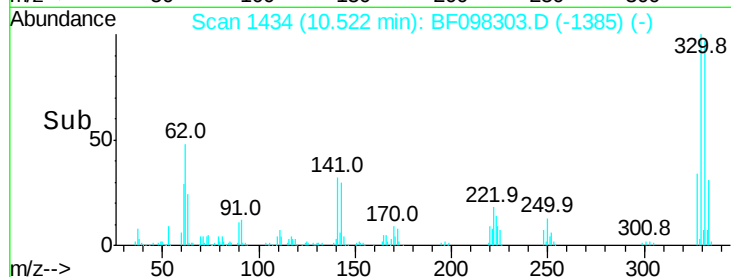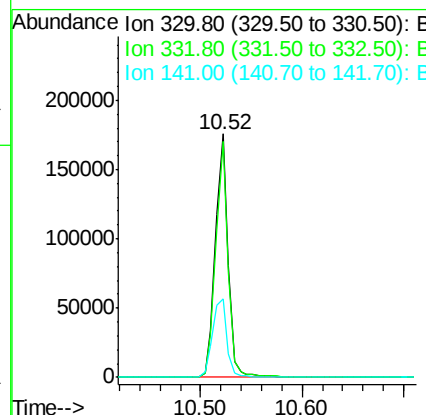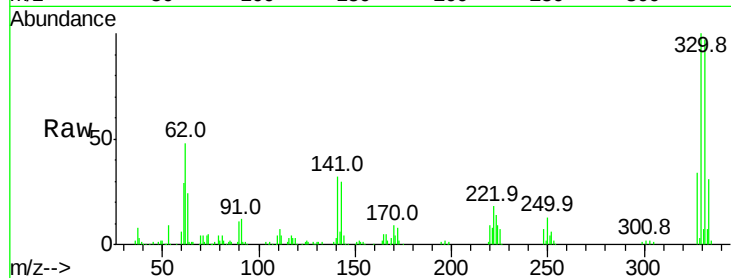

#44
 2-Fluorobiphenyl
 Concen: 51.100 ng
 RT: 9.06 min Scan# 1185
 Delta R.T. -0.01 min
 Lab File: BF098303.D
 Acq: 7 Sep 2017 6:00

Tgt Ion:172 Resp: 912376
 Ion Ratio Lower Upper
 172 100
 171 36.4 29.6 44.4
 170 24.1 19.8 29.8

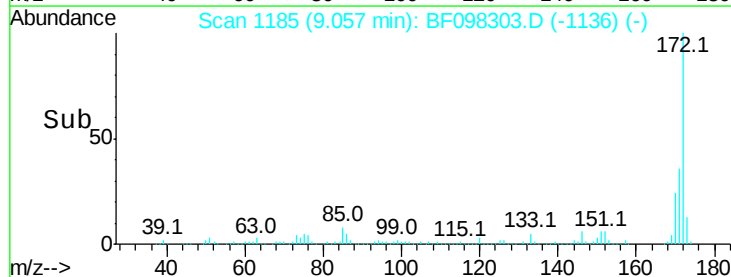
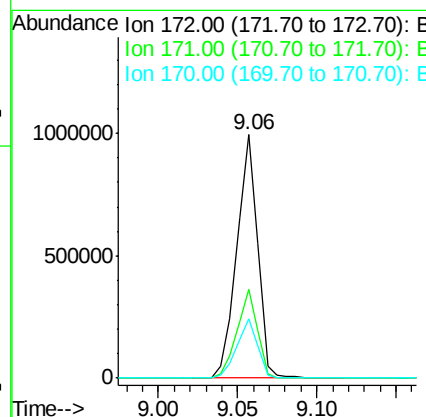
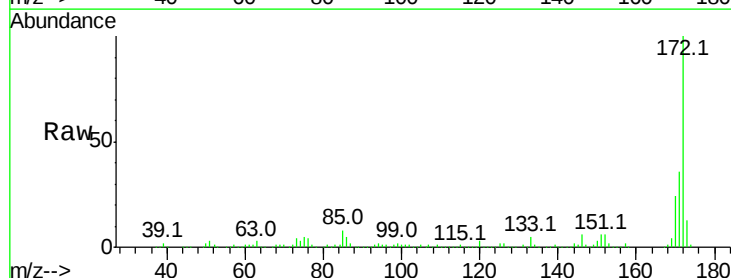


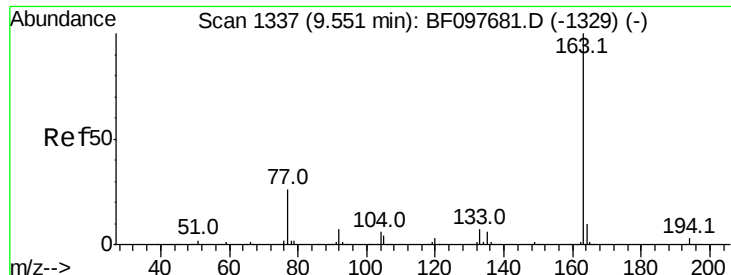

#49
Dimethylphthalate
Concen: 6.510 ng
RT: 9.45 min Scan# 1252
Delta R.T. -0.02 min
Lab File: BF098303.D
Acq: 7 Sep 2017 6:00




Instrument :
BNA_F
ClientSampleId :
CLEAN-SAND-8


Tot Ion:163 Resp: 124838
Ion Ratio Lower Upper
163 100
194 3.7 2.6 4.0
164 9.7 8.4 12.6

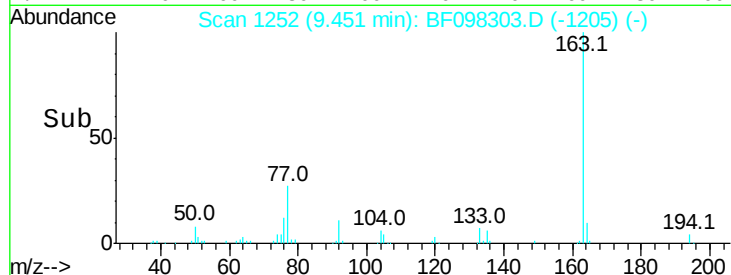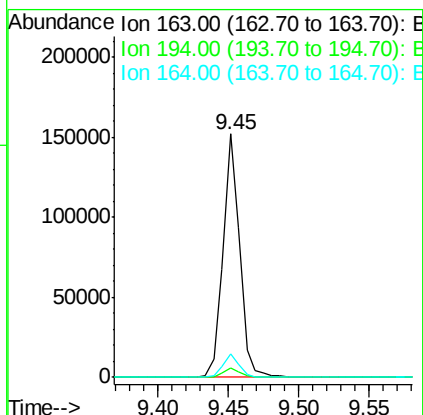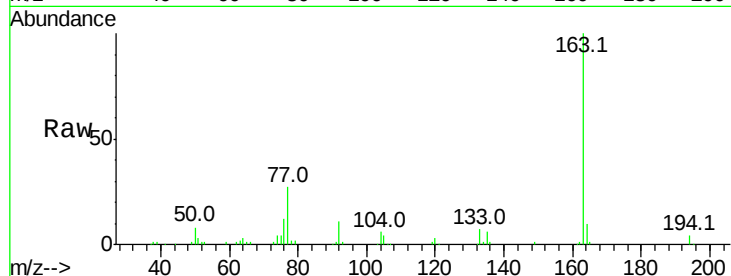

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.22 min Scan# 1552
Delta R.T. -0.01 min
Lab File: BF098303.D
Acq: 7 Sep 2017 6:00

Tgt Ion:188 Resp: 442655
Ion Ratio Lower Upper
188 100
94 11.2 9.4 14.2
80 12.5 10.2 15.2

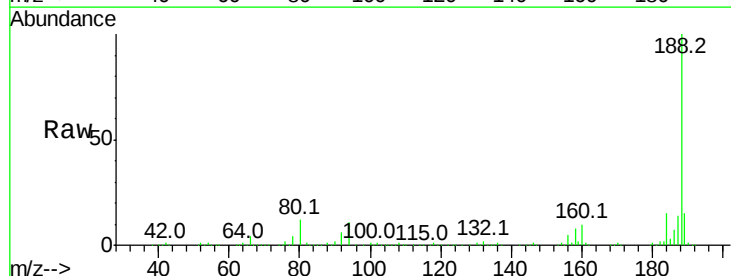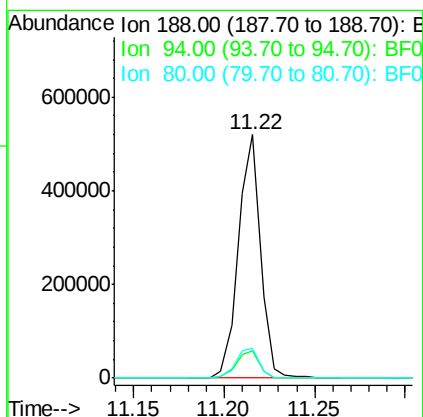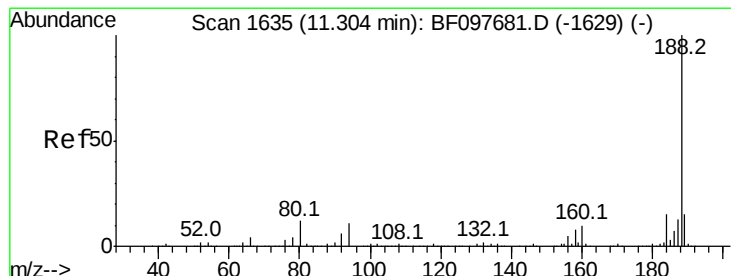

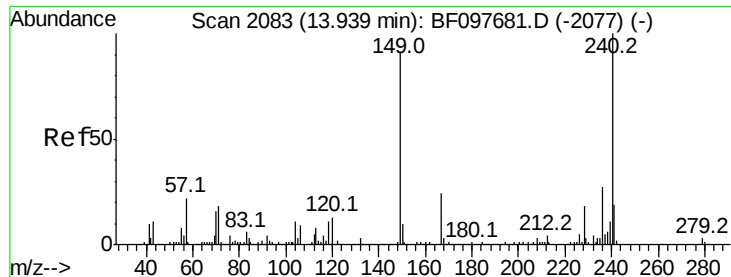

#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.84 min Scan# 1999

Delta R.T. -0.02 min

Lab File: BF098303.D

Acq: 7 Sep 2017 6:00

Instrument :

BNA_F

ClientSampleId :

CLEAN-SAND-8


Tot Ion:240 Resp: 414578

Ion Ratio Lower Upper

240 100

120 15.7 5.8 8.8#



236 26.7 20.5 30.7

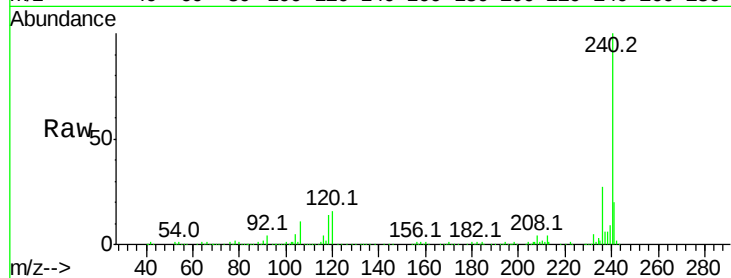

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

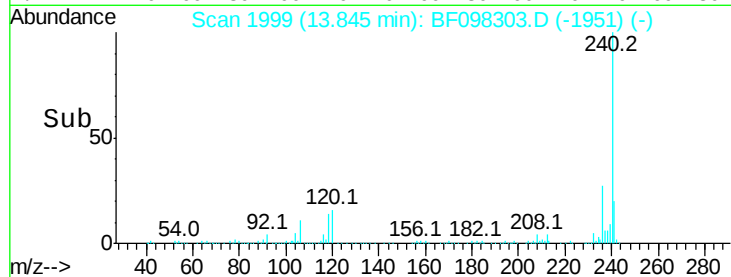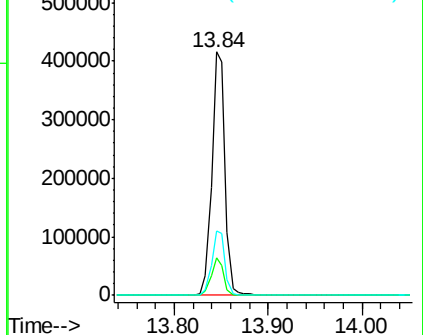

#78

Terphenyl-d14

Concen: 34.199 ng

RT: 12.80 min Scan# 1821

Delta R.T. -0.01 min

Lab File: BF098303.D

Acq: 7 Sep 2017 6:00


Tgt Ion:244 Resp: 679906

Ion Ratio Lower Upper

244 100

212 7.2 6.0 9.0



122 13.3 10.3 15.5

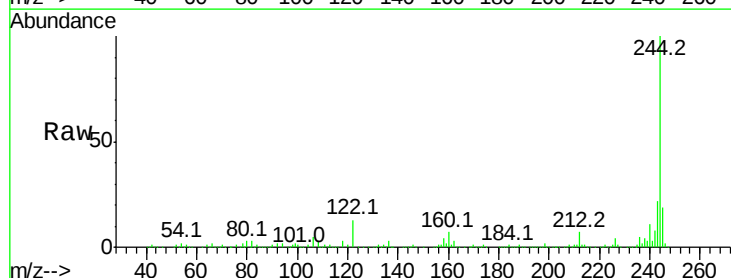


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

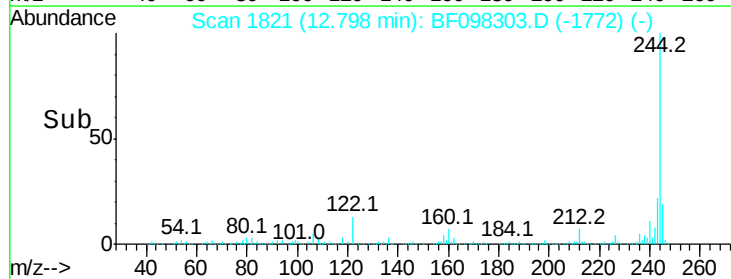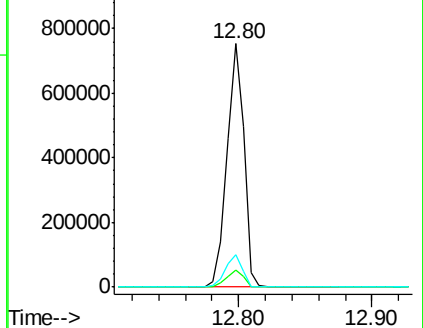


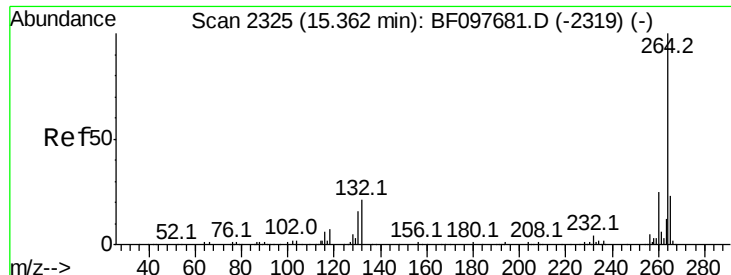

#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.26 min Scan# 2239
 Delta R.T. -0.01 min
 Lab File: BF098303.D
 Acq: 7 Sep 2017 6:00

Instrument :
 BNA_F
 ClientSampleId :
 CLEAN-SAND-8

Tot Ion	Ratio	Lower	Upper
264	100		
260	25.3	19.5	29.3
265	21.3	17.2	25.8

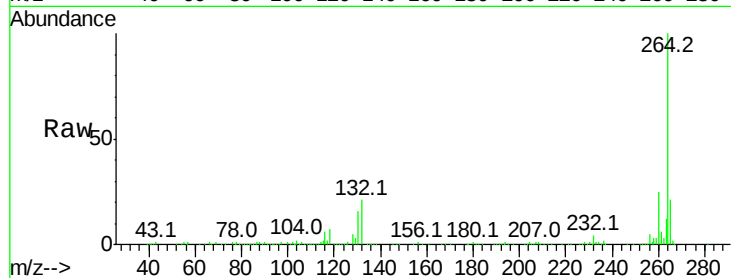

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

