


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF090617\
 Data File : BF098273.D
 Acq On : 6 Sep 2017 14:55
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 05 17:28:20 2017

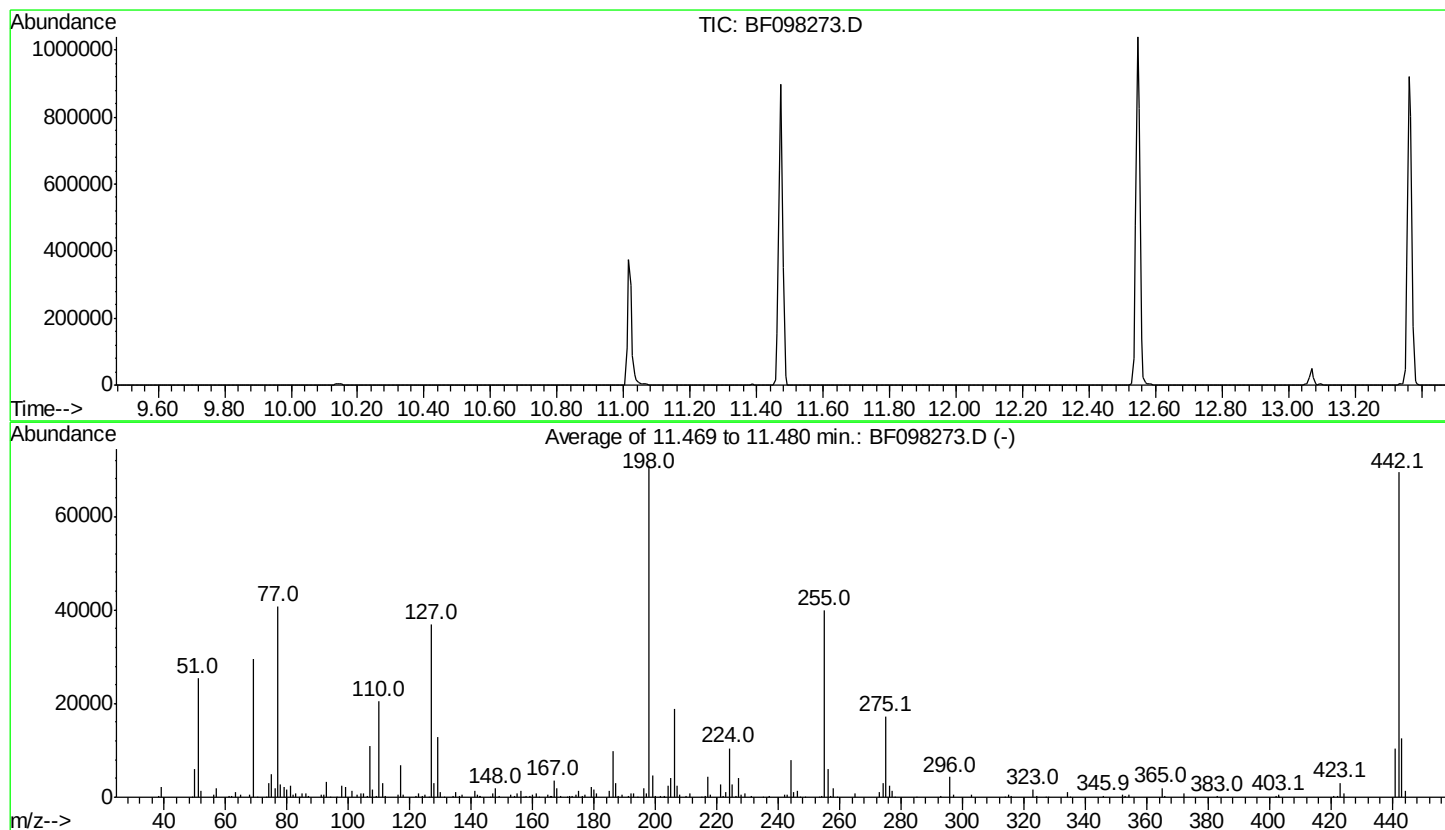

AutoFind: Scans 1595, 1596, 1597; Background Corrected with Scan 1590

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	25388	PASS
68	69	0.00	2	1.5	453	PASS
69	198	0.00	100	41.5	29407	PASS
70	69	0.00	2	0.4	109	PASS
127	198	10	80	52.1	36875	PASS
197	198	0.00	2	1.1	770	PASS
198	198	100	100	100.0	70805	PASS
199	198	5	9	6.6	4696	PASS
275	198	10	60	24.2	17152	PASS
365	198	1	100	2.8	1997	PASS
441	442	0.01	24	15.1	10531	PASS
442	198	50	100	98.2	69538	PASS
443	442	15	24	18.1	12601	PASS