


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF090617\
Data File : BF098298.D
Acq On : 7 Sep 2017 3:40
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Sep 05 17:28:20 2017

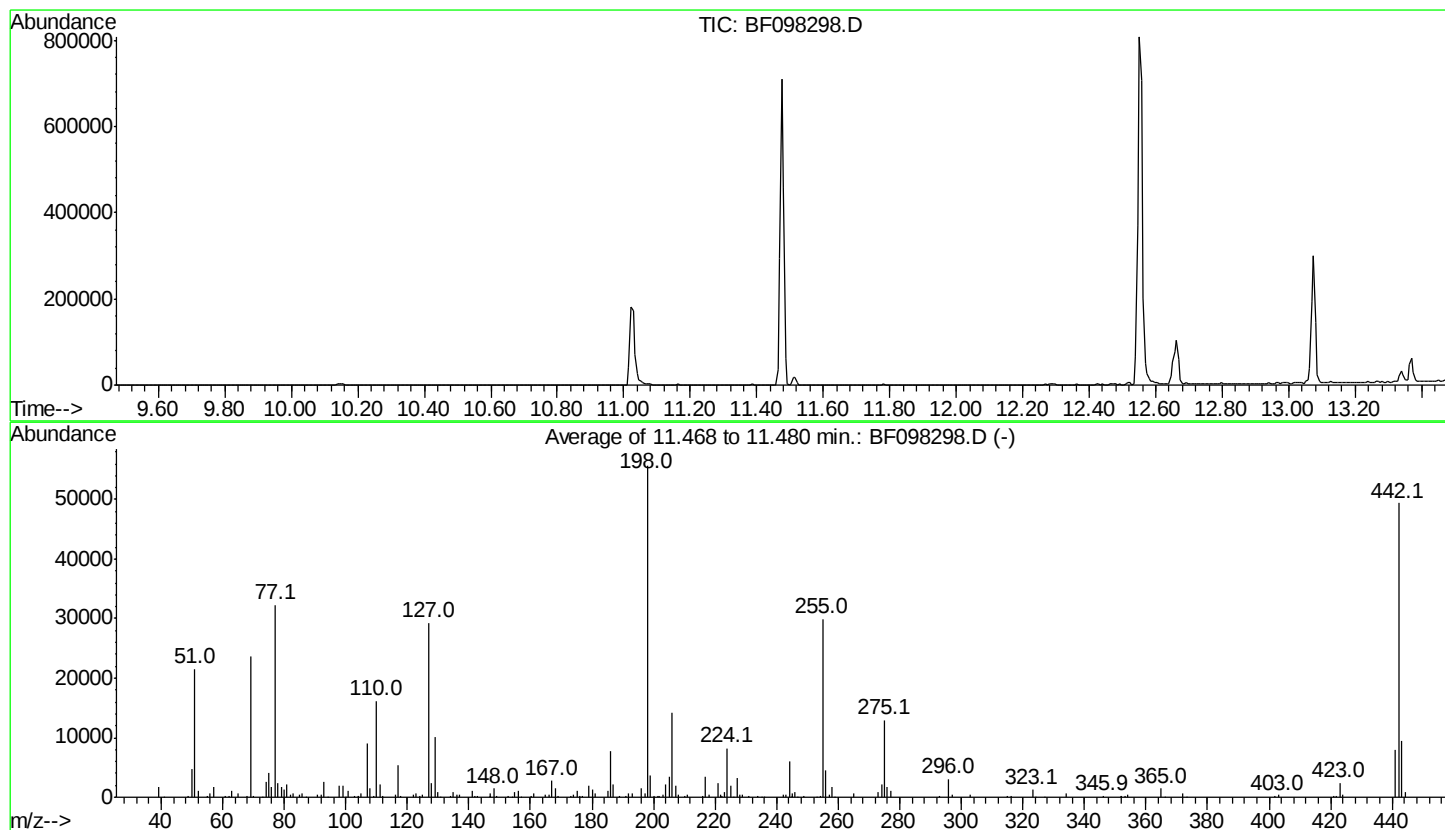

AutoFind: Scans 1595, 1596, 1597; Background Corrected with Scan 1591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	21585	PASS
68	69	0.00	2	1.2	277	PASS
69	198	0.00	100	42.6	23713	PASS
70	69	0.00	2	0.5	118	PASS
127	198	10	80	52.6	29320	PASS
197	198	0.00	2	1.2	654	PASS
198	198	100	100	100.0	55690	PASS
199	198	5	9	6.5	3627	PASS
275	198	10	60	23.3	12952	PASS
365	198	1	100	2.6	1453	PASS
441	442	0.01	24	16.0	7895	PASS
442	198	50	100	88.7	49418	PASS
443	442	15	24	19.3	9543	PASS