
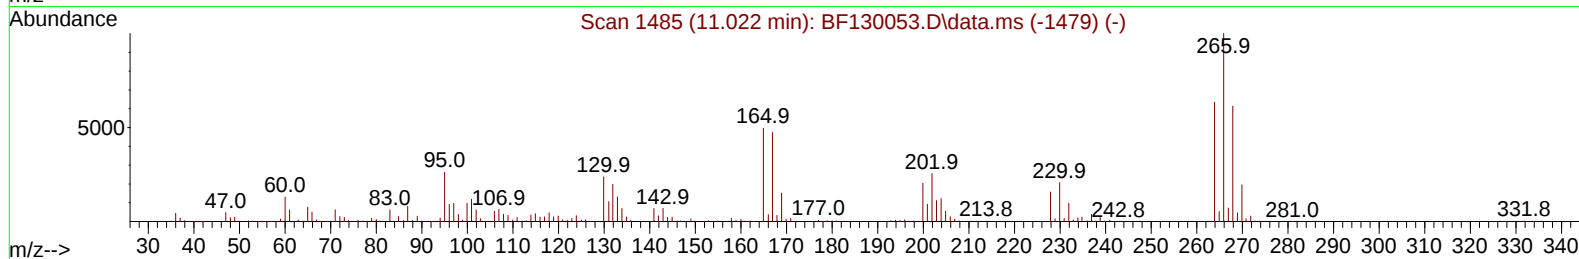
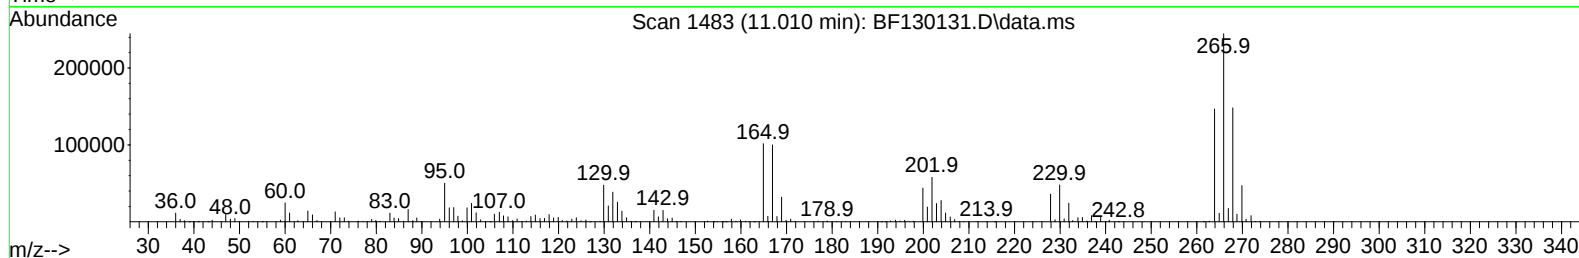


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090622\
Data File : BF130131.D
Acq On : 06 Sep 2022 11:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 07 07:12:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 07 02:05:07 2022
Response via : Initial Calibration

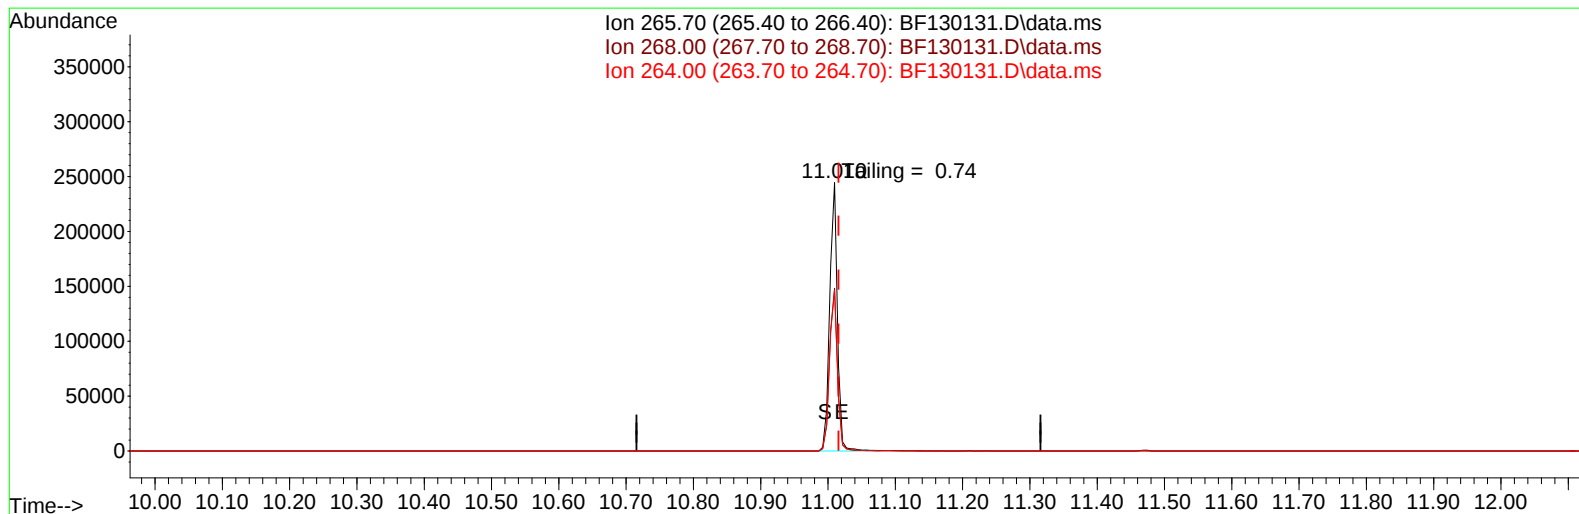

TIC: BF130131.D\data.ms

(70) Pentachlorophenol (C)




11.010min (-0.006) 498285.08 ng

response 195869

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	60.63
264.00	59.90	60.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090622\
Data File : BF130131.D
Acq On : 06 Sep 2022 11:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 07 07:12:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 07 02:05:07 2022
Response via : Initial Calibration

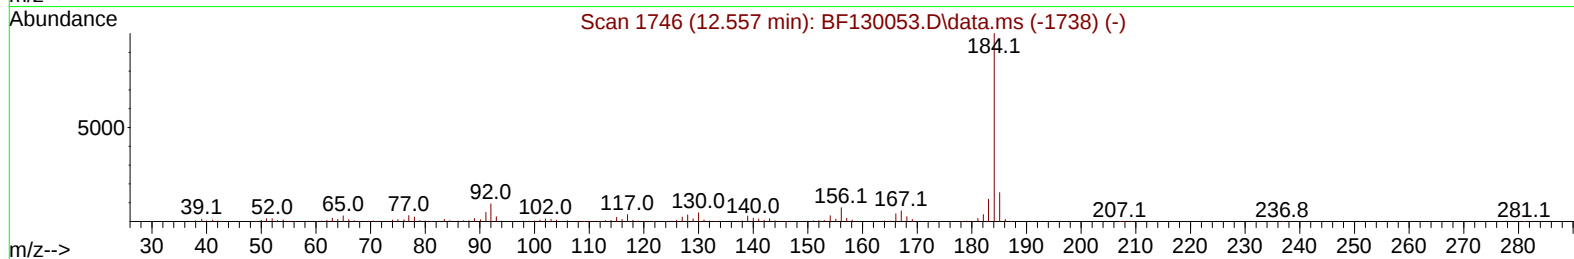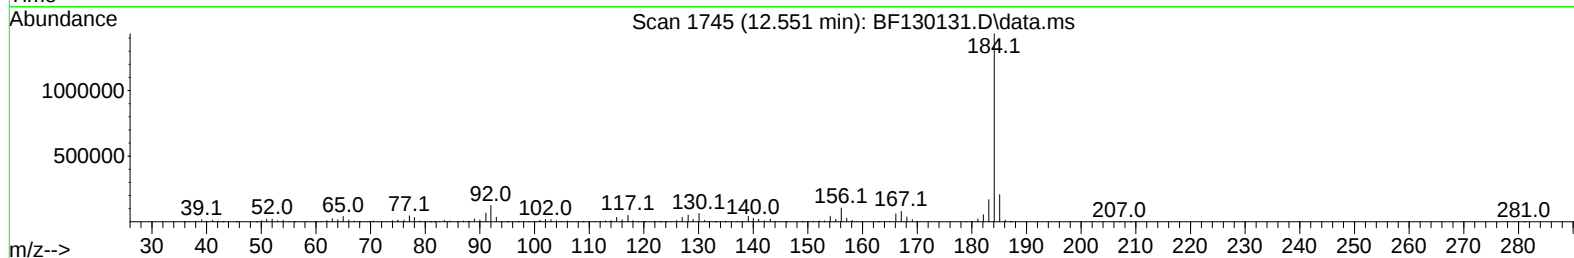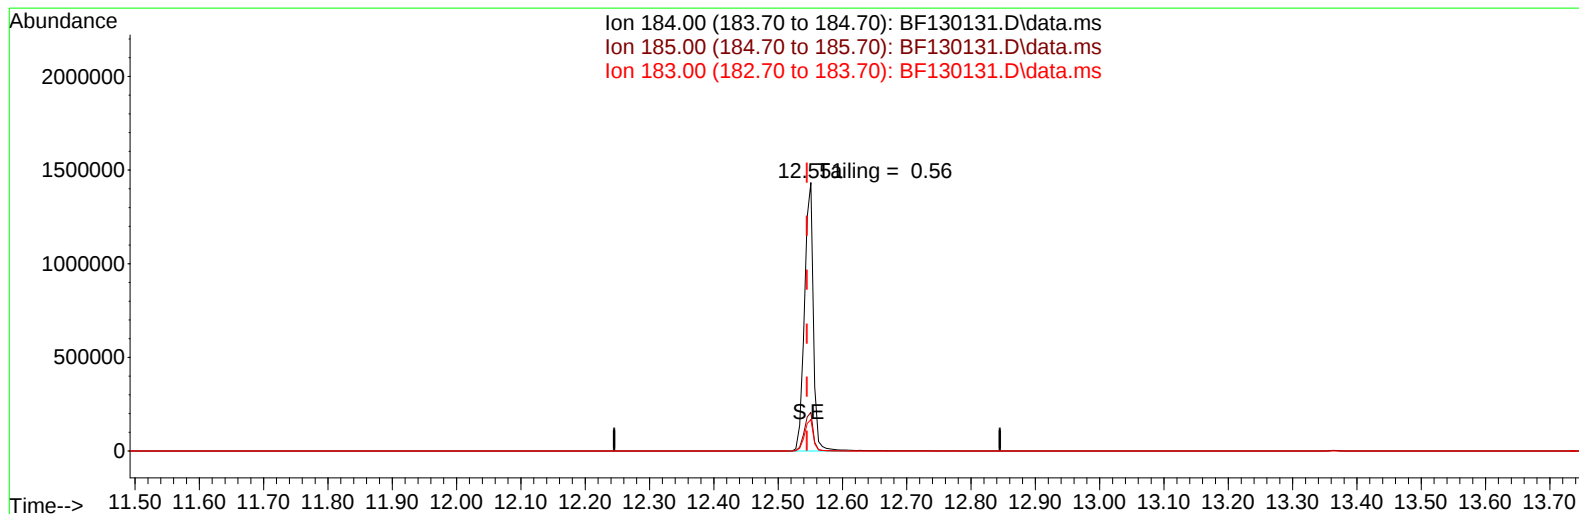

TIC: BF130131.D\data.ms

(77) Benzidine

12.551min (+ 0.006) 74420.69 ng

response 1384396

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.41
183.00	11.80	11.77
0.00	0.00	0.00