

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090622\
 Data File : BF130133.D
 Acq On : 06 Sep 2022 12:43
 Operator : CG\JU
 Sample : PB147410BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB147410BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130133.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.304	508	513	516	rBV	4003344	4183041	50.63%	9.917%
2	6.328	681	687	690	rBV	4006194	4143448	50.15%	9.823%
3	6.692	746	749	753	rBV	1573240	1359183	16.45%	3.222%
4	7.263	840	846	849	rBV	3575677	3683644	44.59%	8.733%
5	7.975	962	967	971	rBV	1995795	1895500	22.94%	4.494%
6	9.057	1144	1151	1154	rBV	7243317	7368264	89.19%	17.468%
7	9.728	1259	1265	1268	rBV	2507467	2228850	26.98%	5.284%
8	10.510	1392	1398	1402	rBV	3413995	3248354	39.32%	7.701%
9	11.204	1512	1516	1520	rBV	2813308	2357392	28.54%	5.589%
10	12.798	1781	1787	1790	rBV	7627232	8261384	100.00%	19.586%
11	13.833	1959	1963	1967	rBV	2317151	1971951	23.87%	4.675%
12	13.933	1975	1980	1988	rBV	77717	93261	1.13%	0.221%
13	15.233	2196	2201	2206	rBV	1230109	1386144	16.78%	3.286%




Sum of corrected areas: 42180416

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090622\
Data File : BF130133.D
Acq On : 06 Sep 2022 12:43
Operator : CG\JU
Sample : PB147410BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147410BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

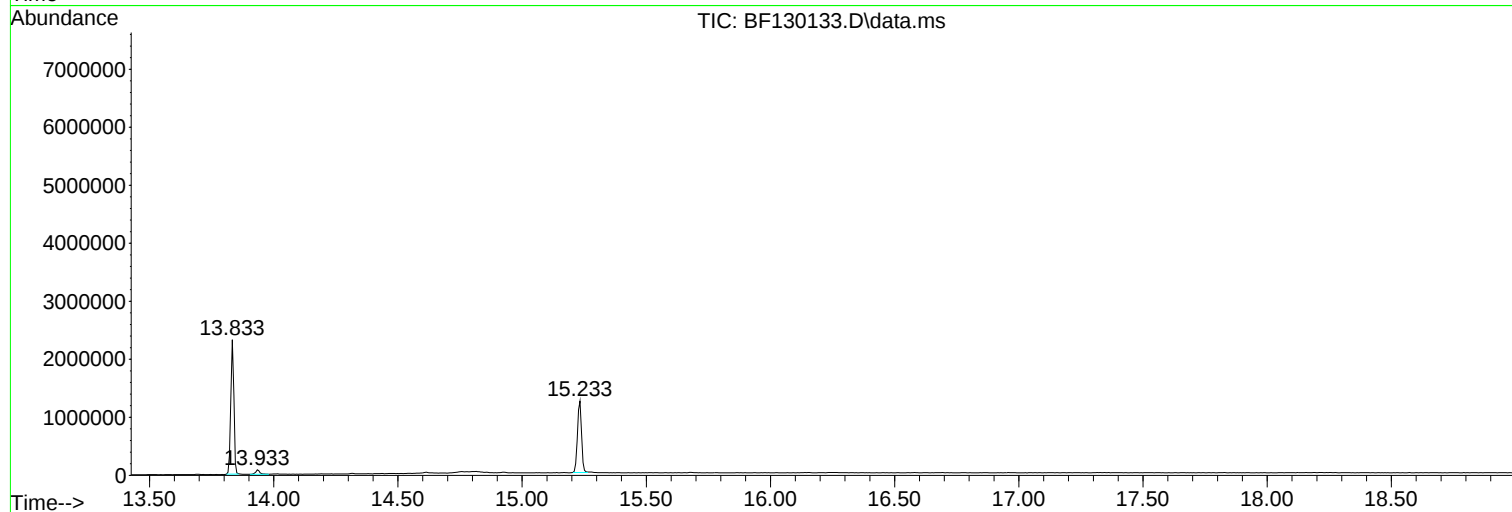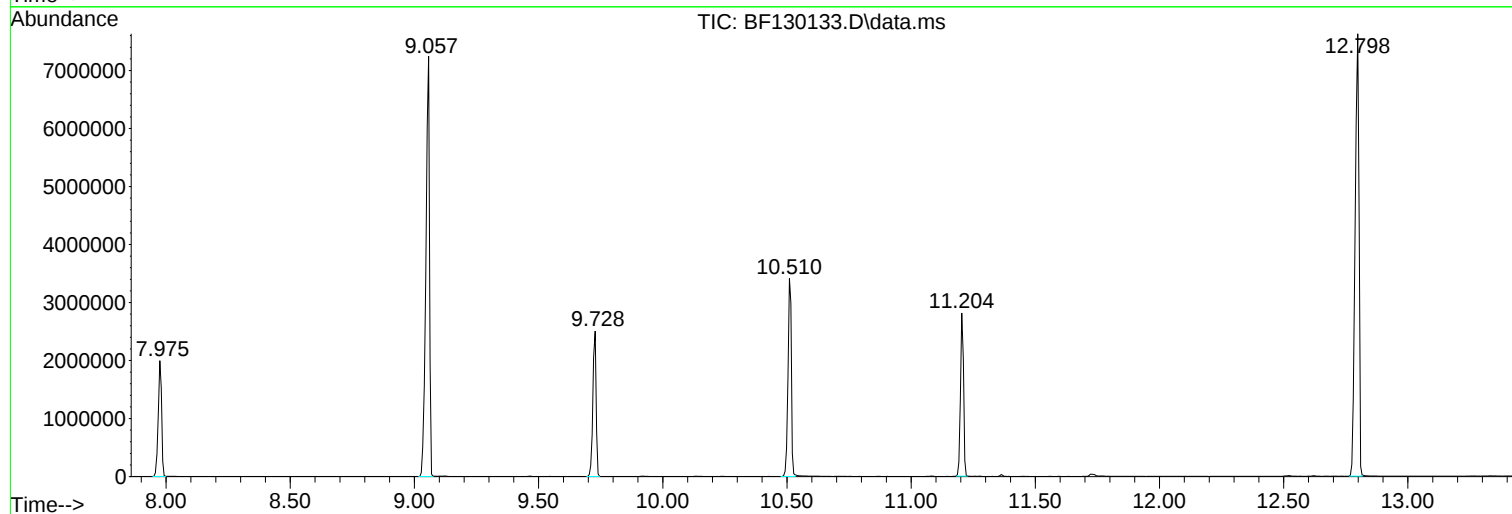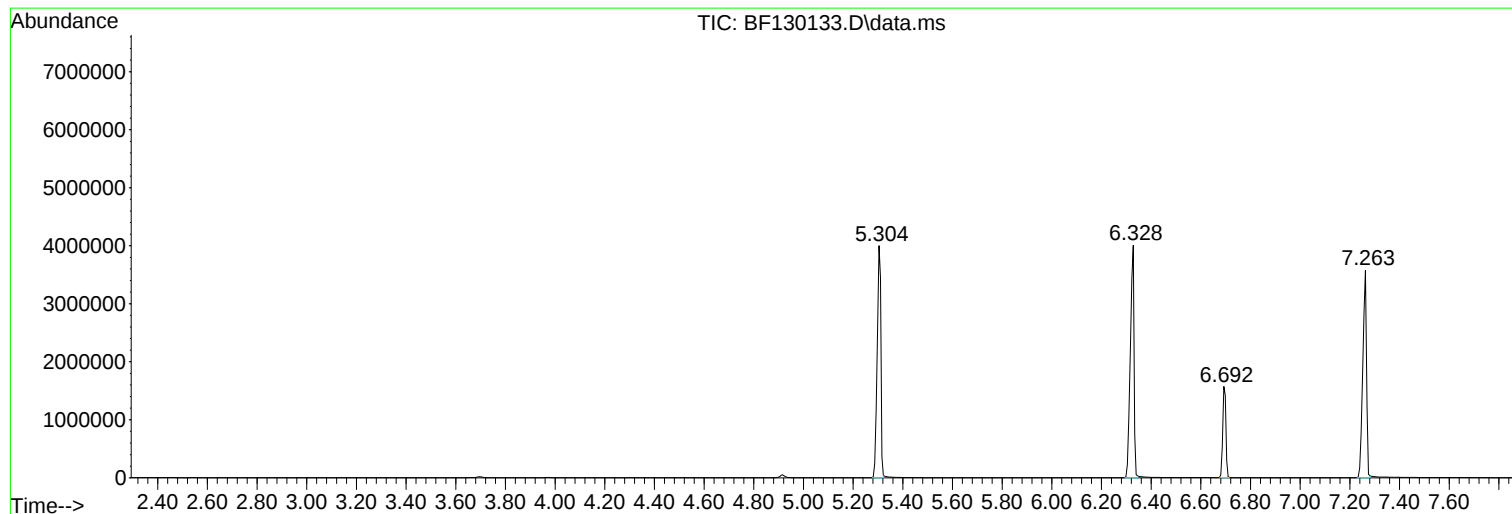

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090622\
Data File : BF130133.D
Acq On : 06 Sep 2022 12:43
Operator : CG\JU
Sample : PB147410BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147410BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090622\
Data File : BF130133.D
Acq On : 06 Sep 2022 12:43
Operator : CG\JU
Sample : PB147410BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147410BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------