
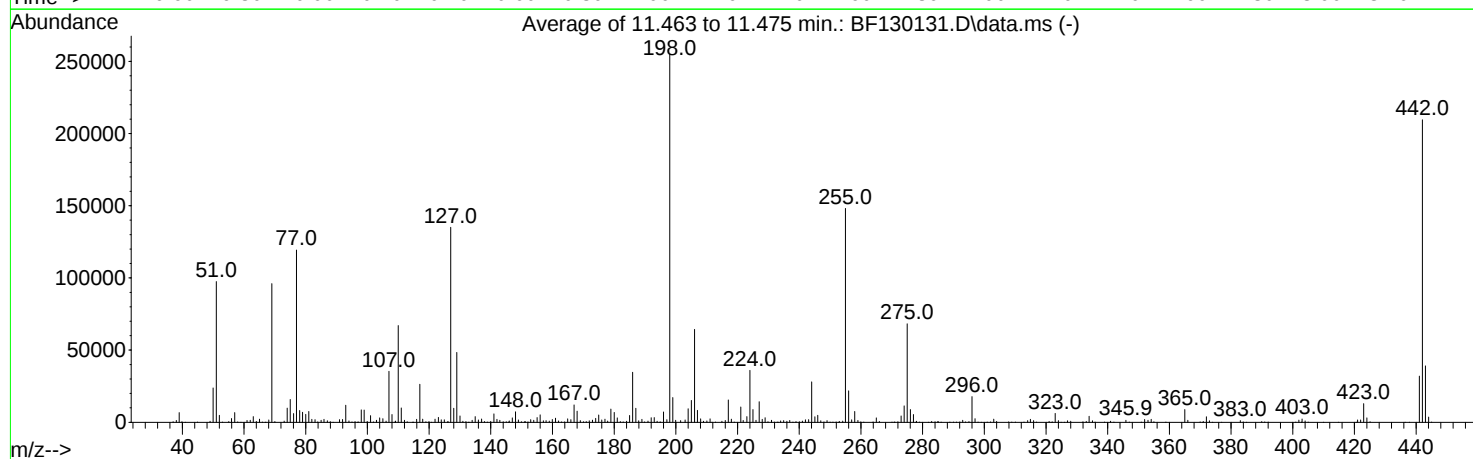


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090622\
 Data File : BF130131.D
 Acq On : 06 Sep 2022 11:29
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 07 02:05:07 2022

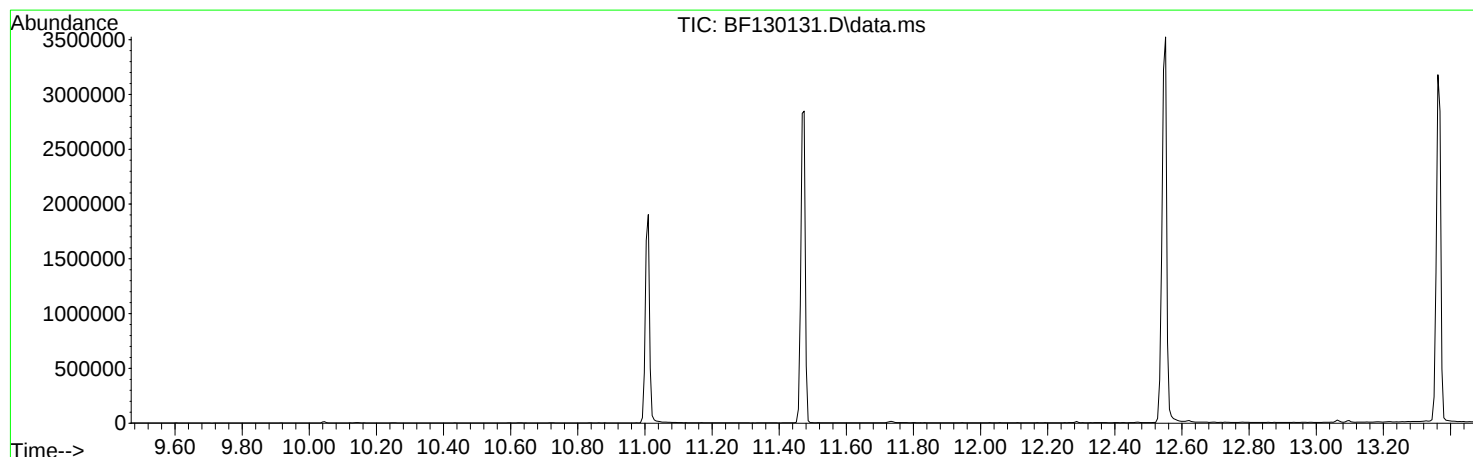




AutoFind: Scans 1560, 1561, 1562; Background Corrected with Scan 1555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	97453	PASS
68	69	0.00	2	1.7	1624	PASS
69	198	0.00	100	37.7	96008	PASS
70	69	0.00	2	0.5	495	PASS
127	198	10	80	53.0	135075	PASS
197	198	0.00	2	0.7	1849	PASS
198	198	100	100	100.0	254824	PASS
199	198	5	9	6.7	17151	PASS
275	198	10	60	26.8	68261	PASS
365	198	1	100	3.5	8803	PASS
441	198	0.01	100	12.6	32005	PASS
442	442	50	100	100.0	209493	PASS
443	442	15	24	18.7	39112	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090622\
Data File : BF130131.D
Acq On : 06 Sep 2022 11:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 07 07:12:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 07 02:05:07 2022
Response via : Initial Calibration

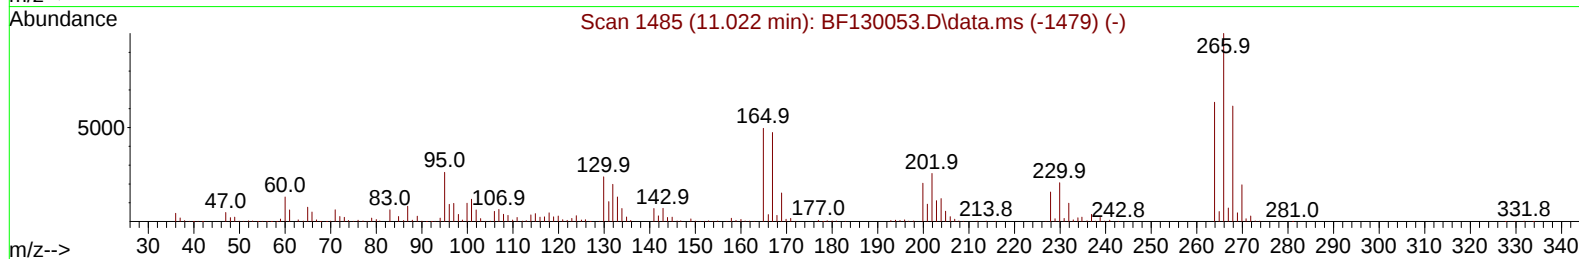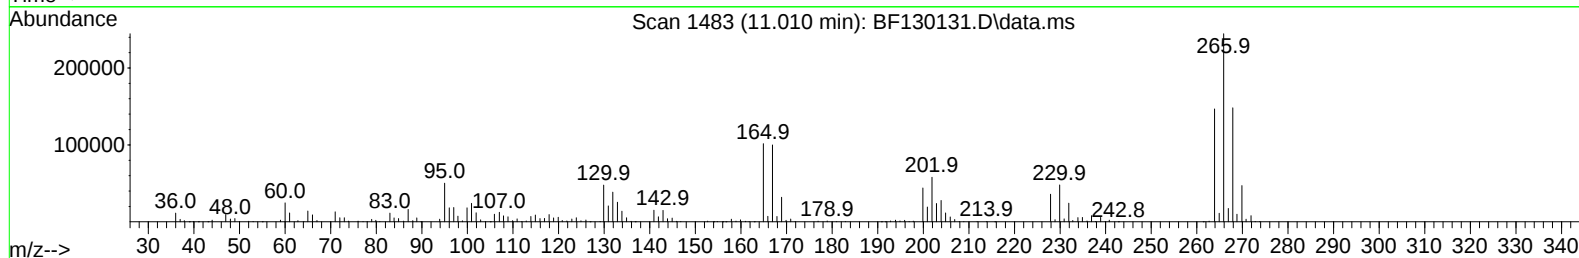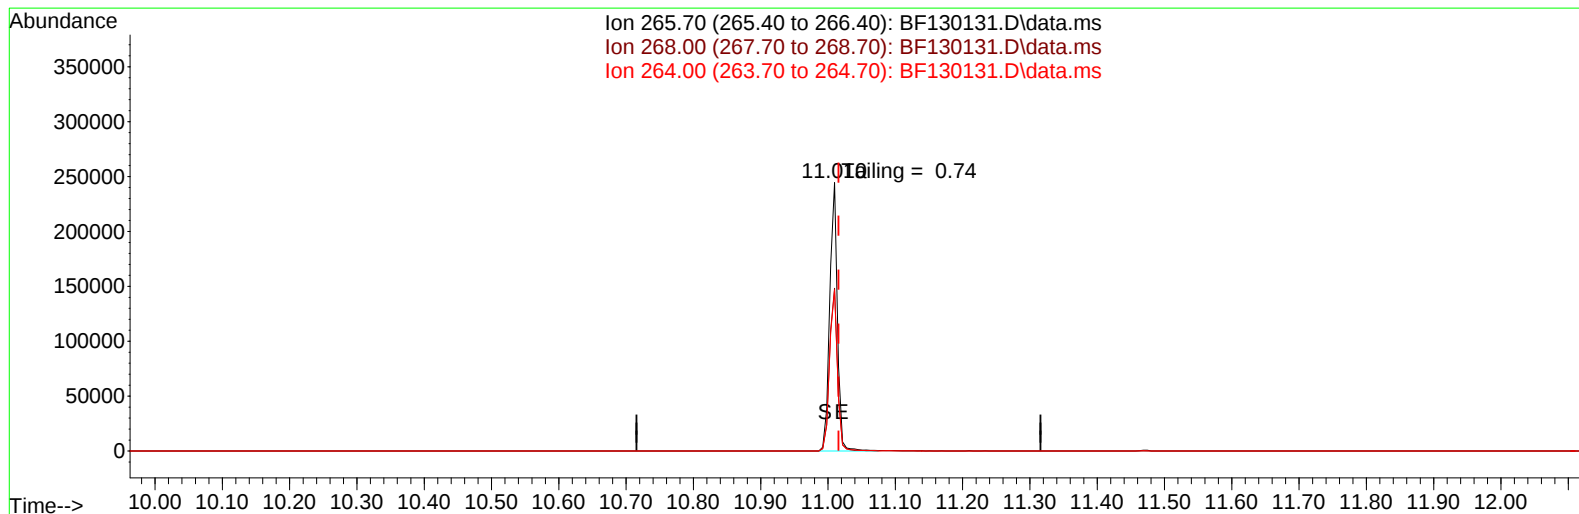

TIC: BF130131.D\data.ms

(70) Pentachlorophenol (C)

11.010min (-0.006) 498285.08 ng




response 195869

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	60.63
264.00	59.90	60.03
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090622\  
Data File : BF130131.D  
Acq On    : 06 Sep 2022  11:29  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 07 07:12:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 07 02:05:07 2022
Response via : Initial Calibration

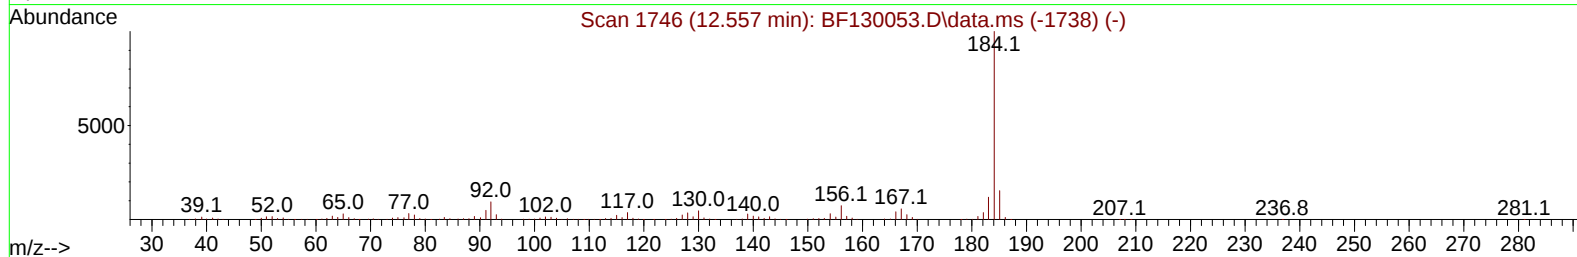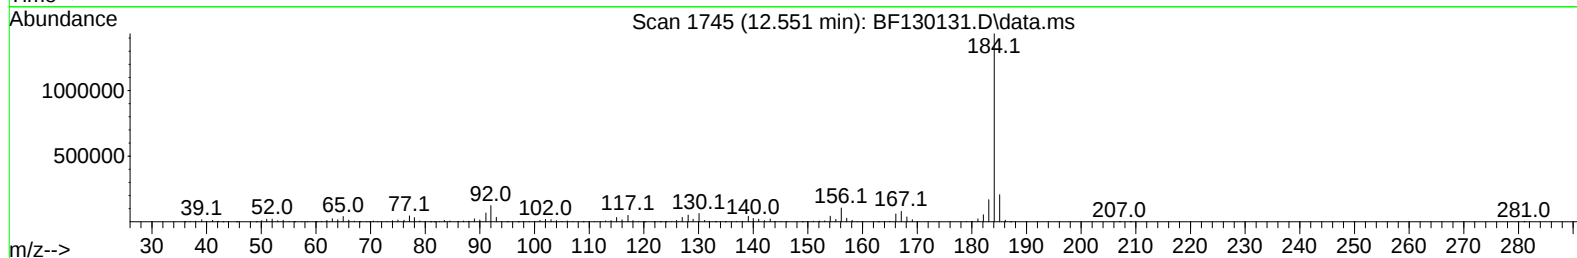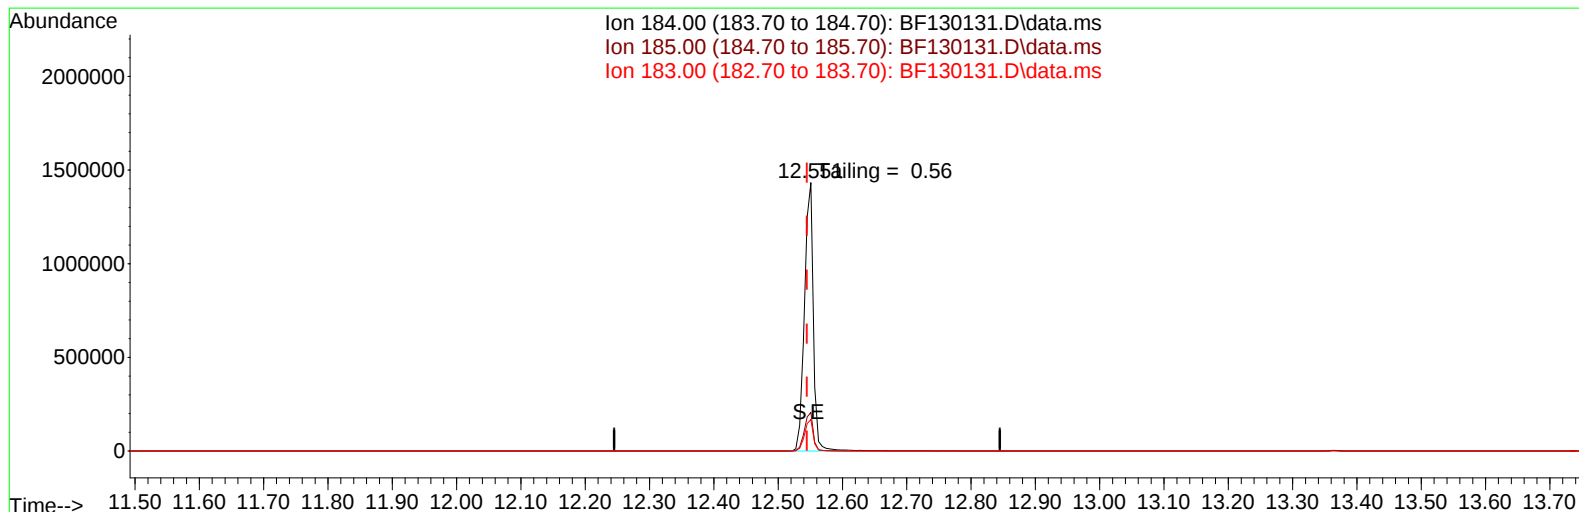

TIC: BF130131.D\data.ms

(77) Benzidine

12.551min (+ 0.006) 74420.69 ng

```
response      1384396
```

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.41
183.00	11.80	11.77
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/6/2022	BNA_F	<u>BF130131.D</u>
Compound Name	Response	Retention Time
DDT	473989	13.369
DDD	5147	13.063
DDE	366	12.727
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5513	479502	1.15

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP