
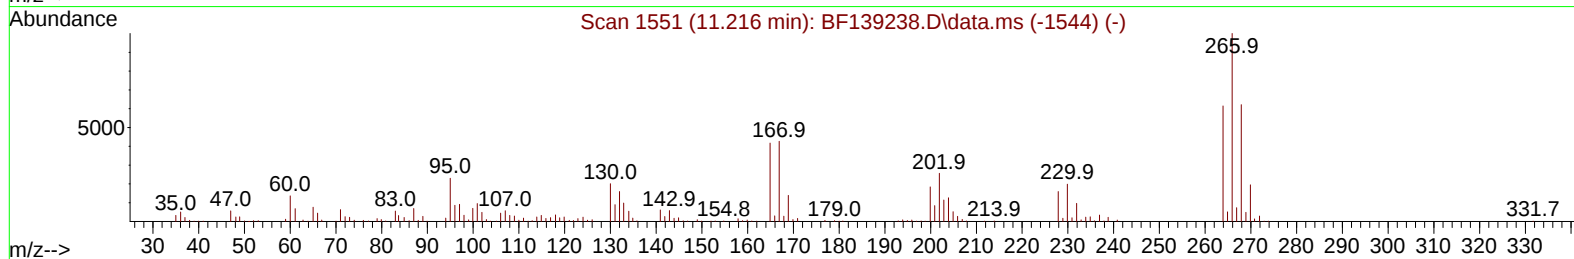
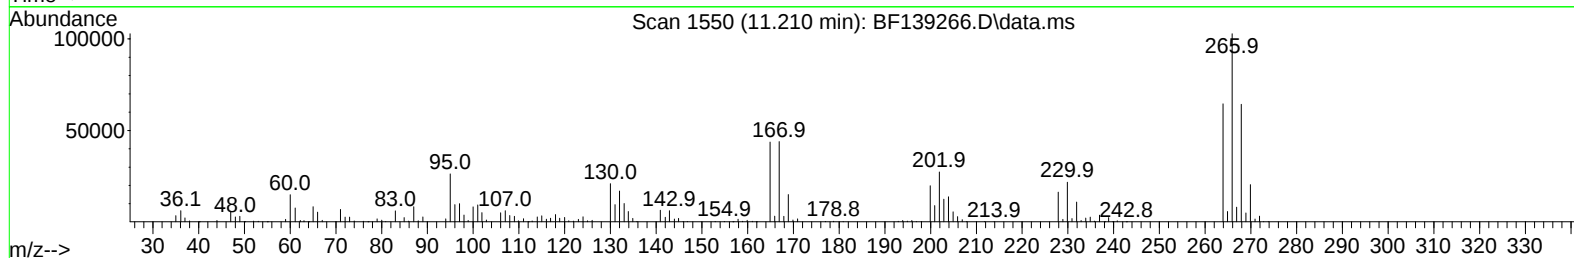


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090624\
Data File : BF139266.D
Acq On : 06 Sep 2024 08:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 06 10:37:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 16:11:43 2024
Response via : Initial Calibration

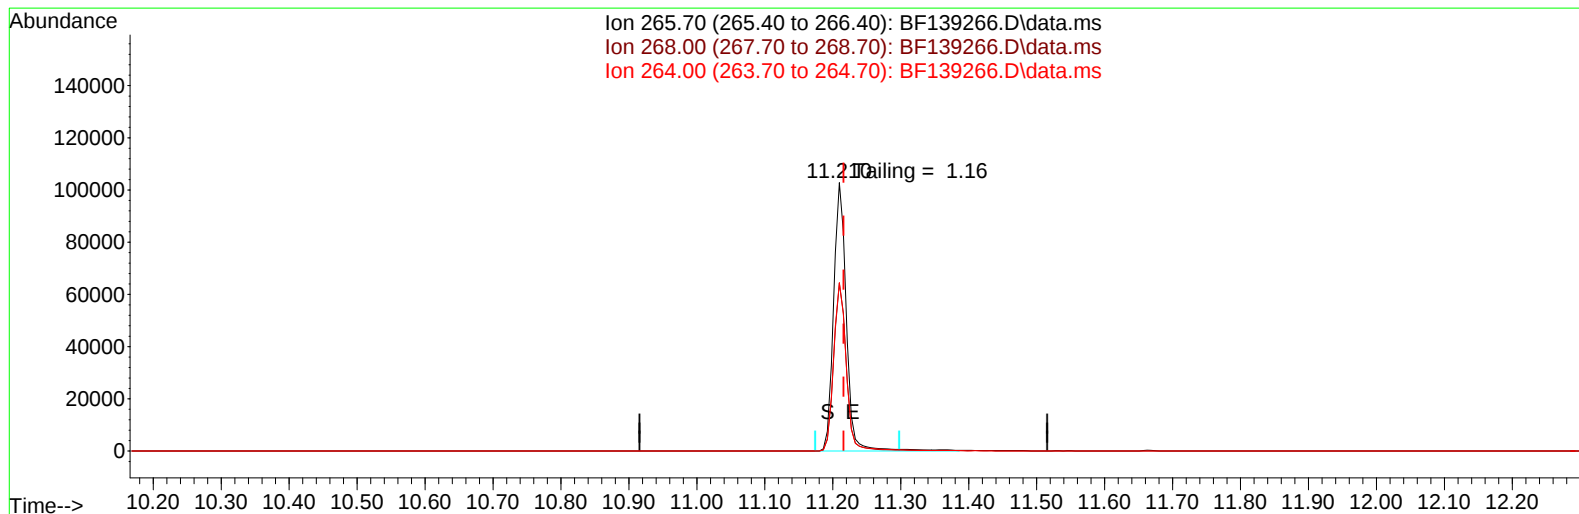

TIC: BF139266.D\data.ms

(70) Pentachlorophenol (C)




11.210min (-0.006) 122473.46 ng

response 132798

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.10	62.50
264.00	61.50	62.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090624\
Data File : BF139266.D
Acq On : 06 Sep 2024 08:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 06 10:37:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 16:11:43 2024
Response via : Initial Calibration

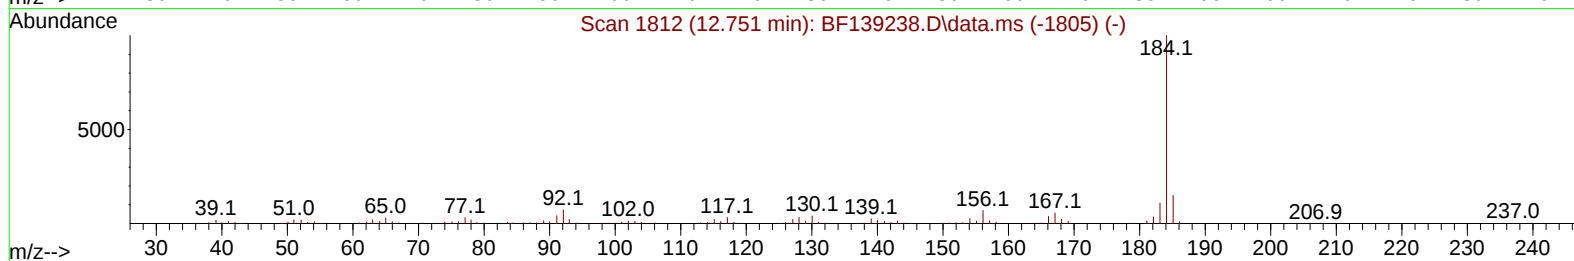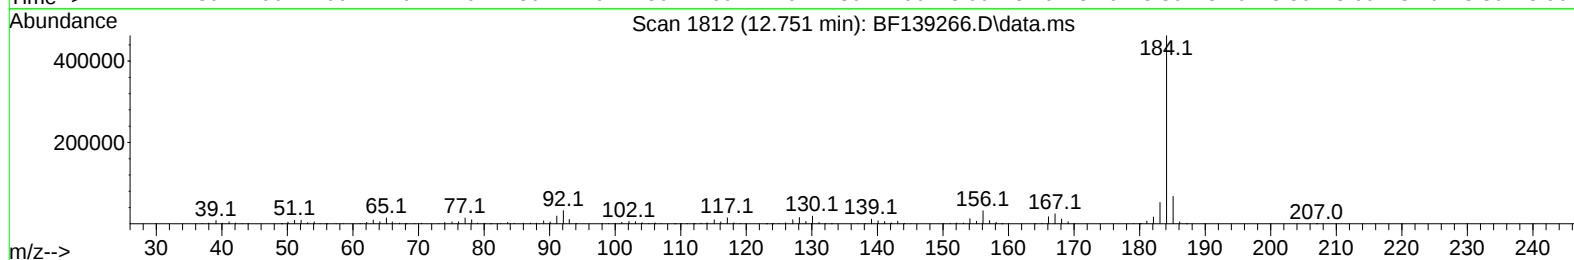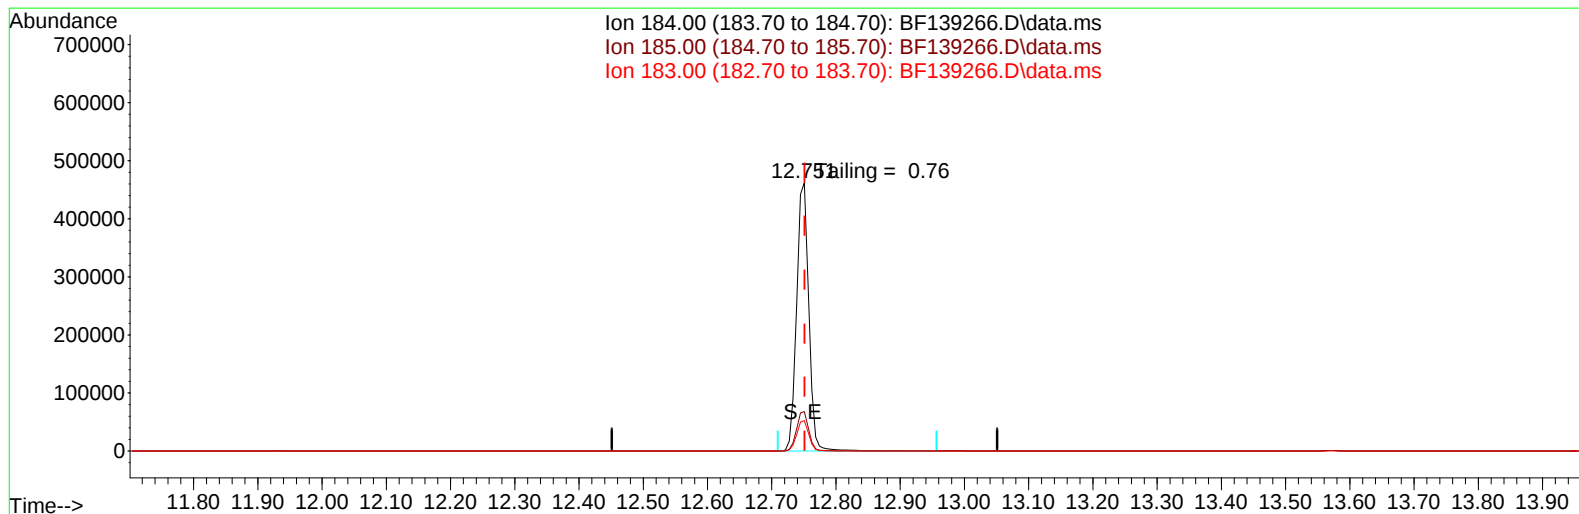

TIC: BF139266.D\data.ms

(77) Benzidine

12.751min (-0.000) 18958.26 ng

response 611916

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.66
183.00	11.00	11.36
0.00	0.00	0.00