
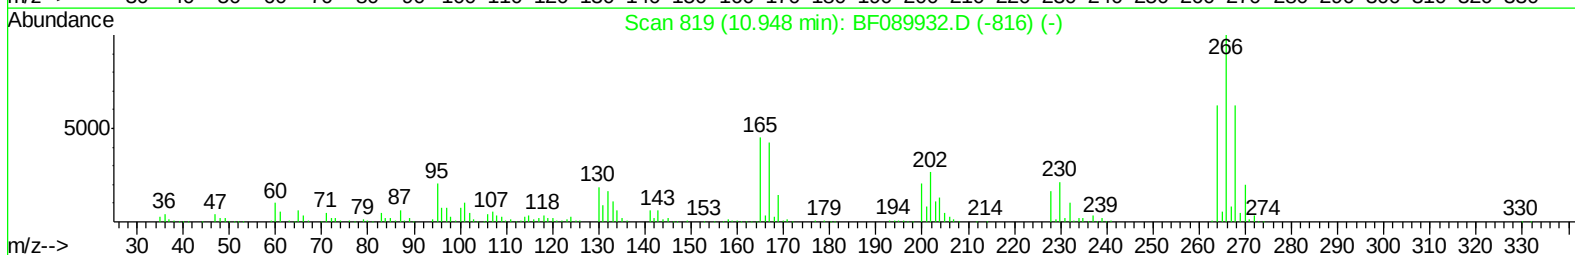
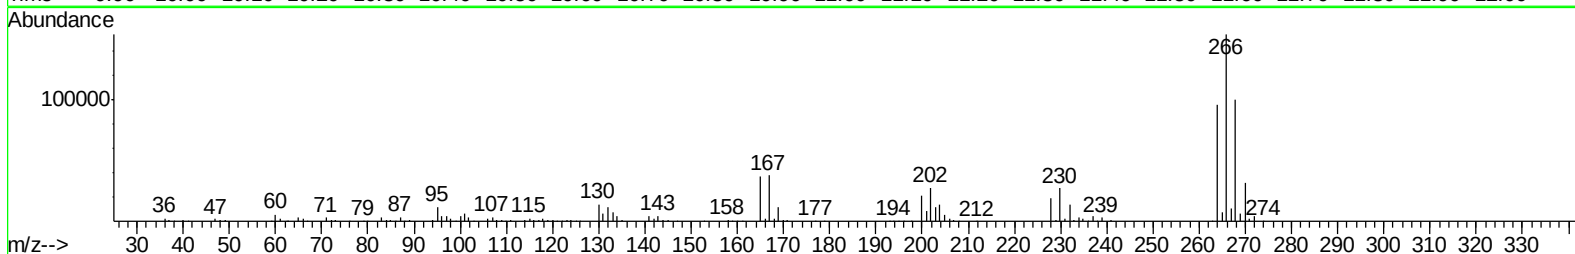


Data Path : Z:\HPCHEM1\BNA F\DATA\BF090716\
Data File : BF089995.D
Acq On : 7 Sep 2016 8:44
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 07 19:07:12 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 02 13:29:08 2016
Response via : Initial Calibration

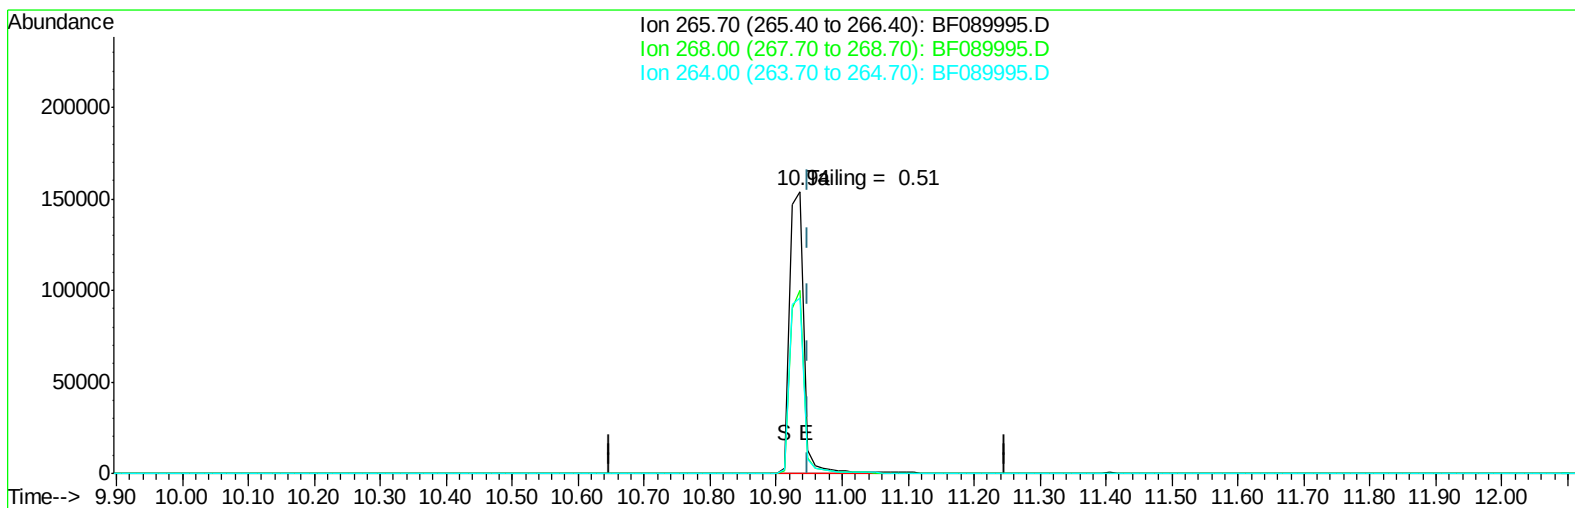

TIC: BF089995.D

(69) Pentachlorophenol (C)




10.936min (-0.011) 39769.15ng

response 228074

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	65.11
264.00	63.20	62.47
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF090716\
Data File : BF089995.D
Acq On : 7 Sep 2016 8:44
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 07 19:07:12 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 02 13:29:08 2016
Response via : Initial Calibration

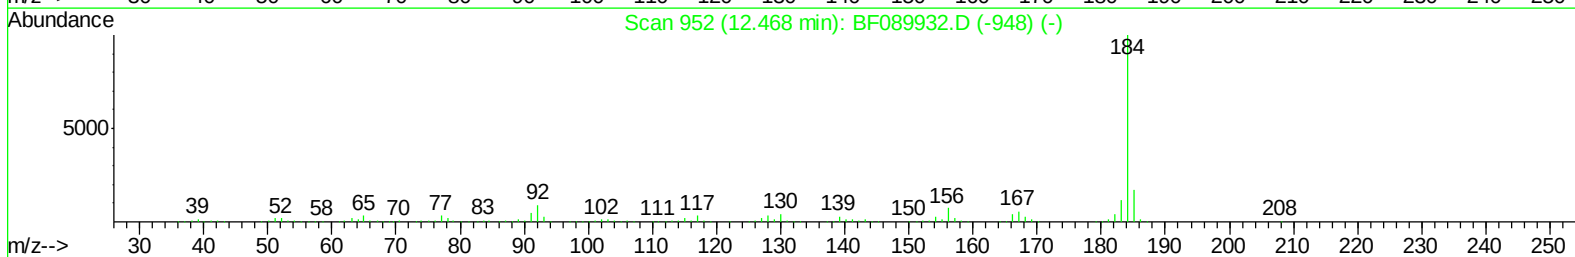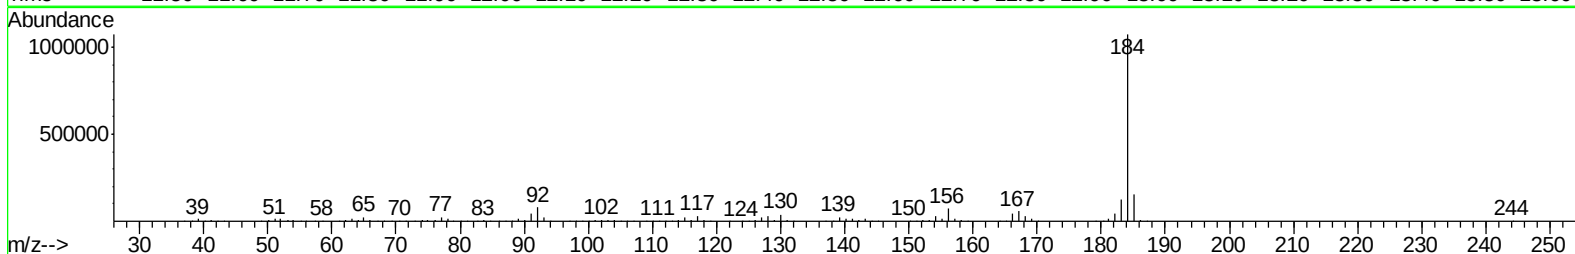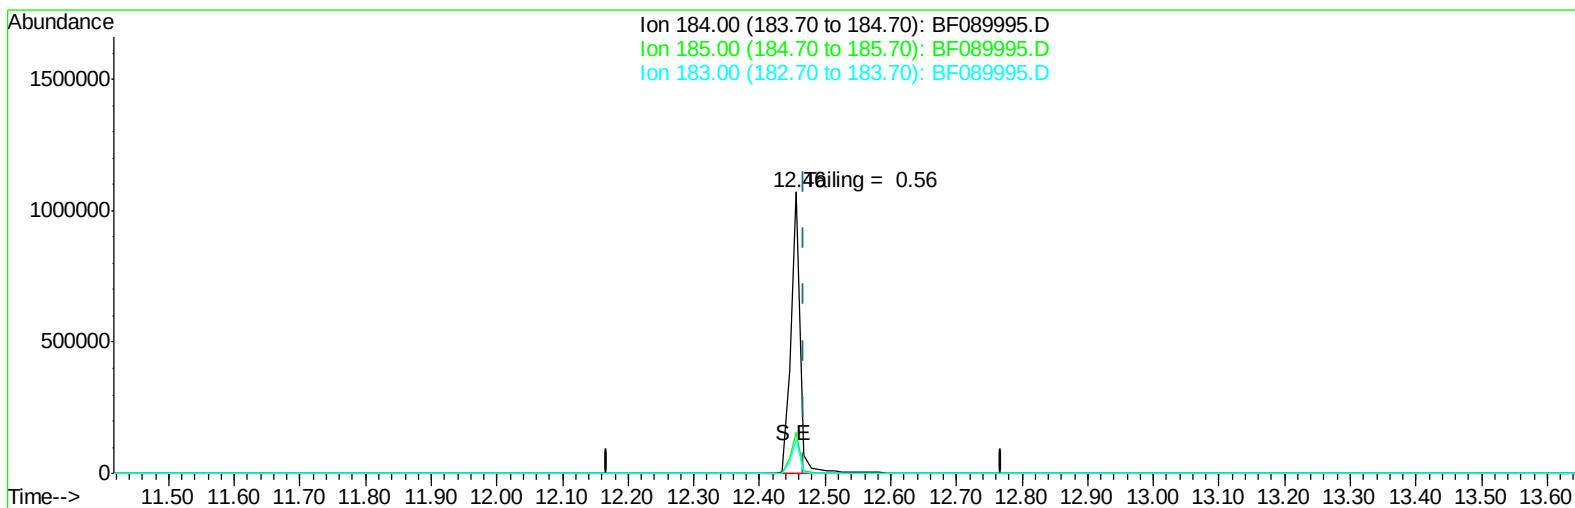

TIC: BF089995.D

(76) Benzidine

12.456min (-0.011) 19975.41ng

response 1115421

Ion	Exp%	Act%
184.00	100	100
185.00	17.30	14.41
183.00	12.00	12.02
0.00	0.00	0.00