


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF090716\
 Data File : BF089995.D
 Acq On : 7 Sep 2016 8:44
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF083116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 02 13:29:08 2016

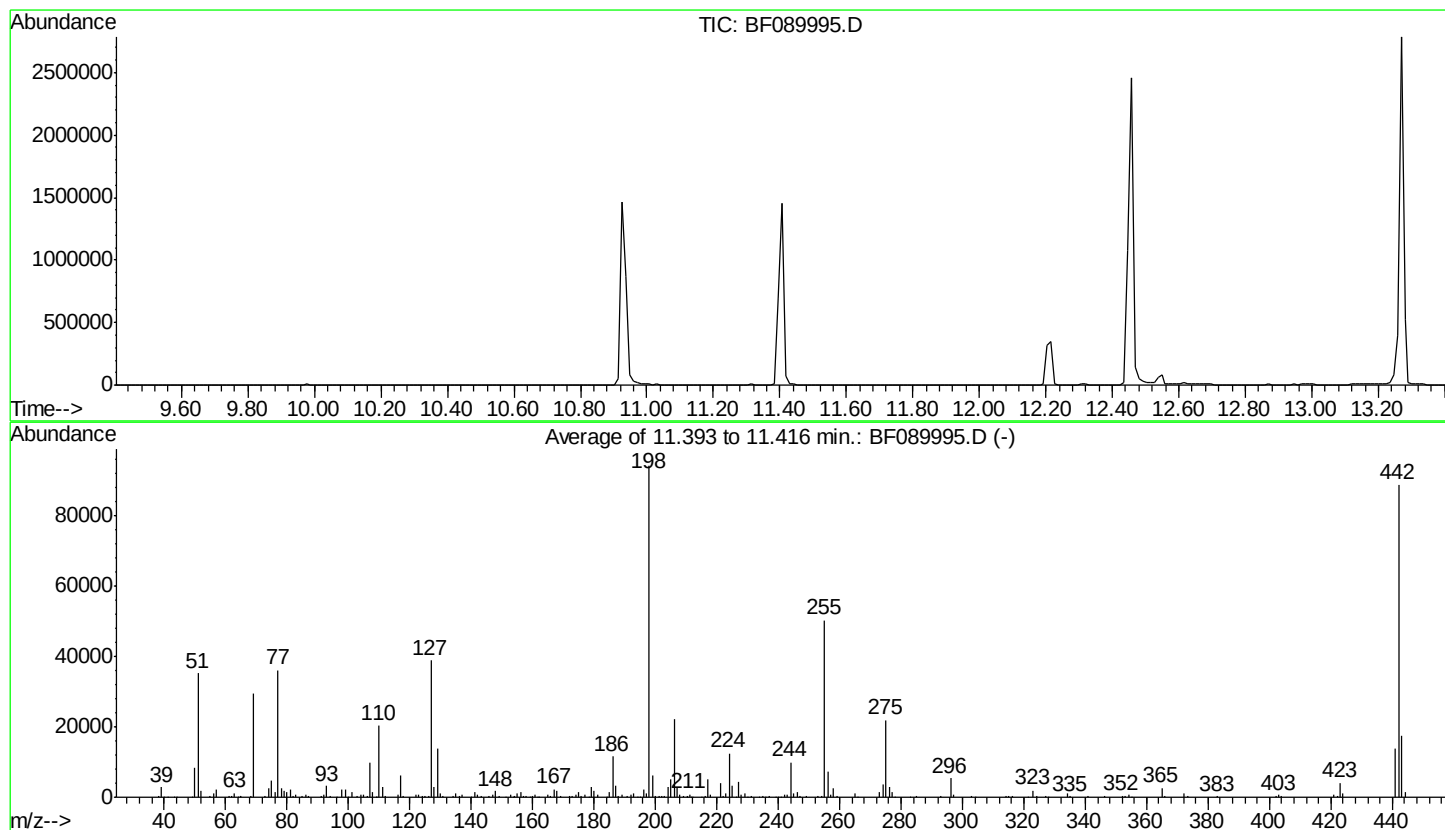

AutoFind: Scans 858, 859, 860; Background Corrected with Scan 854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	35159	PASS
68	69	0.00	2	1.5	426	PASS
69	198	0.00	100	31.1	29331	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.2	38828	PASS
197	198	0.00	2	1.2	1105	PASS
198	198	100	100	100.0	94169	PASS
199	198	5	9	6.7	6267	PASS
275	198	10	60	23.2	21852	PASS
365	198	1	100	2.7	2560	PASS
441	442	0.01	24	15.7	13911	PASS
442	198	50	100	94.2	88727	PASS
443	442	15	24	19.7	17435	PASS