
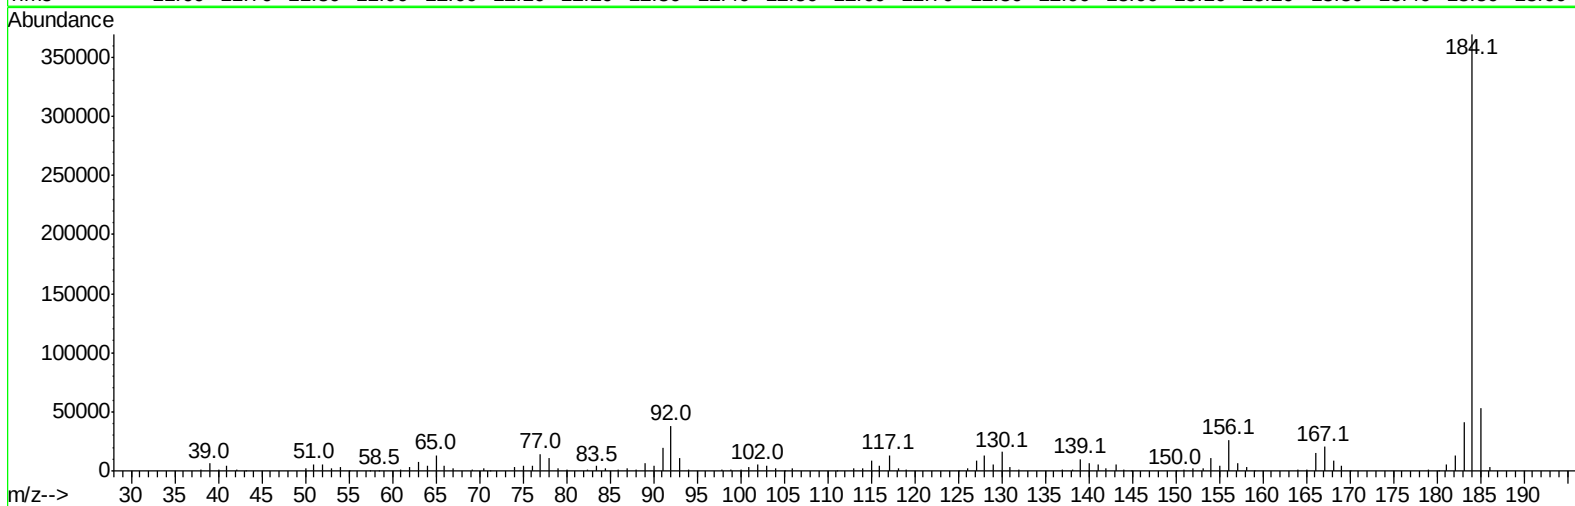


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF090717\
 Data File : BF098311.D
 Acq On : 7 Sep 2017 13:30
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 08 07:34:00 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 05 17:28:20 2017
 Response via : Initial Calibration

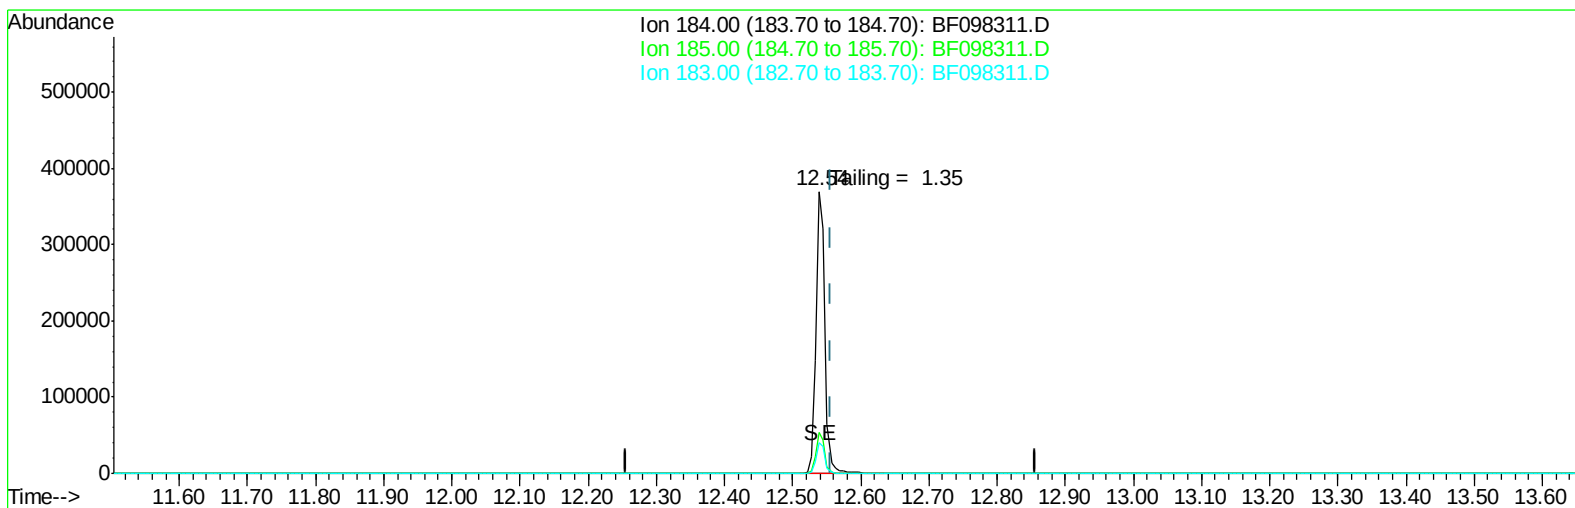

TIC: BF098311.D

(76) Benzidine



12.539min (-0.018) 0.00ng

response 339317

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.41#
183.00	12.20	11.05
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF090717\
Data File : BF098311.D
Acq On : 7 Sep 2017 13:30
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 08 07:34:00 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 05 17:28:20 2017
Response via : Initial Calibration

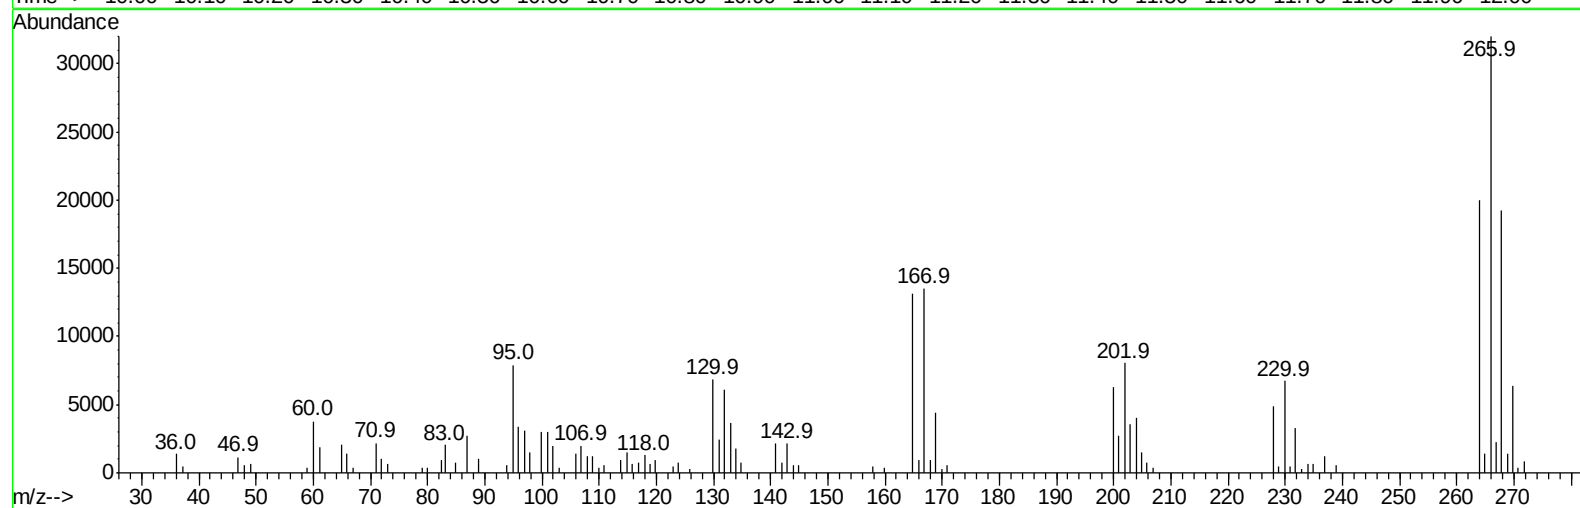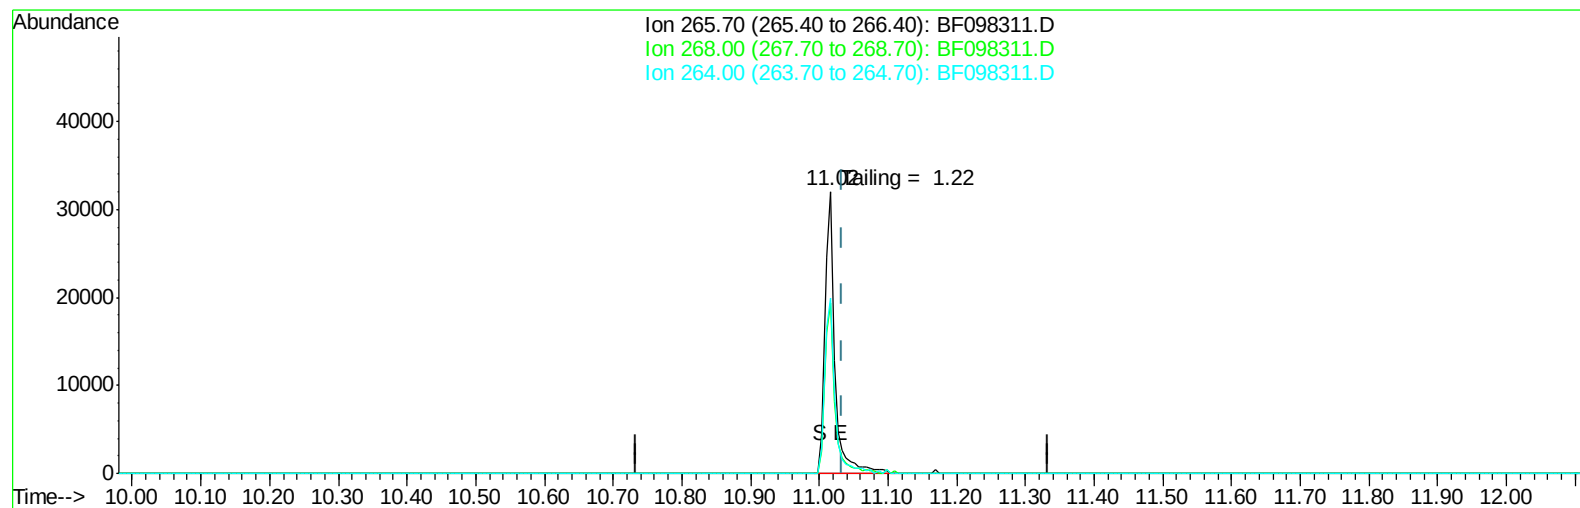

TIC: BF098311.D

(69) Pentachlorophenol (C)

11.016min (-0.018) 18463.85ng

response 31677

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.26
264.00	64.60	62.46
0.00	0.00	0.00