

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF090717\
 Data File : BF098313.D
 Acq On : 7 Sep 2017 15:01
 Operator : SJ/JU
 Sample : I5075-01
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 72-11948

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.251	363	368	376	rVB4	15654	25692	1.47%	0.119%
2	4.793	457	460	463	rVB	21936	24242	1.38%	0.113%
3	4.857	463	471	479	rBV2	118563	178644	10.19%	0.830%
4	5.063	502	506	508	rBV	42025	41780	2.38%	0.194%
5	5.287	540	544	552	rVB	1637831	1599306	91.21%	7.427%
6	5.351	552	555	558	rVB	27140	26026	1.48%	0.121%
7	5.434	565	569	574	rVB3	23545	28655	1.63%	0.133%
8	5.475	574	576	580	rVB	23162	20933	1.19%	0.097%
9	5.581	590	594	599	rVB2	26083	27659	1.58%	0.128%
10	5.692	605	613	616	rBV3	23937	34536	1.97%	0.160%
11	5.828	629	636	641	rVB2	22577	23540	1.34%	0.109%
12	5.928	650	653	659	rBV3	27217	35028	2.00%	0.163%
13	5.981	659	662	665	rBV	22112	21873	1.25%	0.102%
14	6.116	680	685	688	rBV4	16126	21528	1.23%	0.100%
15	6.210	698	701	704	rBV3	30099	31413	1.79%	0.146%
16	6.328	717	721	728	rBV	1768813	1753350	100.00%	8.142%
17	6.428	733	738	739	rBV3	14646	23864	1.36%	0.111%
18	6.457	739	743	746	rVV	1882605	1653254	94.29%	7.678%
19	6.522	750	754	759	rBV4	46721	54294	3.10%	0.252%
20	6.686	778	782	788	rVB	864319	757712	43.22%	3.519%
21	6.745	788	792	795	rBV2	23775	26388	1.51%	0.123%
22	6.839	804	808	811	rBV	1439748	1227155	69.99%	5.699%
23	6.869	811	813	816	rVB	29053	23490	1.34%	0.109%
24	6.963	825	829	832	rVB3	30016	46683	2.66%	0.217%
25	7.028	838	840	844	rBV2	21485	23745	1.35%	0.110%
26	7.075	846	848	851	rBV3	40333	39137	2.23%	0.182%
27	7.210	867	871	872	rBV2	26339	26015	1.48%	0.121%
28	7.251	874	878	881	rVV	1200284	1041084	59.38%	4.835%
29	7.286	881	884	887	rVB	76132	75413	4.30%	0.350%
30	7.339	887	893	895	rBV4	32410	50770	2.90%	0.236%
31	7.363	895	897	901	rBV2	36745	45120	2.57%	0.210%
32	7.475	913	916	917	rBV2	26197	23971	1.37%	0.111%
33	7.492	917	919	922	rVB2	57894	45583	2.60%	0.212%
34	7.604	935	938	943	rVB7	50515	62841	3.58%	0.292%

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF090717\
 Data File : BF098313.D
 Acq On : 7 Sep 2017 15:01
 Operator : SJ/JU
 Sample : I5075-01
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 72-11948

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	7.657	943	947	949	rBV3	23874	29451	1.68%	0.137%
36	7.728	954	959	962	rVB6	35834	44861	2.56%	0.208%
37	7.792	968	970	974	rVB3	30189	30313	1.73%	0.141%
38	7.857	974	981	983	rBV3	40578	65149	3.72%	0.303%
39	7.875	983	984	988	rVB3	28867	22593	1.29%	0.105%
40	7.969	994	1000	1003	rBV	1150207	1021949	58.29%	4.746%
41	8.039	1010	1012	1014	rVB	59951	44500	2.54%	0.207%
42	8.063	1014	1016	1019	rBV3	19849	23257	1.33%	0.108%
43	8.139	1026	1029	1032	rBV4	20245	25813	1.47%	0.120%
44	8.175	1032	1035	1038	rVB2	53491	43222	2.47%	0.201%
45	8.263	1045	1050	1053	rBV6	41561	62425	3.56%	0.290%
46	8.322	1057	1060	1062	rBV3	41570	43454	2.48%	0.202%
47	8.351	1063	1065	1069	rVB4	35123	36178	2.06%	0.168%
48	8.398	1069	1073	1075	rBV	105159	110690	6.31%	0.514%
49	8.475	1083	1086	1089	rBV3	27243	25186	1.44%	0.117%
50	8.510	1089	1092	1094	rBV3	44065	40550	2.31%	0.188%
51	8.569	1099	1102	1104	rBV2	75207	62660	3.57%	0.291%
52	8.657	1115	1117	1120	rVB2	23681	25895	1.48%	0.120%
53	8.680	1120	1121	1124	rVB	32727	22739	1.30%	0.106%
54	8.710	1124	1126	1130	rBV4	15072	21634	1.23%	0.100%
55	8.780	1136	1138	1144	rVB5	31553	40479	2.31%	0.188%
56	8.851	1147	1150	1152	rBV3	43232	43259	2.47%	0.201%
57	8.880	1152	1155	1159	rVB5	19186	27849	1.59%	0.129%
58	8.928	1159	1163	1166	rVB5	17397	26697	1.52%	0.124%
59	8.963	1166	1169	1172	rBV3	18841	27489	1.57%	0.128%
60	8.992	1172	1174	1178	rVB2	101862	95030	5.42%	0.441%
61	9.045	1179	1183	1186	rBV	1963157	1724946	98.38%	8.010%
62	9.127	1192	1197	1202	rBV3	92120	132308	7.55%	0.614%
63	9.175	1202	1205	1207	rBV4	19658	25101	1.43%	0.117%
64	9.357	1232	1236	1238	rBV5	25258	32206	1.84%	0.150%
65	9.445	1246	1251	1254	rBV2	325768	336300	19.18%	1.562%
66	9.475	1254	1256	1259	rVB3	27042	27015	1.54%	0.125%
67	9.539	1264	1267	1272	rVB5	22668	30092	1.72%	0.140%
68	9.592	1272	1276	1279	rBV5	25860	41365	2.36%	0.192%
69	9.633	1280	1283	1285	rVB2	43780	40560	2.31%	0.188%
70	9.657	1285	1287	1292	rBV2	44856	49889	2.85%	0.232%
71	9.722	1292	1298	1301	rBV2	1140550	1020987	58.23%	4.741%

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF090717\
 Data File : BF098313.D
 Acq On : 7 Sep 2017 15:01
 Operator : SJ/JU
 Sample : I5075-01
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 72-11948

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	9.751	1301	1303	1307	rVB2	43080	41129	2.35%	0.191%
73	9.927	1330	1333	1338	rVB3	56555	76836	4.38%	0.357%
74	9.980	1340	1342	1350	rVB6	32115	42566	2.43%	0.198%
75	10.127	1364	1367	1369	rBV4	33765	33042	1.88%	0.153%
76	10.157	1370	1372	1375	rVB	37239	32969	1.88%	0.153%
77	10.269	1388	1391	1398	rBV3	43409	58172	3.32%	0.270%
78	10.380	1407	1410	1415	rVB	73820	85190	4.86%	0.396%
79	10.510	1427	1432	1435	rBV	1057420	950879	54.23%	4.416%
80	10.645	1450	1455	1462	rVB	133045	181758	10.37%	0.844%
81	11.080	1526	1529	1531	rBV2	42341	42486	2.42%	0.197%
82	11.104	1531	1533	1537	rVB2	93135	98416	5.61%	0.457%
83	11.204	1546	1550	1553	rBV	997577	888168	50.66%	4.125%
84	11.227	1553	1554	1557	rVB	110617	58892	3.36%	0.273%
85	11.439	1587	1590	1592	rBV2	64020	73745	4.21%	0.342%
86	11.504	1599	1601	1603	rVB	29663	20093	1.15%	0.093%
87	11.733	1638	1640	1644	rVB2	34827	41541	2.37%	0.193%
88	11.886	1663	1666	1668	rBV4	28412	37021	2.11%	0.172%
89	12.257	1726	1729	1731	rBV2	39043	36890	2.10%	0.171%
90	12.416	1753	1756	1759	rVB	90415	83206	4.75%	0.386%
91	12.639	1792	1794	1797	rVB	114156	90556	5.16%	0.421%
92	12.786	1813	1819	1828	rVB	1418758	1663449	94.87%	7.725%
93	13.651	1960	1966	1970	rBV2	155343	347936	19.84%	1.616%
94	13.692	1970	1973	1980	rVB4	153963	205081	11.70%	0.952%
95	13.839	1994	1998	2001	rBV	771390	693037	39.53%	3.218%
96	14.268	2067	2071	2076	rBV	170545	328379	18.73%	1.525%
97	15.251	2234	2238	2245	rVB	520183	657440	37.50%	3.053%


Sum of corrected areas: 21533692

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF090717\
Data File : BF098313.D
Acq On : 7 Sep 2017 15:01
Operator : SJ/JU
Sample : I5075-01
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
72-11948

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

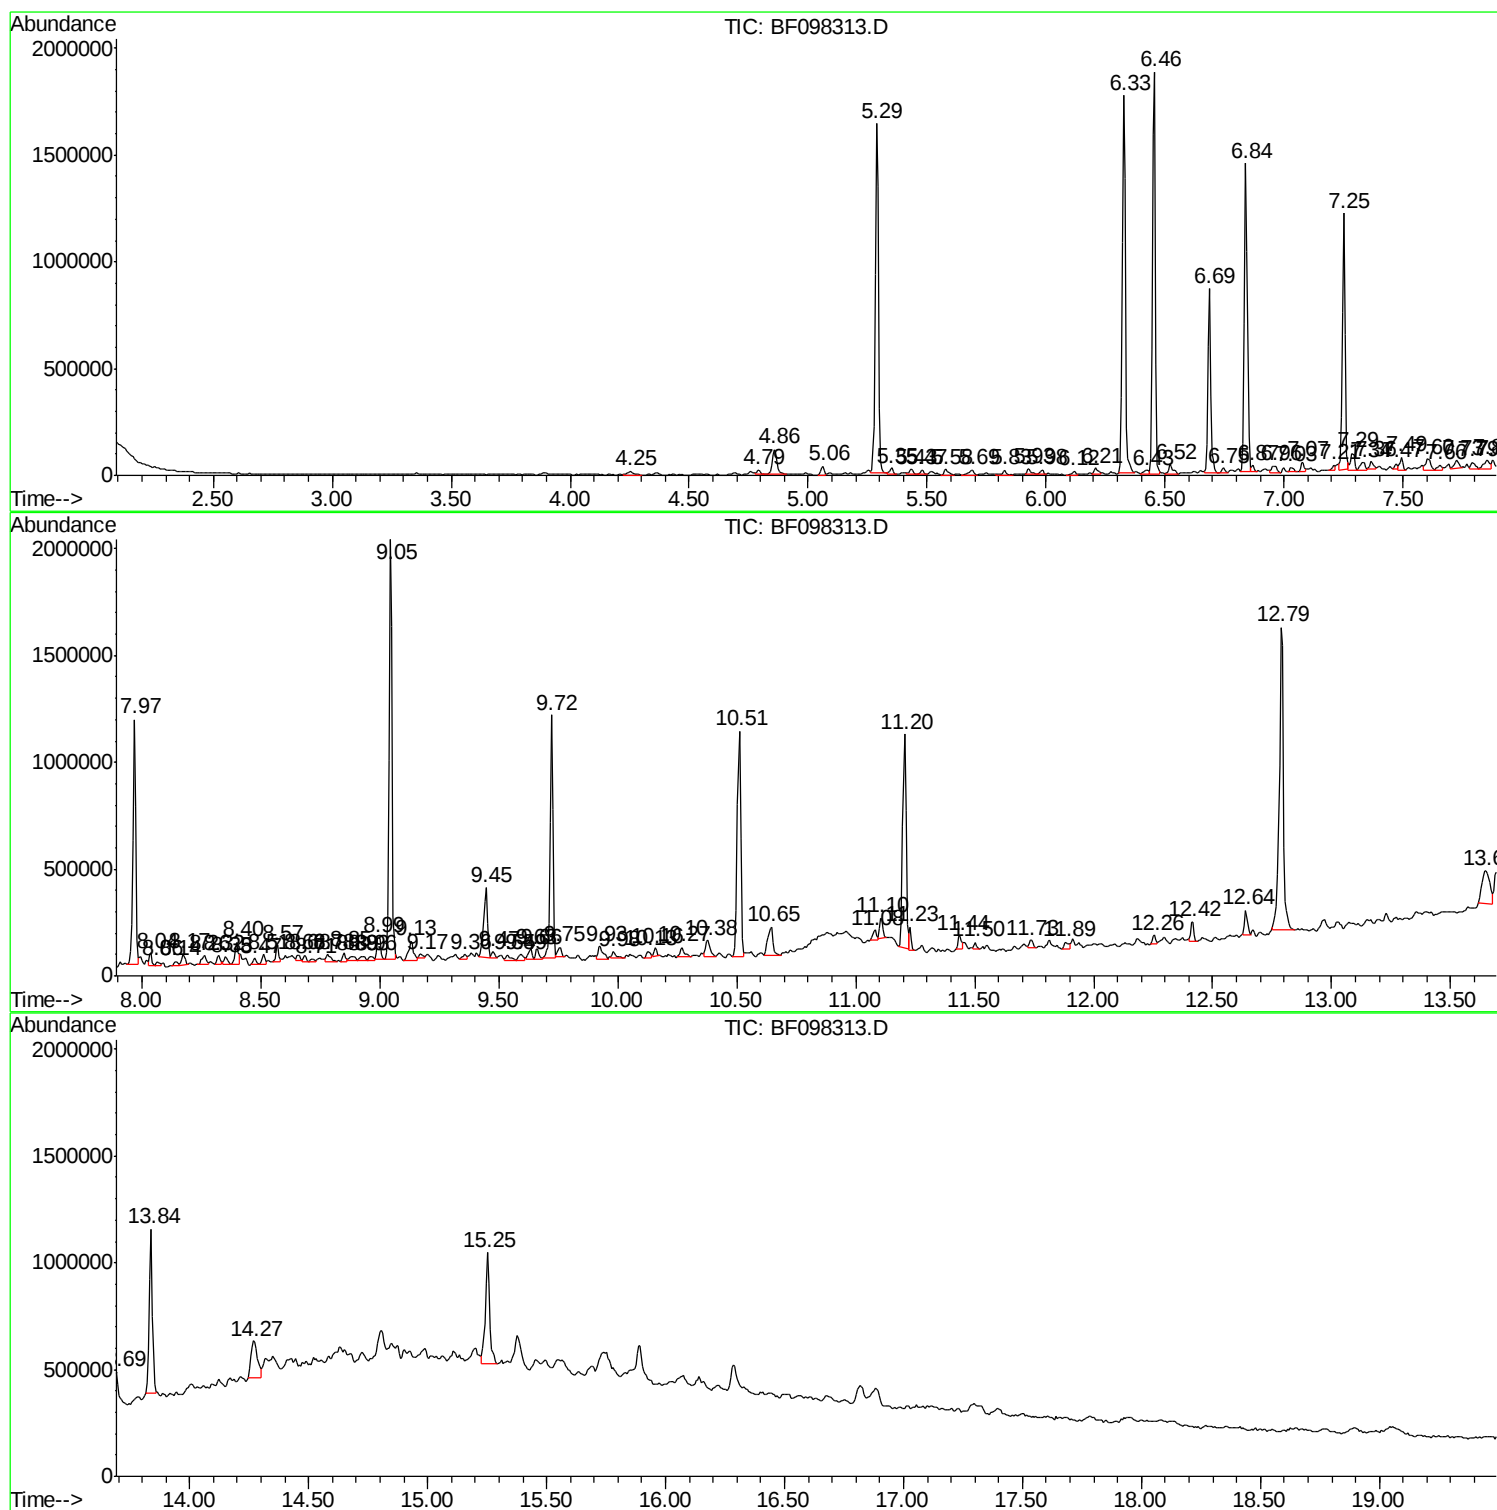

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF090717\
Data File : BF098313.D
Acq On : 7 Sep 2017 15:01
Operator : SJ/JU
Sample : I5075-01
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
72-11948










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown4.866 Concentration Rank 6

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.86	4.72 ng	178644	1,4-Dichlorobenzene-d4	6.69

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	37
2			3-Hexanol, 4,4-dimethyl-	130	C8H18O	019550-09-5	37
3			Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	36
4			2-Octanol, 2,6-dimethyl-	158	C10H22O	018479-57-7	25
5			n-Propyl t-butyl ether	116	C7H16O	1000334-81-9	25

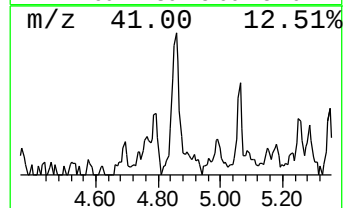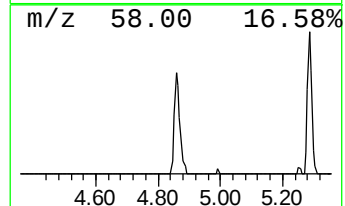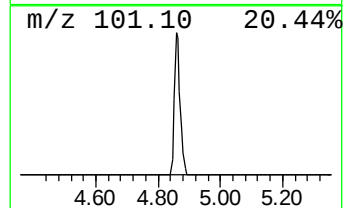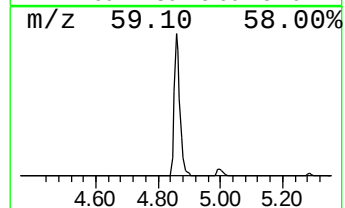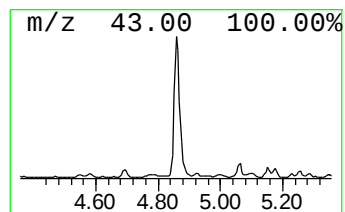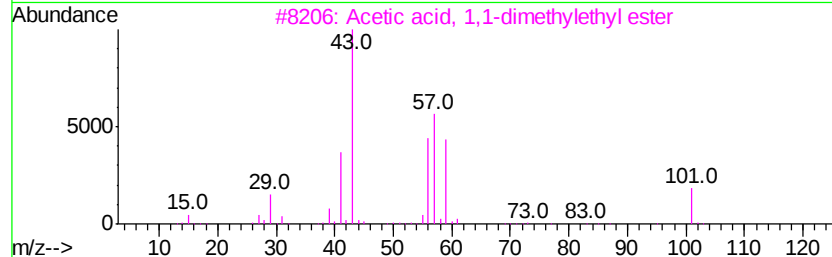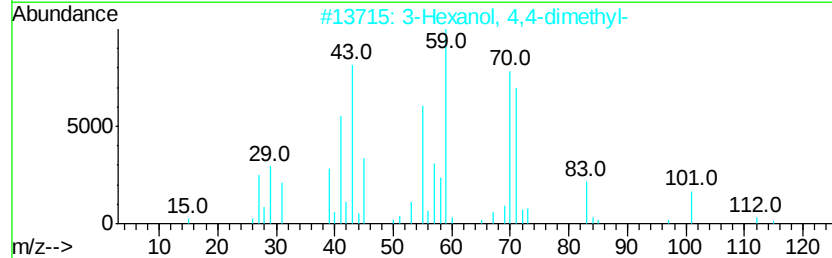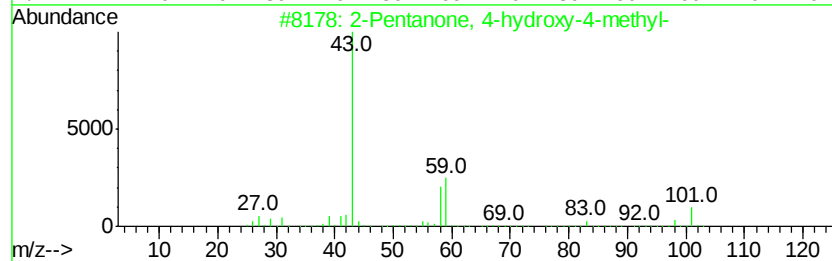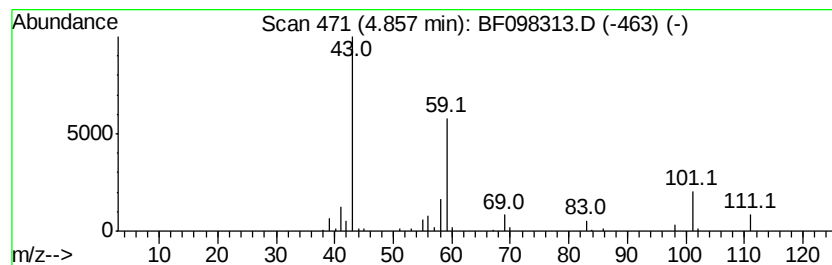

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF090717\
Data File : BF098313.D
Acq On : 7 Sep 2017 15:01
Operator : SJ/JU
Sample : I5075-01
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
72-11948










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.46 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.46	43.64 ng	1653250	1,4-Dichlorobenzene-d4	6.69

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
2		1,2,4-Trifluorobenzene	132	C6H3F3	000367-23-7	9
3		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9
4		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

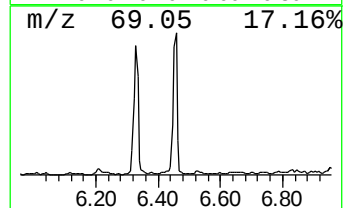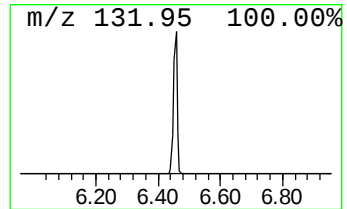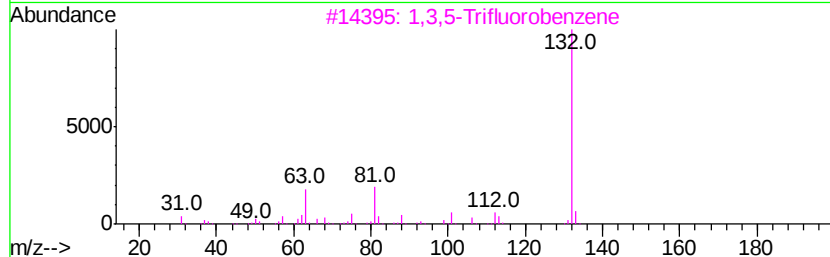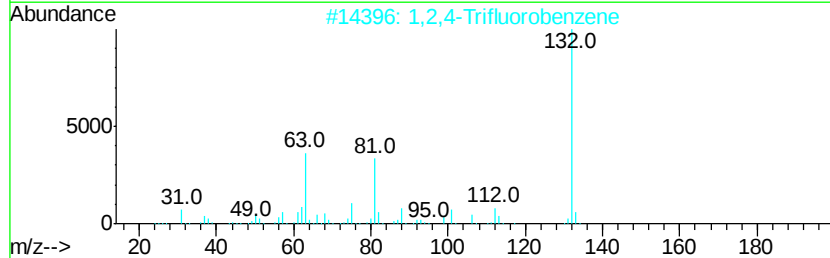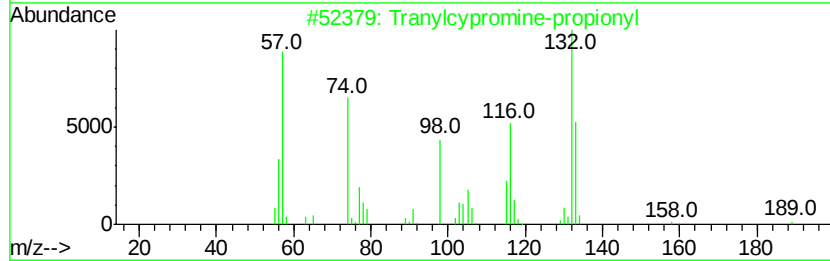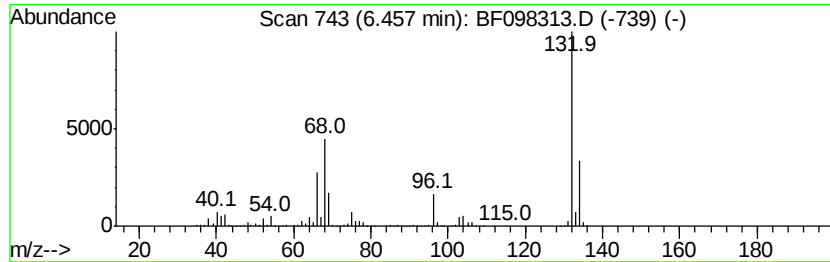

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF090717\
Data File : BF098313.D
Acq On : 7 Sep 2017 15:01
Operator : SJ/JU
Sample : I5075-01
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
72-11948










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 Dodecane, 2,7,10-trimethyl- Concentration Rank 10

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.40	2.17 ng	110690	Napthalene-d8	7.97

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Dodecane, 2,7,10-trimethyl-	212	C15H32	074645-98-0	86
2		Octane, 2,6-dimethyl-	142	C10H22	002051-30-1	86
3		Sulfurous acid, 2-ethylhexyl und...	348	C19H40O3S	1000309-19-4	64
4		Sulfurous acid, 2-ethylhexyl pen...	264	C13H28O3S	1000309-18-9	53
5		Octane, 2-bromo-	192	C8H17Br	000557-35-7	53

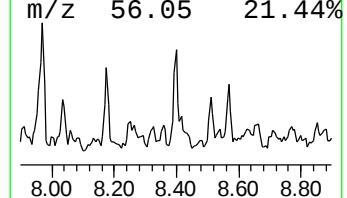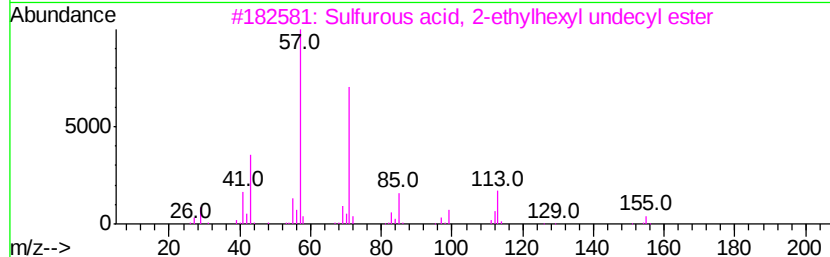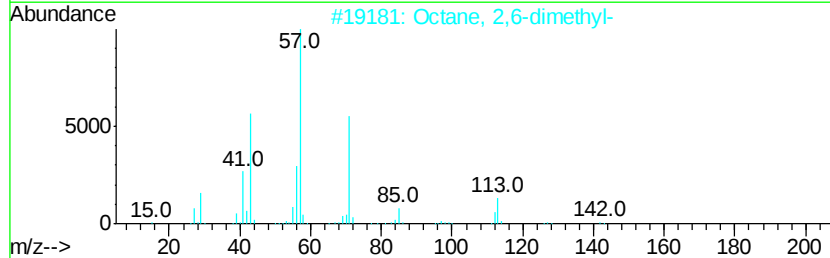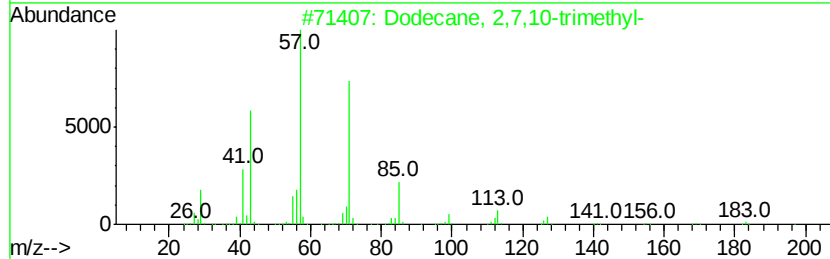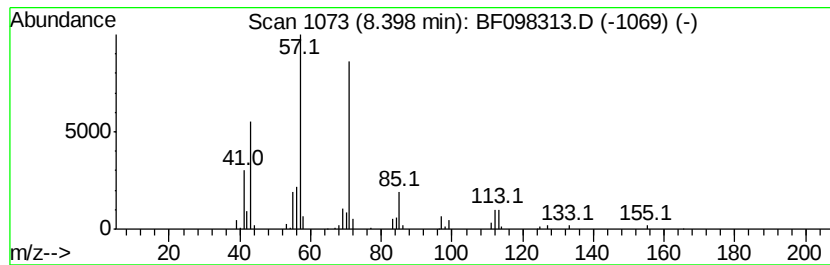

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF090717\
Data File : BF098313.D
Acq On : 7 Sep 2017 15:01
Operator : SJ/JU
Sample : I5075-01
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
72-11948










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 5 Tetracontane, 3,5,24-trimet... Concentration Rank 8

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.13	2.59 ng	132308	Acenaphthene-d10	9.72

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetracontane, 3,5,24-trimethyl-	605	C43H88	055162-61-3	80
2			Octadecane, 1-chloro-	288	C18H37Cl	003386-33-2	80
3			Dodecane	170	C12H26	000112-40-3	64
4			Hexadecane	226	C16H34	000544-76-3	64
5			Decane, 2,3,5,8-tetramethyl-	198	C14H30	192823-15-7	64

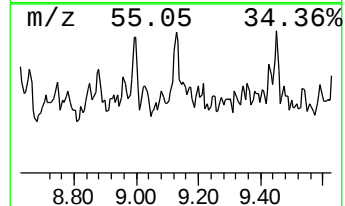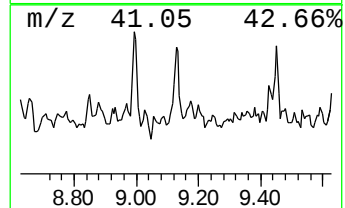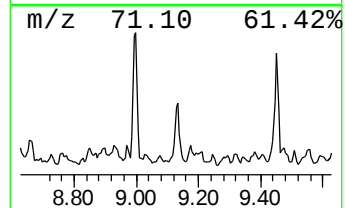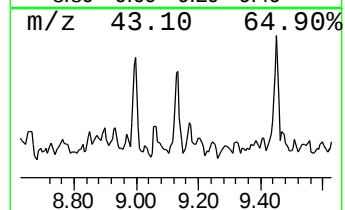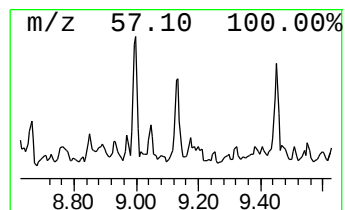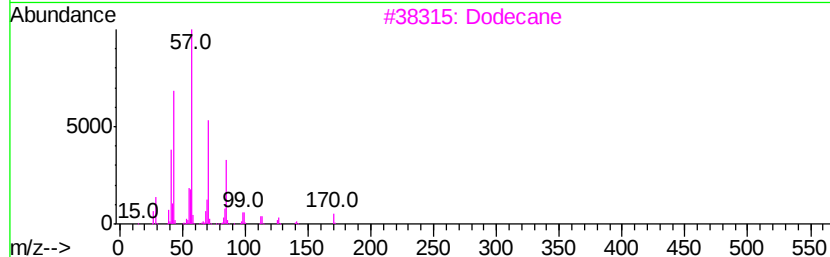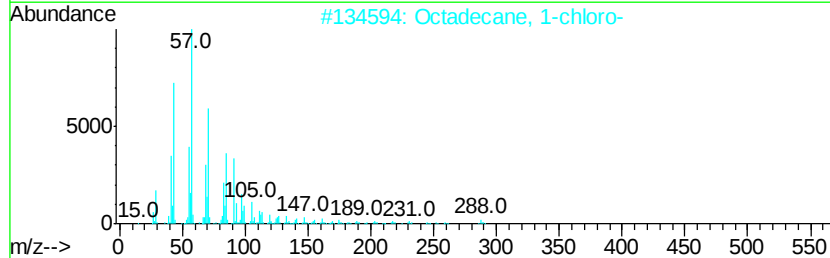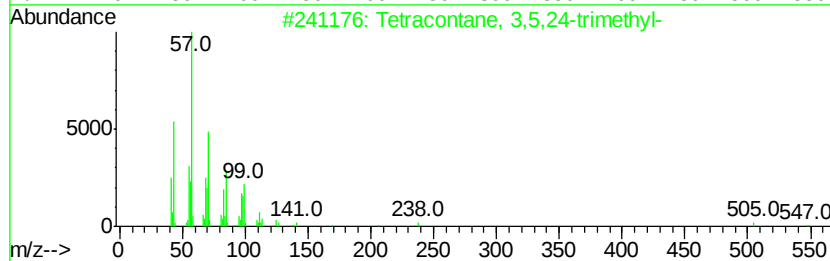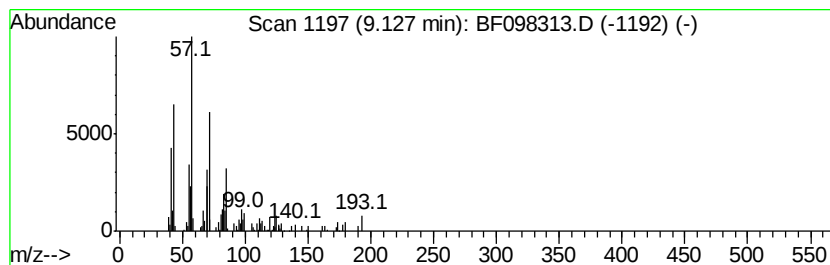

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF090717\
Data File : BF098313.D
Acq On : 7 Sep 2017 15:01
Operator : SJ/JU
Sample : I5075-01
Misc :
ALS Vial : 3 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
72-11948

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 6 Tridecane, 5-propyl- Concentration Rank 7

R.T.	EstConc	Area	Relative to ISTD	R.T.	
10.65	4.09 ng	181758	Phenanthrene-d10	11.20	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Tridecane, 5-propyl-	226	C16H34	055045-11-9	90
2	Hexadecane, 2,6,10,14-tetramethyl-	282	C20H42	000638-36-8	86
3	Dodecane, 2,7,10-trimethyl-	212	C15H32	074645-98-0	80
4	Dodecane, 4,6-dimethyl-	198	C14H30	061141-72-8	78
5	Heptane, 3-ethyl-5-methyl-	142	C10H22	052896-90-9	64

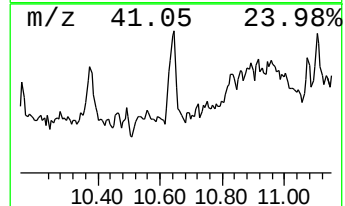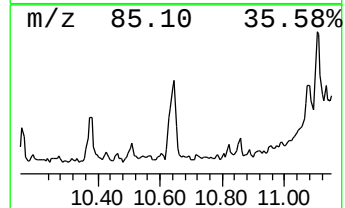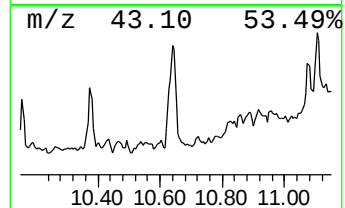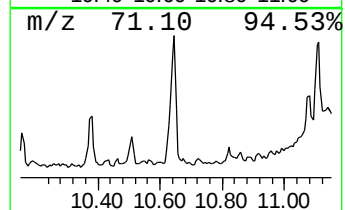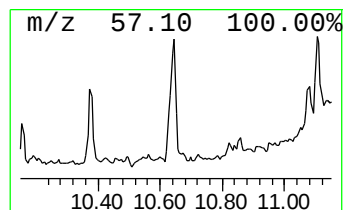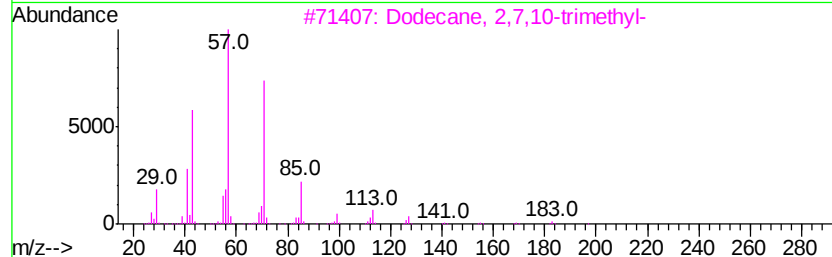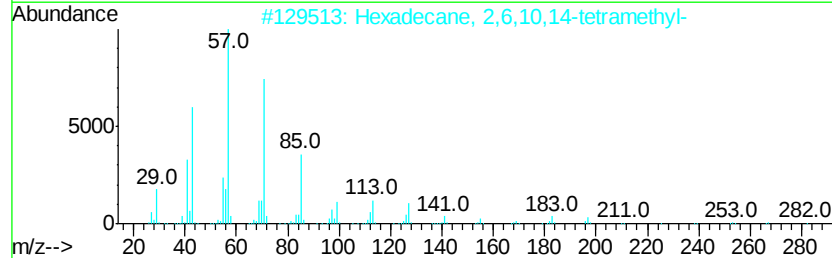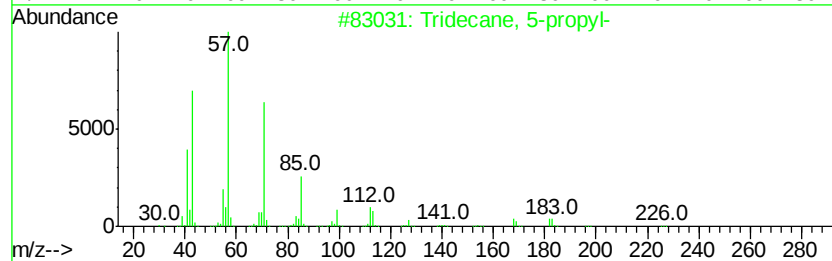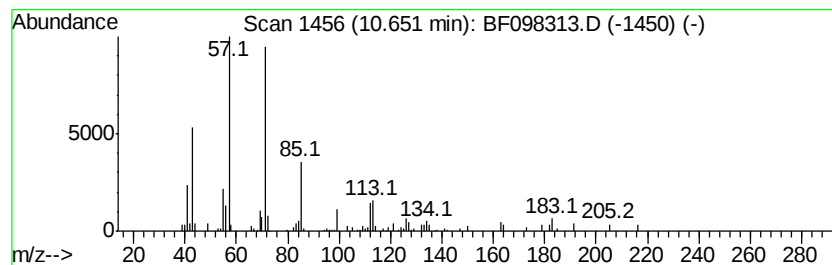

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF090717\
Data File : BF098313.D
Acq On : 7 Sep 2017 15:01
Operator : SJ/JU
Sample : I5075-01
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
72-11948










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 7 Tridecane Concentration Rank 9

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.10	2.22 ng	98416	Phenanthrene-d10	11.20

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Tridecane		184	C13H28	000629-50-5	91
2	Heptadecane		240	C17H36	000629-78-7	80
3	2-Bromo dodecane		248	C12H25Br	013187-99-0	80
4	Octadecane, 1-iodo-		380	C18H37I	000629-93-6	80
5	Undecane, 5-ethyl-5-propyl-		226	C16H34	002755-07-9	78

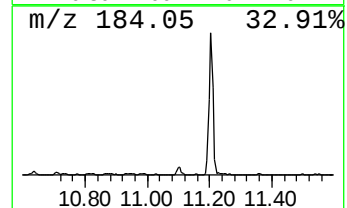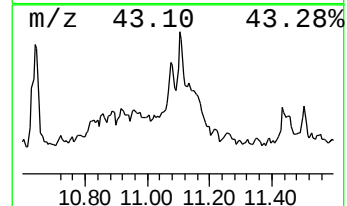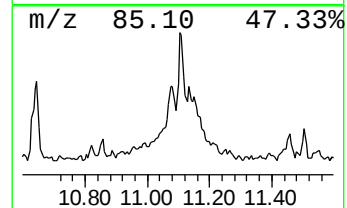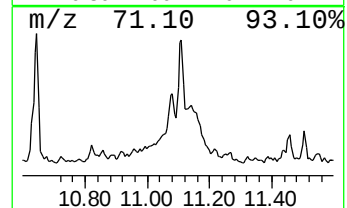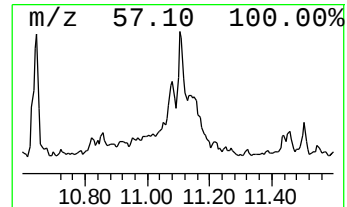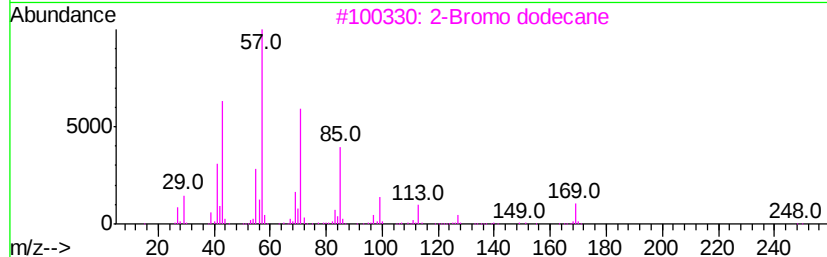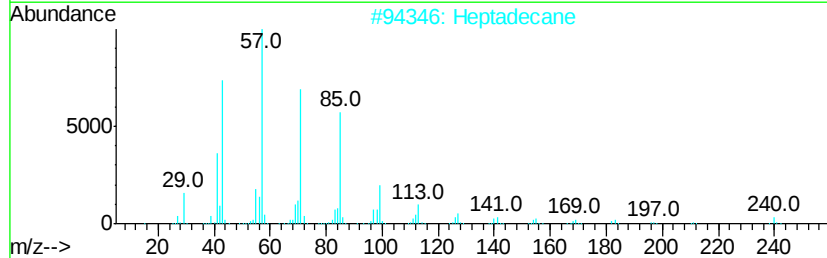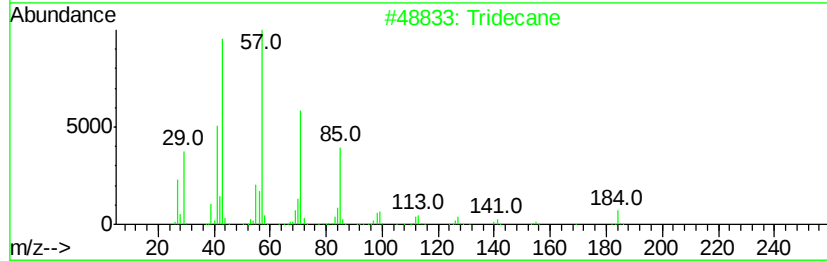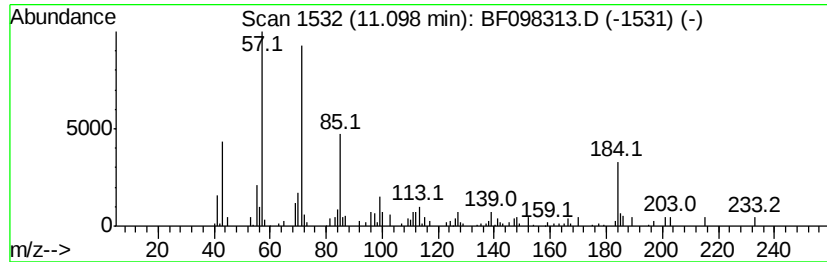

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF090717\
Data File : BF098313.D
Acq On : 7 Sep 2017 15:01
Operator : SJ/JU
Sample : I5075-01
Misc :
ALS Vial : 3 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
72-11948

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 8 Hexadecane Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.	
13.65	10.04 ng	347936	Chrysene-d12	13.84	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Hexadecane	226	C16H34	000544-76-3	86
2	Docosane, 11-butyl-	366	C26H54	013475-76-8	86
3	Octadecane, 1-iodo-	380	C18H37I	000629-93-6	86
4	Nonadecane	268	C19H40	000629-92-5	86
5	Eicosane, 7-hexyl-	366	C26H54	055333-99-8	86

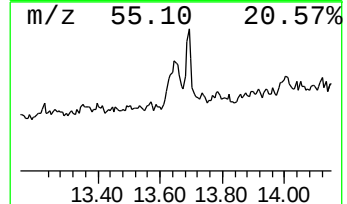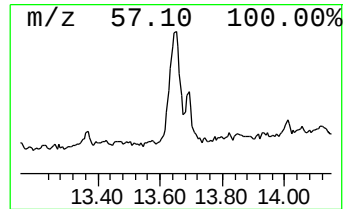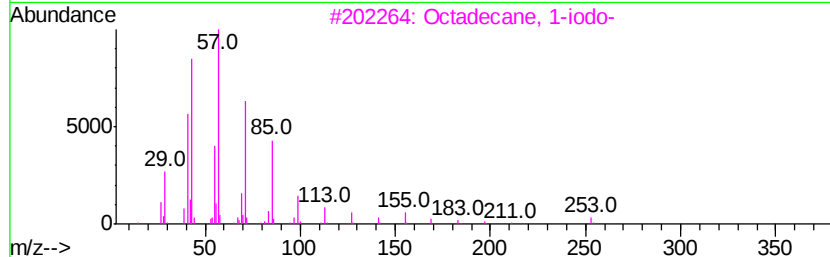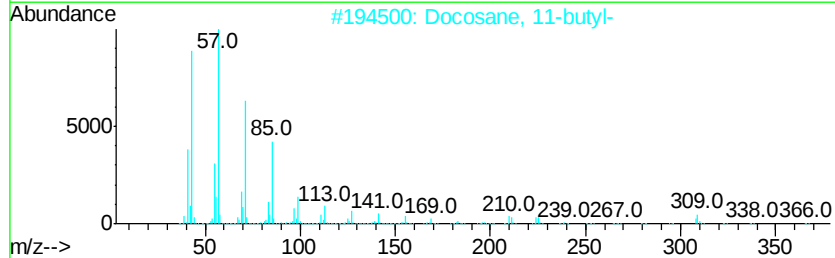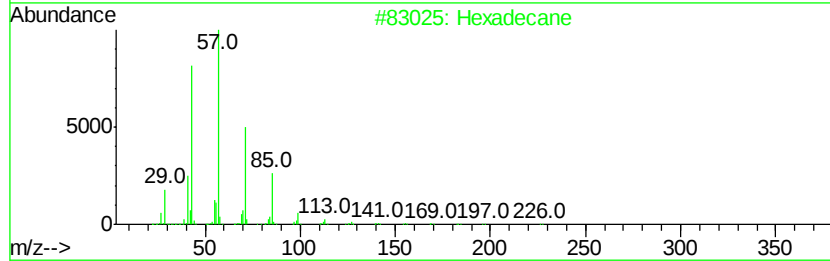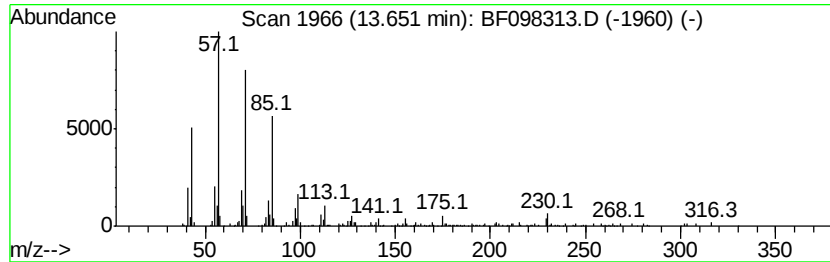

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF090717\
Data File : BF098313.D
Acq On : 7 Sep 2017 15:01
Operator : SJ/JU
Sample : I5075-01
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
72-11948










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 9 Trichloroacetic acid, hexad... Concentration Rank 5

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.69	5.92 ng	205081	Chrysene-d12	13.84

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	72
2		Cyclopentane, decyl-	210	C15H30	001795-21-7	72
3		Cyclopentane, undecyl-	224	C16H32	006785-23-5	64
4		Octacosanol	410	C28H58O	000557-61-9	62
5		Thieno[2,3-d]-1,3-thiaselenol-2-...	238	C5H2S3Se	081803-09-0	53

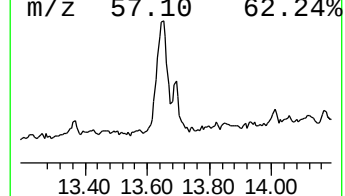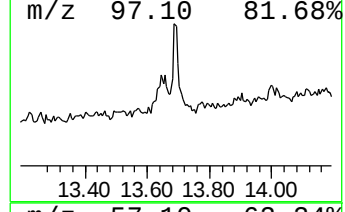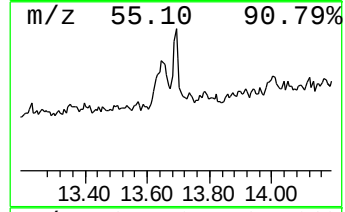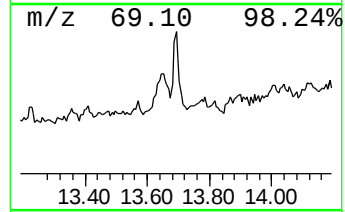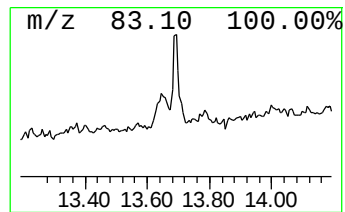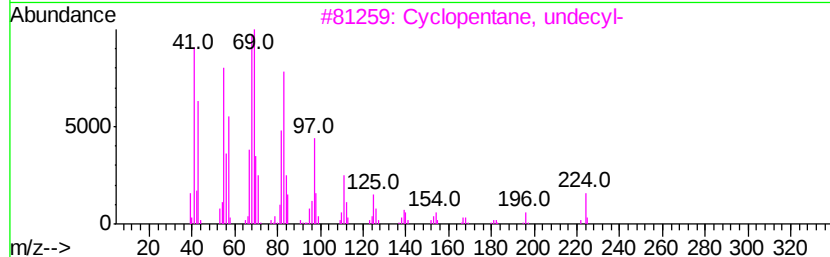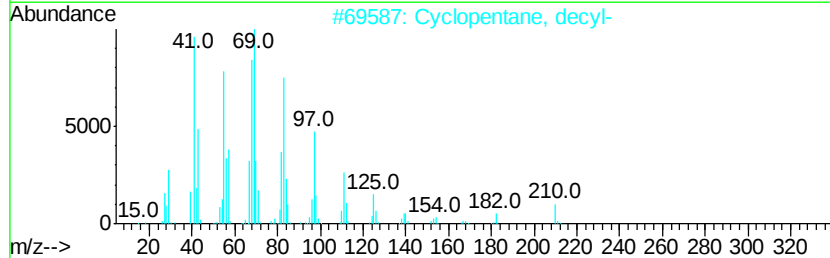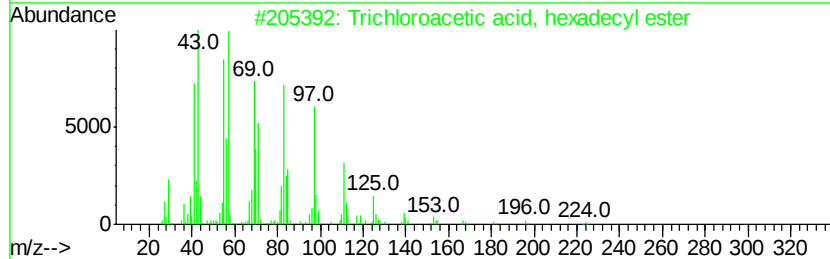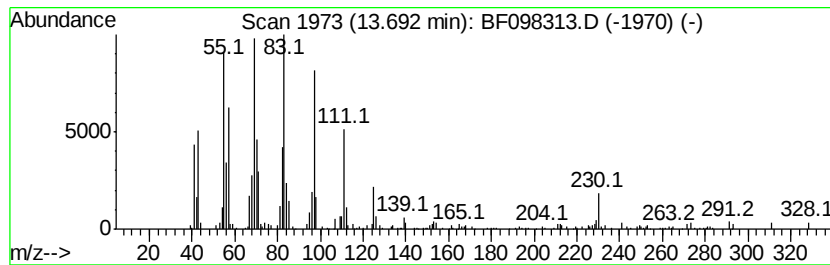

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF090717\
Data File : BF098313.D
Acq On : 7 Sep 2017 15:01
Operator : SJ/JU
Sample : I5075-01
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
72-11948










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 10 2-Bromo dodecane Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.27	9.48 ng	328379	Chrysene-d12	13.84

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Bromo dodecane	248	C12H25Br	013187-99-0	93
2			Hexacosane	366	C26H54	000630-01-3	91
3			Hentriacontane	437	C31H64	000630-04-6	91
4			Heneicosane	296	C21H44	000629-94-7	90
5			Heptacosane	380	C27H56	000593-49-7	90

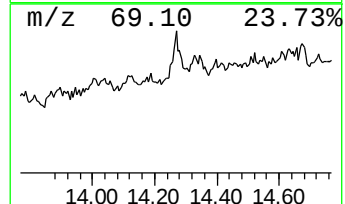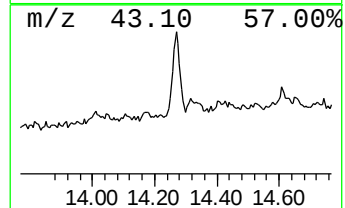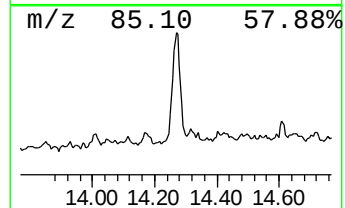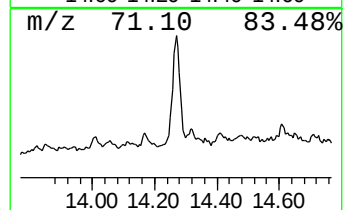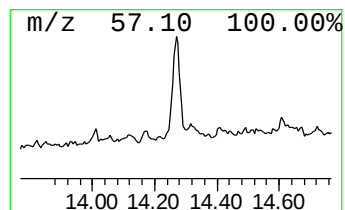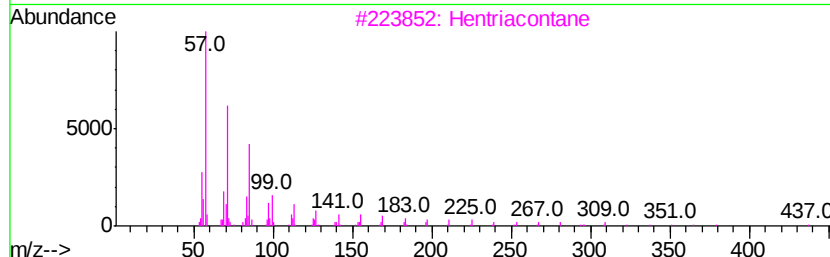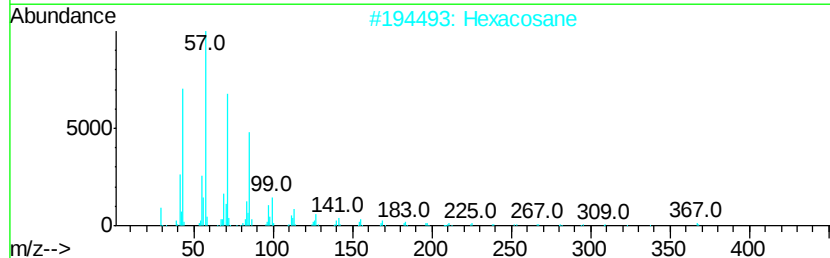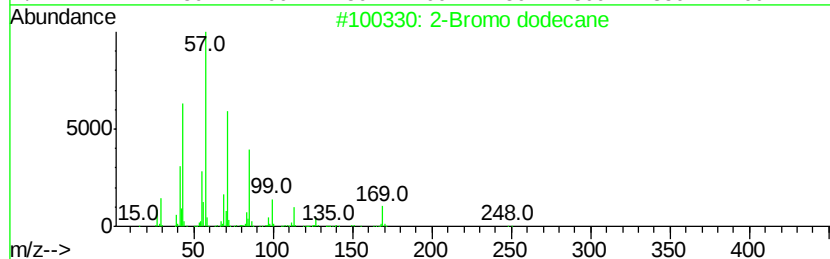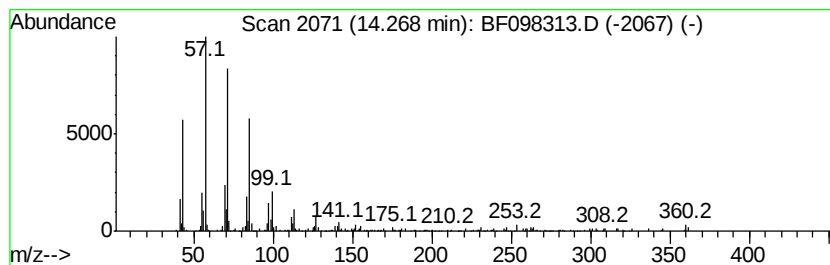

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF090717\
Data File : BF098313.D
Acq On : 7 Sep 2017 15:01
Operator : SJ/JU
Sample : I5075-01
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
72-11948

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown4.866	4.86	4.7	ng	178644	1	6.69	757712	20.0
unknown6.46	6.46	43.6	ng	1653250	1	6.69	757712	20.0
Dodecane, 2,7,10-...	8.40	2.2	ng	110690	2	7.97	1021950	20.0
Tetracontane, 3,5...	9.13	2.6	ng	132308	3	9.72	1020990	20.0
Tridecane, 5-propyl-	10.65	4.1	ng	181758	4	11.20	888168	20.0
Tridecane	11.10	2.2	ng	98416	4	11.20	888168	20.0
Hexadecane	13.65	10.0	ng	347936	5	13.84	693037	20.0
Trichloroacetic a...	13.69	5.9	ng	205081	5	13.84	693037	20.0
2-Bromo dodecane	14.27	9.5	ng	328379	5	13.84	693037	20.0