

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF090717\
 Data File : BF098321.D
 Acq On : 7 Sep 2017 18:45
 Operator : SJ/JU
 Sample : I5052-06 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G30A-0-3-COMP

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.857	468	471	479	rBV	18722	22629	2.46%	0.345%
2	5.287	540	544	553	rVB	225205	215133	23.38%	3.278%
3	6.328	717	721	733	rBV	239694	236625	25.71%	3.606%
4	6.451	739	742	750	rVB	256844	237456	25.80%	3.619%
5	6.686	778	782	789	rBV	886954	707036	76.82%	10.774%
6	6.839	805	808	812	rBV	206807	174376	18.95%	2.657%
7	7.251	875	878	883	rBV	153697	127830	13.89%	1.948%
8	7.969	996	1000	1004	rBV	991456	920350	100.00%	14.025%
9	9.045	1180	1183	1187	rBV	336386	250397	27.21%	3.816%
10	9.127	1192	1197	1203	rBV2	6537	10915	1.19%	0.166%
11	9.445	1247	1251	1255	rBV	38259	34517	3.75%	0.526%
12	9.722	1294	1298	1302	rBV	950073	909042	98.77%	13.853%
13	10.510	1429	1432	1437	rVB	131692	107788	11.71%	1.643%
14	10.639	1450	1454	1458	rBV2	18187	26265	2.85%	0.400%
15	11.110	1531	1534	1539	rVB2	11320	12958	1.41%	0.197%
16	11.204	1546	1550	1553	rBV	907175	829125	90.09%	12.635%
17	11.227	1553	1554	1557	rVV	42863	26613	2.89%	0.406%
18	11.280	1561	1563	1567	rVB	14205	11712	1.27%	0.178%
19	11.733	1638	1640	1644	rVB3	11213	10918	1.19%	0.166%
20	12.186	1714	1717	1719	rBV3	11047	14956	1.63%	0.228%
21	12.257	1726	1729	1732	rBV4	14892	16990	1.85%	0.259%
22	12.345	1740	1744	1746	rBV4	13097	17226	1.87%	0.263%
23	12.415	1753	1756	1759	rBV	58218	48261	5.24%	0.735%
24	12.645	1792	1795	1797	rVV	45048	37386	4.06%	0.570%
25	12.668	1797	1799	1802	rVB4	11465	11982	1.30%	0.183%
26	12.786	1816	1819	1823	rBV	232393	201386	21.88%	3.069%
27	13.227	1892	1894	1897	rBV3	20008	23268	2.53%	0.355%
28	13.839	1994	1998	2001	rBV	839227	788255	85.65%	12.012%
29	15.251	2234	2238	2242	rBV	471678	530756	57.67%	8.088%


Sum of corrected areas: 6562151

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF090717\
Data File : BF098321.D
Acq On : 7 Sep 2017 18:45
Operator : SJ/JU
Sample : I5052-06 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G30A-0-3-COMP

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

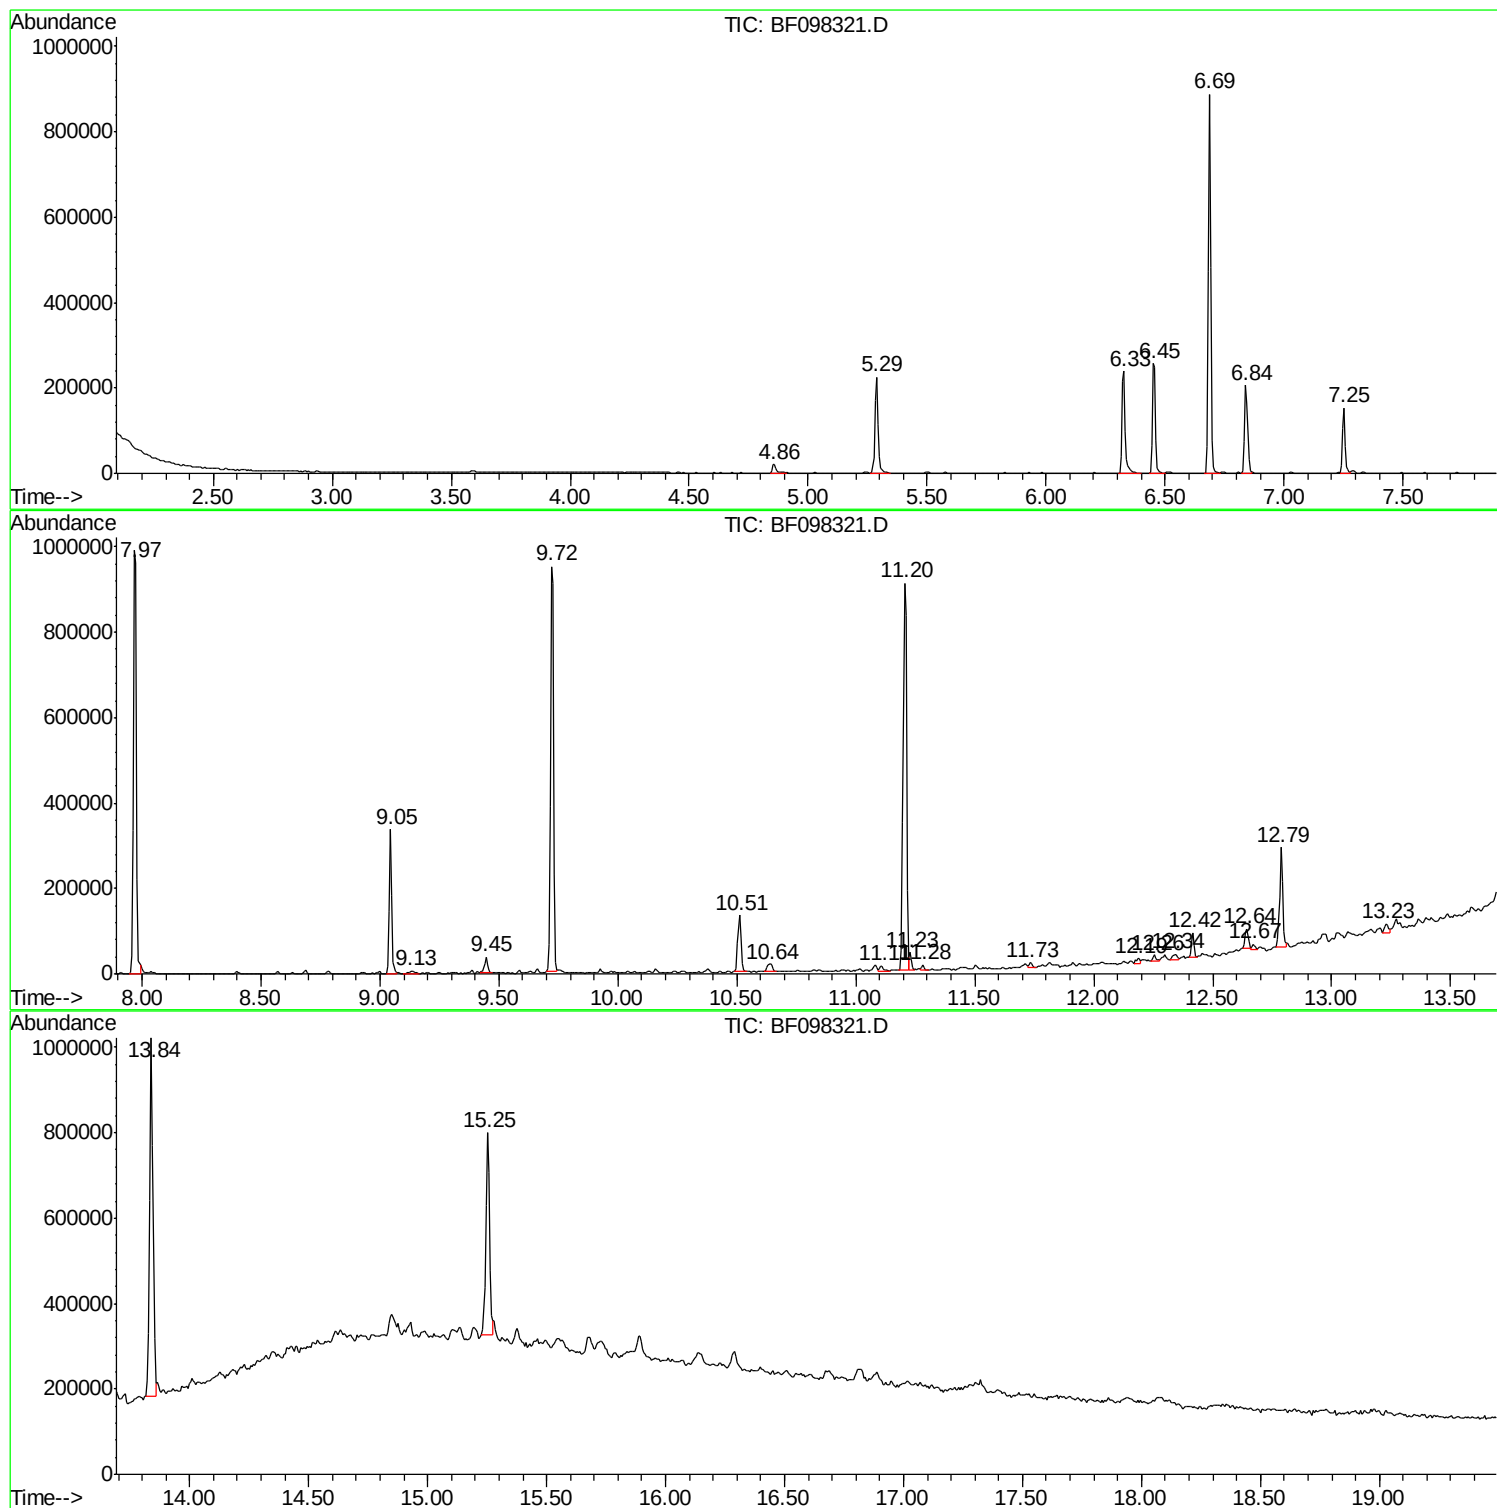

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF090717\
Data File : BF098321.D
Acq On : 7 Sep 2017 18:45
Operator : SJ/JU
Sample : I5052-06 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G30A-0-3-COMP










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.45 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.45	6.72 ng	237456	1,4-Dichlorobenzene-d4	6.69

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			5-Aminoindole	132	C8H8N2	005192-03-0	10
2			1,2,4-Trifluorobenzene	132	C6H3F3	000367-23-7	9
3			1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9
4			Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5			Benzene, 1-ethenyl-3,5-dimethyl-	132	C10H12	005379-20-4	9

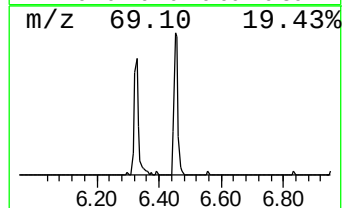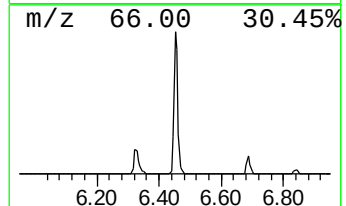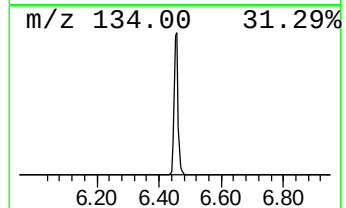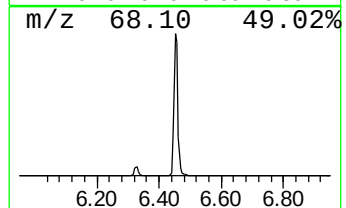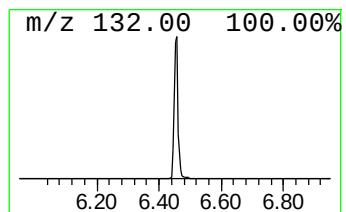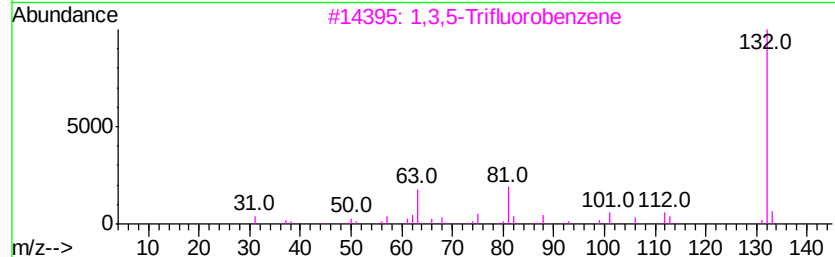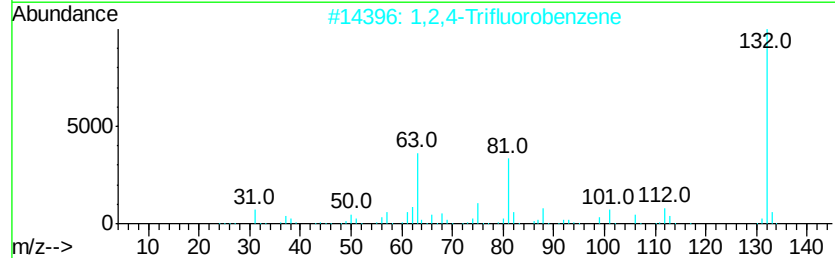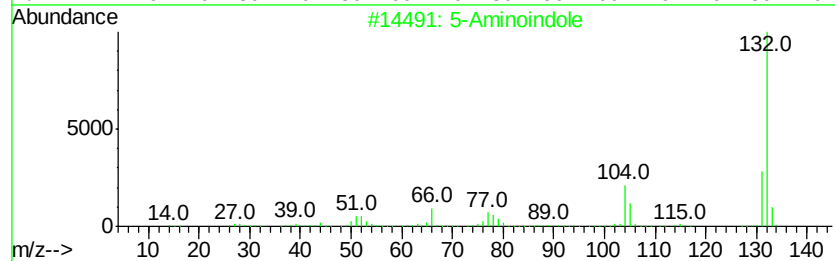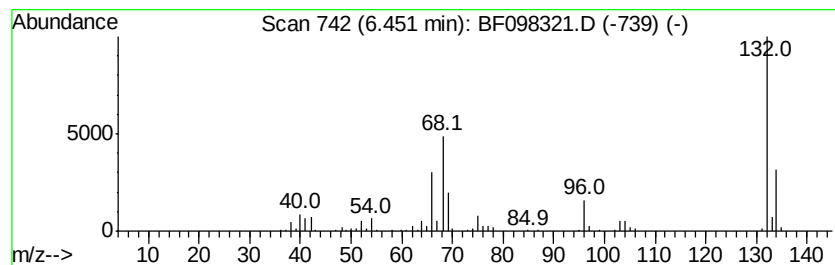

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF090717\
Data File : BF098321.D
Acq On : 7 Sep 2017 18:45
Operator : SJ/JU
Sample : I5052-06 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G30A-0-3-COMP

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.45	6.45	6.7	ng	237456	1	6.69	707036	20.0