

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF090717\
 Data File : BF098334.D
 Acq On : 8 Sep 2017 00:50
 Operator : SJ/JU
 Sample : I5071-17 5X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G57A-0-1.5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.851	467	470	481	rVB	32178	37909	4.36%	0.467%
2	5.287	540	544	551	rBV	427217	401920	46.19%	4.950%
3	6.328	718	721	730	rBV	526803	457488	52.57%	5.634%
4	6.457	739	743	749	rBV	519781	436644	50.18%	5.378%
5	6.687	779	782	786	rBV	790289	653119	75.06%	8.044%
6	6.839	805	808	812	rBV	358018	321748	36.97%	3.963%
7	7.251	875	878	884	rBV	288796	236738	27.21%	2.916%
8	7.975	997	1001	1004	rBV	1004416	839686	96.50%	10.341%
9	9.045	1180	1183	1187	rBV	603968	499001	57.34%	6.146%
10	9.445	1247	1251	1255	rBV	72246	59355	6.82%	0.731%
11	9.728	1295	1299	1302	rBV	1007499	870185	100.00%	10.717%
12	10.380	1404	1410	1412	rBV3	10560	11700	1.34%	0.144%
13	10.510	1429	1432	1439	rVB	227841	212083	24.37%	2.612%
14	10.633	1450	1453	1459	rVB2	20923	31176	3.58%	0.384%
15	11.080	1526	1529	1531	rBV2	18161	15688	1.80%	0.193%
16	11.110	1531	1534	1539	rVB4	13742	15545	1.79%	0.191%
17	11.210	1547	1551	1554	rBV	1049427	863940	99.28%	10.640%
18	11.504	1599	1601	1604	rVB2	12344	10242	1.18%	0.126%
19	11.910	1668	1670	1673	rVB2	12972	10415	1.20%	0.128%
20	12.186	1714	1717	1719	rBV4	7777	10433	1.20%	0.128%
21	12.298	1734	1736	1741	rVB4	17154	17145	1.97%	0.211%
22	12.416	1753	1756	1759	rBV	48208	41656	4.79%	0.513%
23	12.645	1792	1795	1798	rBV	43841	41141	4.73%	0.507%
24	12.669	1798	1799	1802	rVB3	20795	16123	1.85%	0.199%
25	12.792	1816	1820	1823	rBV	477333	444700	51.10%	5.477%
26	12.969	1848	1850	1854	rVB5	14548	15139	1.74%	0.186%
27	13.027	1857	1860	1864	rVB3	25054	27818	3.20%	0.343%
28	13.274	1899	1902	1905	rBV4	24666	27532	3.16%	0.339%
29	13.368	1915	1918	1921	rBV2	27641	26023	2.99%	0.320%
30	13.698	1971	1974	1980	rVB2	51342	64279	7.39%	0.792%
31	13.845	1994	1999	2002	rBV	790781	758624	87.18%	9.343%
32	14.010	2025	2027	2030	rBV	33534	32317	3.71%	0.398%
33	14.315	2077	2079	2082	rBV	41795	36861	4.24%	0.454%
34	14.610	2127	2129	2132	rBV2	52843	51428	5.91%	0.633%

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF090717\
Data File : BF098334.D
Acq On : 8 Sep 2017 00:50
Operator : SJ/JU
Sample : I5071-17 5X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G57A-0-1.5

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	15.257	2234	2239	2242	rBV	416628	523875	60.20%	6.452%
----	--------	------	------	------	-----	--------	--------	--------	--------


Sum of corrected areas: 8119676

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF090717\
Data File : BF098334.D
Acq On : 8 Sep 2017 00:50
Operator : SJ/JU
Sample : I5071-17 5X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G57A-0-1.5

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

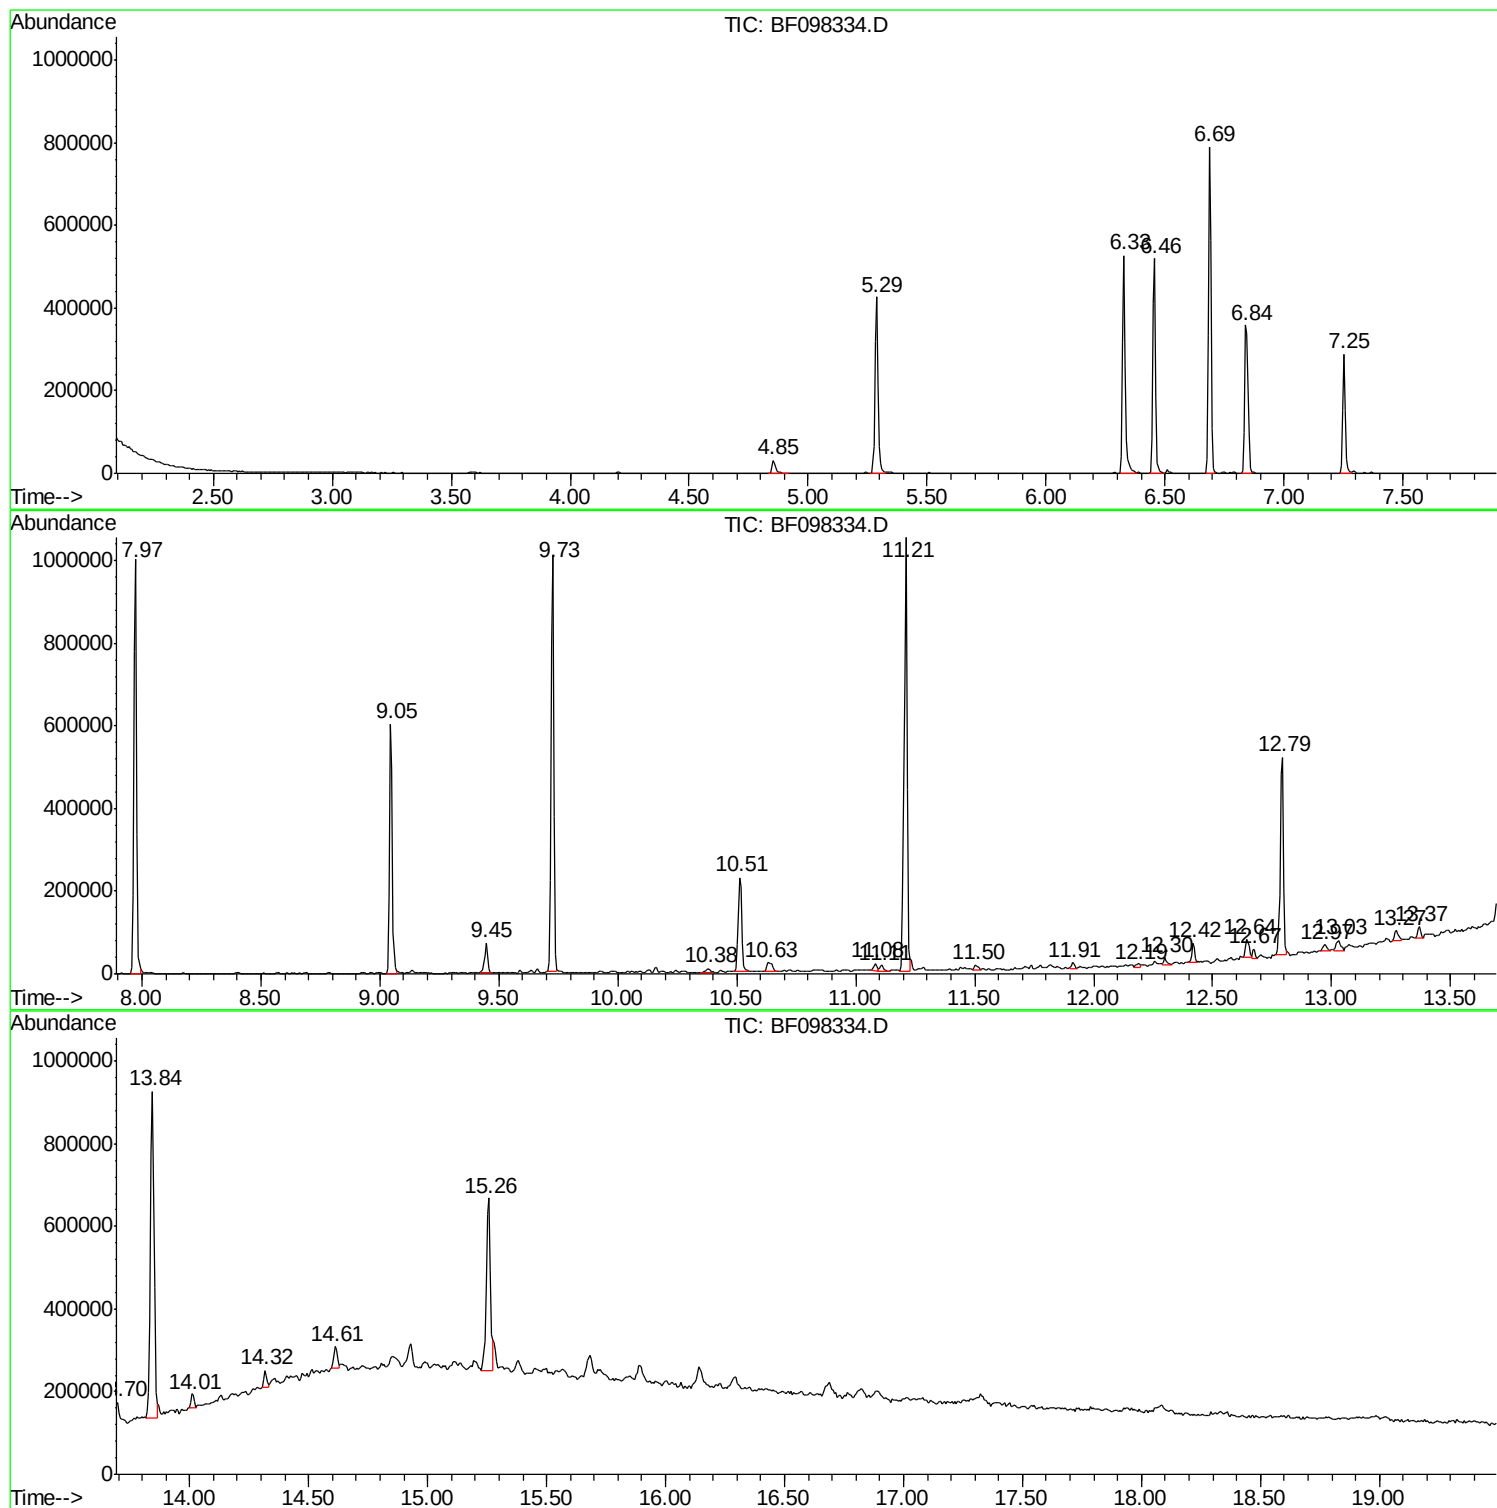

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF090717\
Data File : BF098334.D
Acq On : 8 Sep 2017 00:50
Operator : SJ/JU
Sample : I5071-17 5X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G57A-0-1.5










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.46 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.46	13.37 ng	436644	1,4-Dichlorobenzene-d4	6.69

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9
4		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5		1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	9

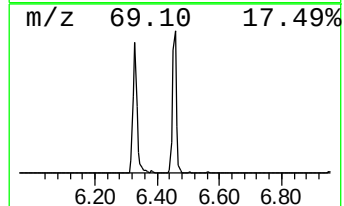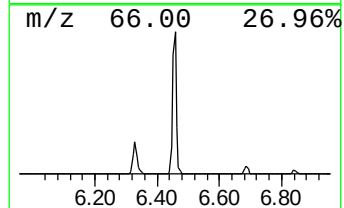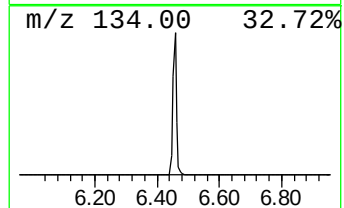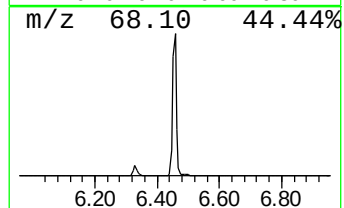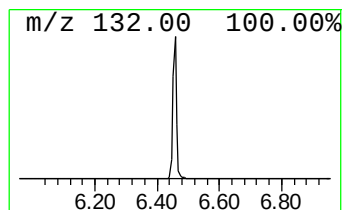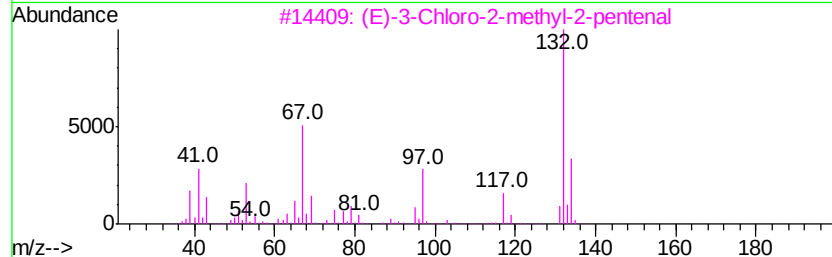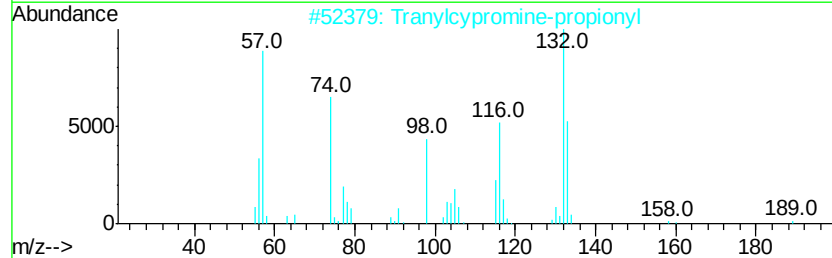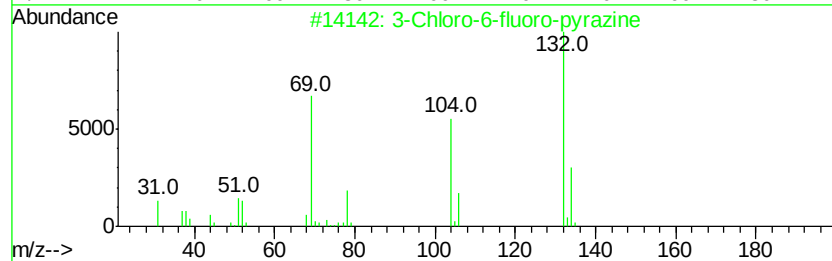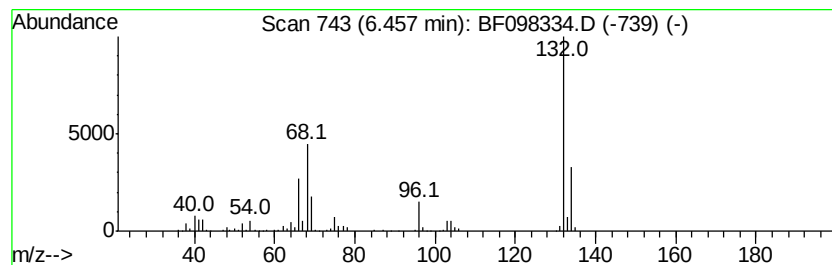

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF090717\
Data File : BF098334.D
Acq On : 8 Sep 2017 00:50
Operator : SJ/JU
Sample : I5071-17 5X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G57A-0-1.5

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.46	6.46	13.4	ng	436644	1	6.69	653119	20.0