

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF090717\
 Data File : BF098342.D
 Acq On : 8 Sep 2017 5:05
 Operator : SJ/JU
 Sample : I5132-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 090617-TIDO-F-D-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.857	468	471	485	rVB	121686	141382	4.99%	0.827%
2	5.287	541	544	560	rBV	1008485	965921	34.10%	5.650%
3	6.328	717	721	733	rBV2	821892	747852	26.40%	4.374%
4	6.457	739	743	746	rBV	1824272	1567645	55.34%	9.170%
5	6.686	779	782	786	rBV	707152	575817	20.33%	3.368%
6	6.845	805	809	812	rBV	2300925	2062651	72.82%	12.065%
7	7.257	874	879	882	rBV	1710502	1664141	58.75%	9.734%
8	7.975	997	1001	1003	rBV	762927	713804	25.20%	4.175%
9	9.051	1179	1184	1187	rBV	3067774	2832564	100.00%	16.569%
10	9.445	1247	1251	1254	rBV	98232	77277	2.73%	0.452%
11	9.722	1294	1298	1302	rBV	770923	715682	25.27%	4.186%
12	10.510	1428	1432	1445	rBV	965704	961374	33.94%	5.623%
13	11.204	1547	1550	1553	rBV	728568	659936	23.30%	3.860%
14	12.798	1816	1821	1824	rBV	2281326	2347388	82.87%	13.731%
15	13.839	1994	1998	2002	rBV	684654	602224	21.26%	3.523%
16	14.674	2136	2140	2143	rBV	29641	32608	1.15%	0.191%
17	15.251	2233	2238	2246	rBV	354332	427619	15.10%	2.501%


Sum of corrected areas: 17095885

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF090717\
Data File : BF098342.D
Acq On : 8 Sep 2017 5:05
Operator : SJ/JU
Sample : I5132-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
090617-TIDO-F-D-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

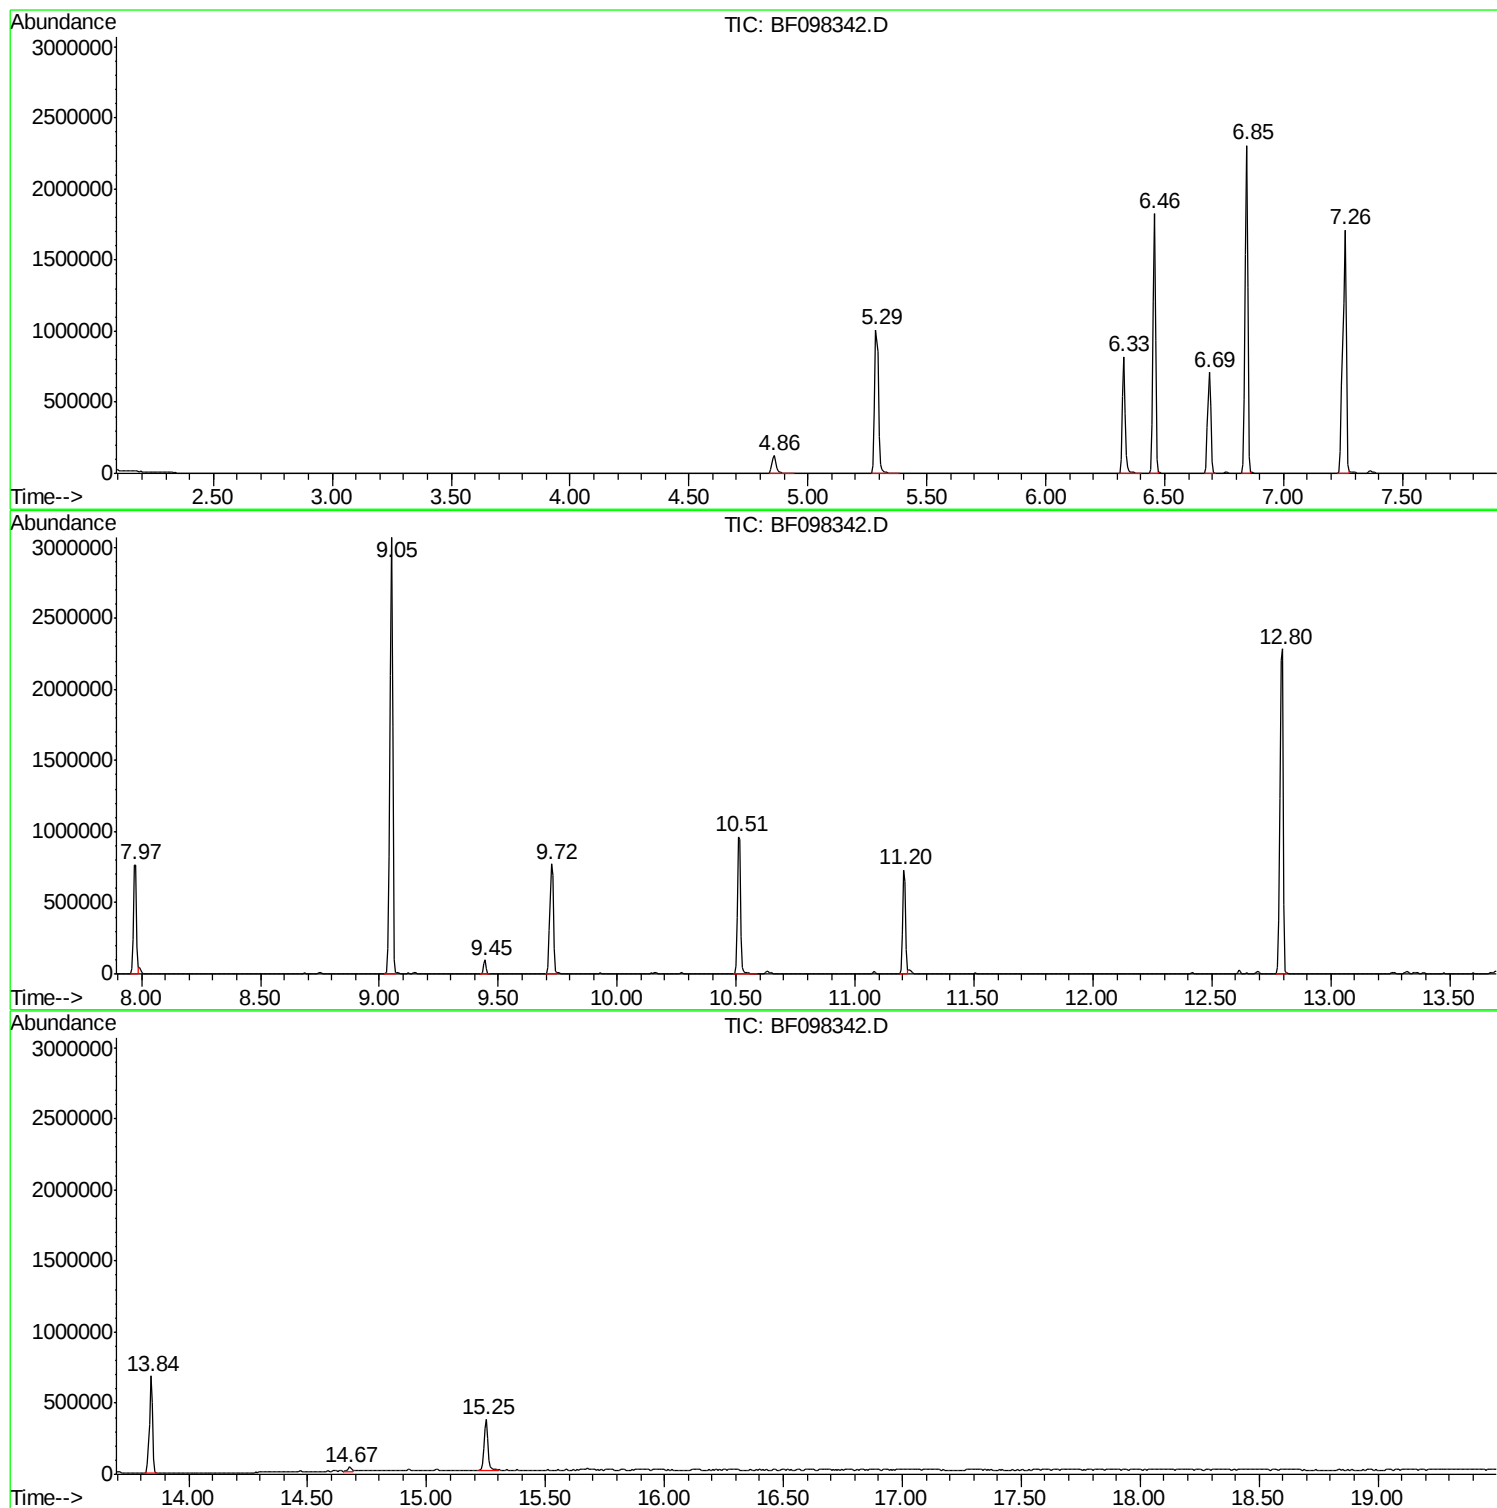

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF090717\
Data File : BF098342.D
Acq On : 8 Sep 2017 5:05
Operator : SJ/JU
Sample : I5132-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
090617-TIDO-F-D-B










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.86	4.91 ng	141382	1,4-Dichlorobenzene-d4	6.69

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
2			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9
3			5-Hexen-2-one	98	C6H10O	000109-49-9	9
4			(+)-4-Amino-4,5-dihydro-2(3H)-f...	101	C4H7NO2	016504-58-8	9
5			Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9

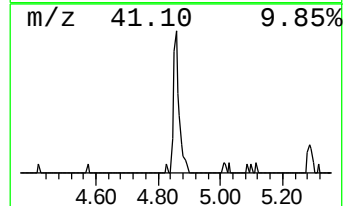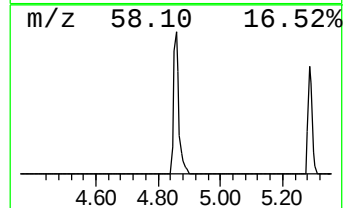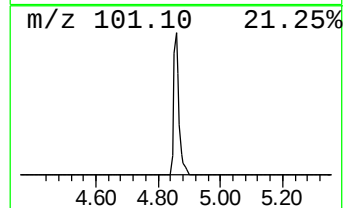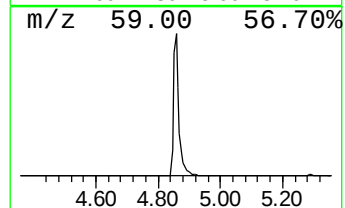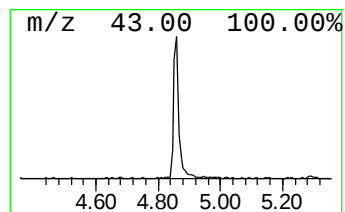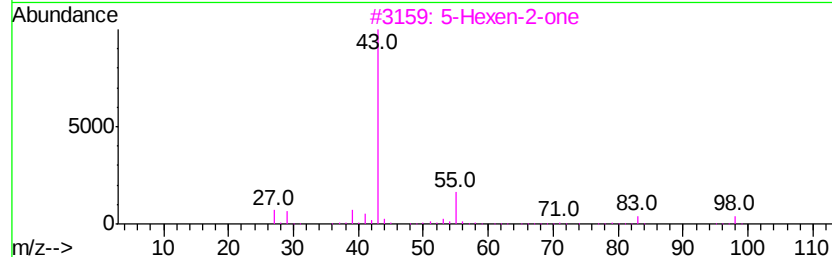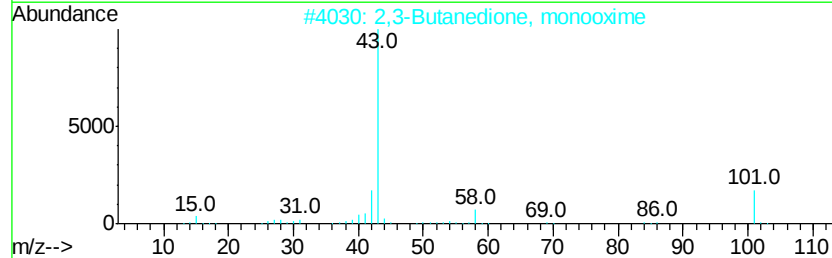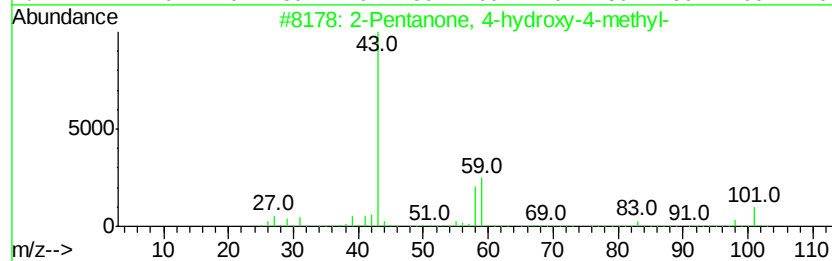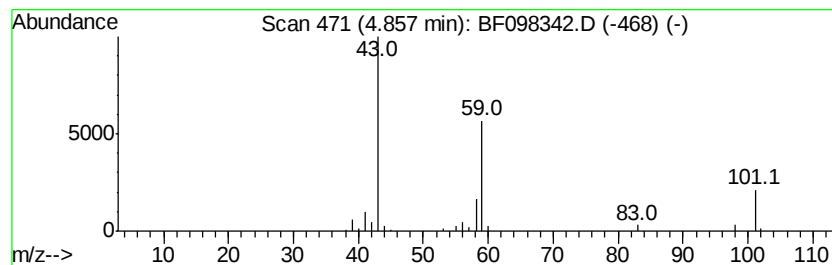

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF090717\
Data File : BF098342.D
Acq On : 8 Sep 2017 5:05
Operator : SJ/JU
Sample : I5132-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
090617-TIDO-F-D-B










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.46 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.46	54.45 ng	1567650	1,4-Dichlorobenzene-d4	6.69

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9
4		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9
5		Xenon	132	Xe	007440-63-3	9

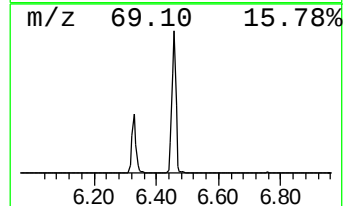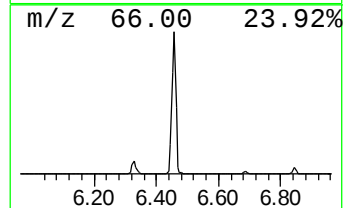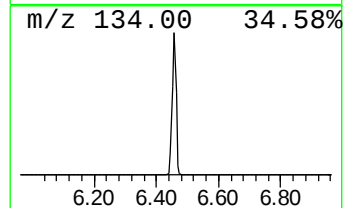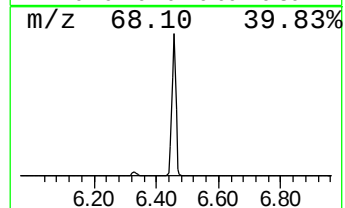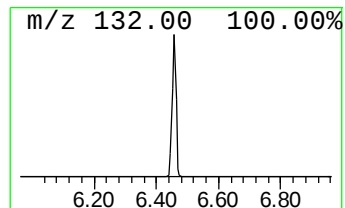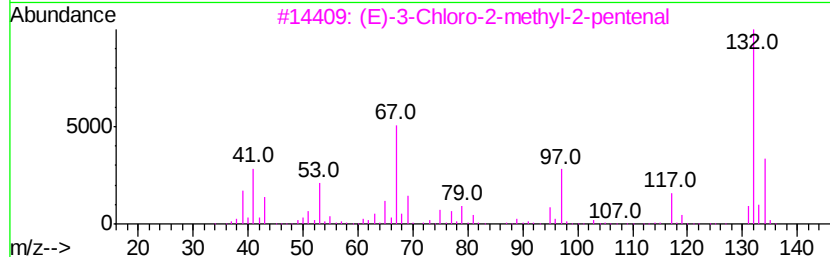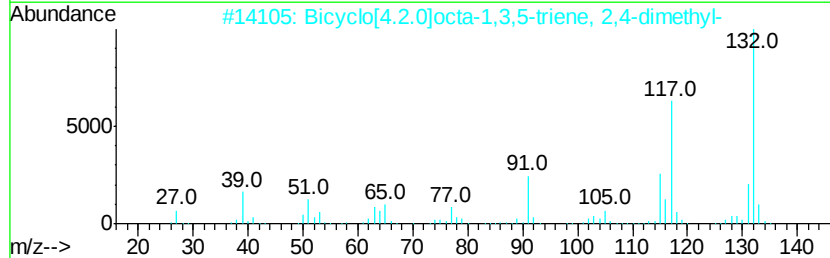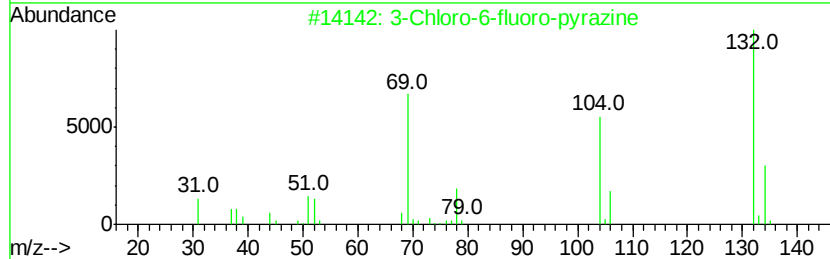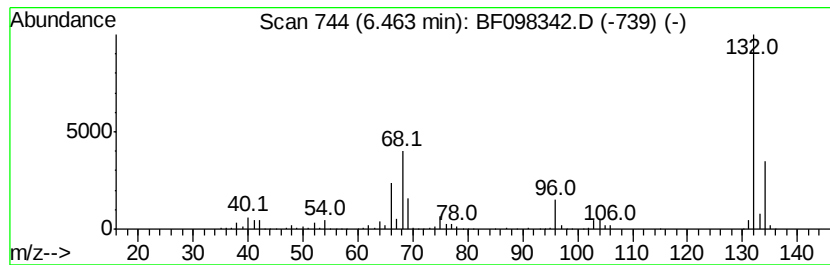

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF090717\
Data File : BF098342.D
Acq On : 8 Sep 2017 5:05
Operator : SJ/JU
Sample : I5132-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
090617-TIDO-F-D-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.86	4.9	ng	141382	1	6.69	575817	20.0
unknown6.46	6.46	54.5	ng	1567650	1	6.69	575817	20.0