


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF090717\
 Data File : BF098311.D
 Acq On : 7 Sep 2017 13:30
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 05 17:28:20 2017

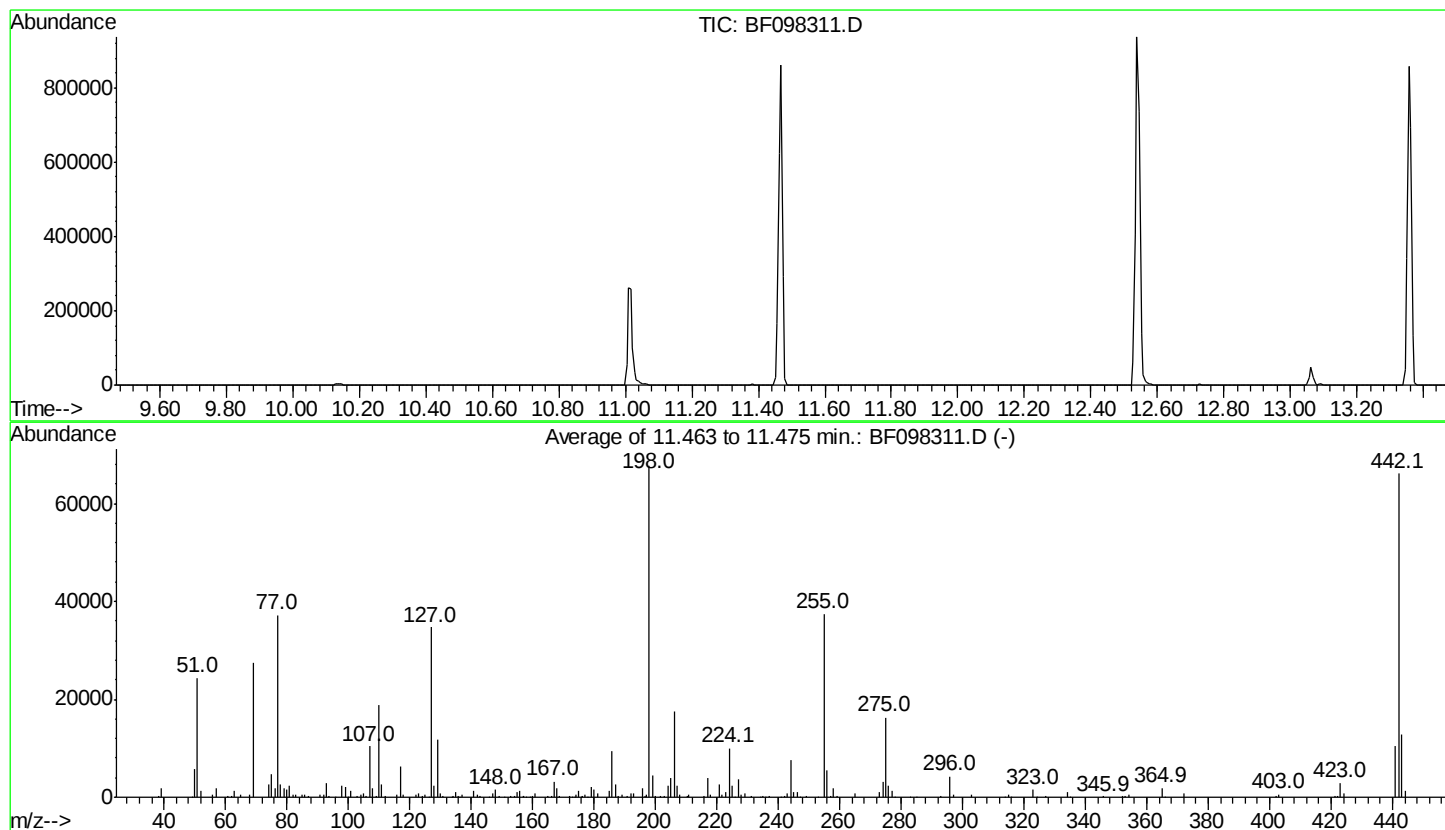

AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	24363	PASS
68	69	0.00	2	1.7	469	PASS
69	198	0.00	100	40.6	27502	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.2	34678	PASS
197	198	0.00	2	1.0	654	PASS
198	198	100	100	100.0	67728	PASS
199	198	5	9	6.5	4370	PASS
275	198	10	60	24.0	16267	PASS
365	198	1	100	2.8	1930	PASS
441	442	0.01	24	15.9	10527	PASS
442	198	50	100	97.7	66160	PASS
443	442	15	24	19.4	12803	PASS