


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF090717\
 Data File : BF098336.D
 Acq On : 8 Sep 2017 2:14
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 05 17:28:20 2017

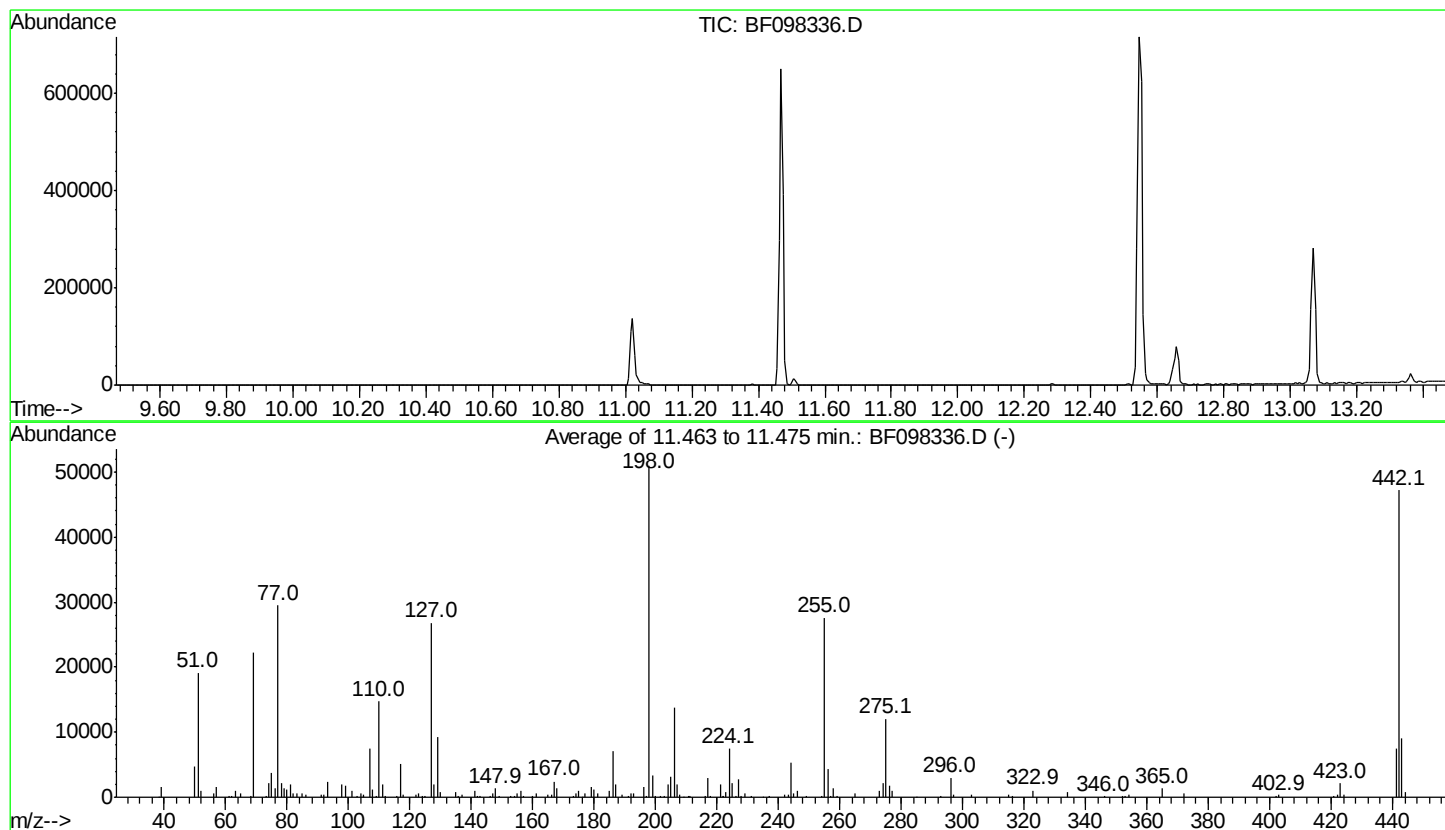

AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1590

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.6	19156	PASS
68	69	0.00	2	1.3	288	PASS
69	198	0.00	100	43.7	22267	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.7	26856	PASS
197	198	0.00	2	0.6	297	PASS
198	198	100	100	100.0	50970	PASS
199	198	5	9	6.6	3365	PASS
275	198	10	60	23.6	12052	PASS
365	198	1	100	2.7	1354	PASS
441	442	0.01	24	16.1	7581	PASS
442	198	50	100	92.5	47148	PASS
443	442	15	24	19.2	9040	PASS