
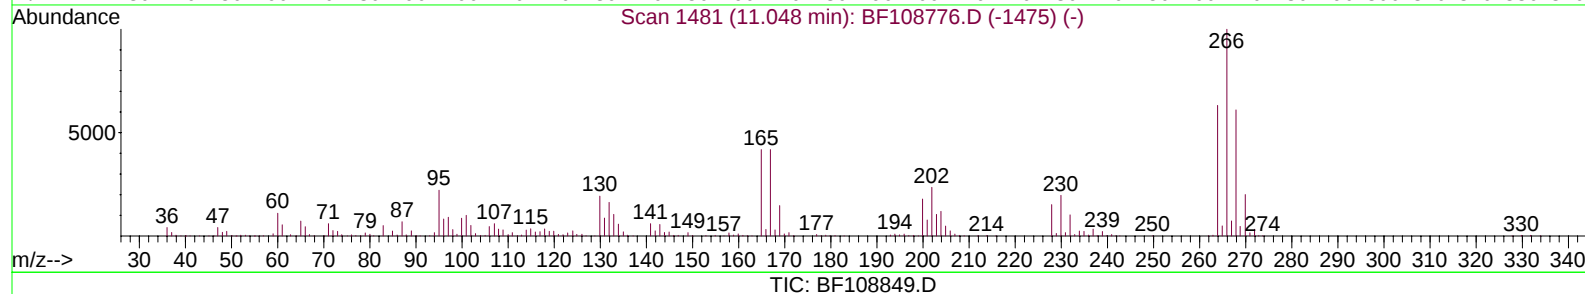
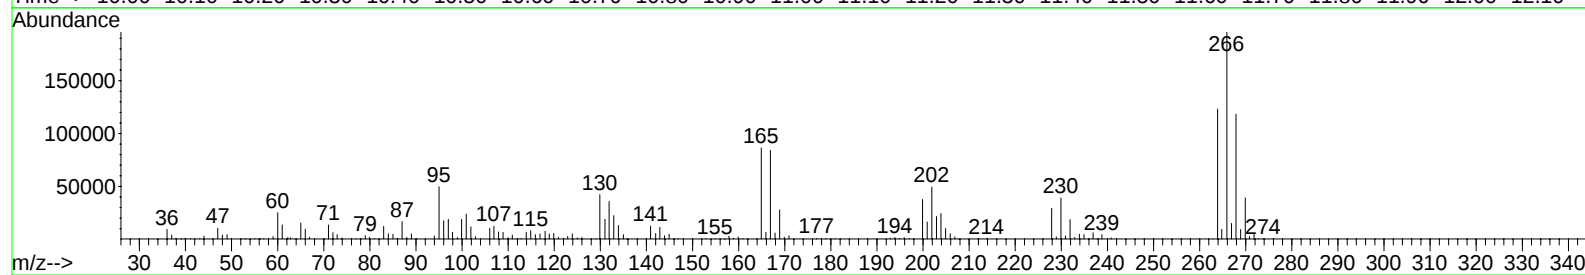


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF090718\
Data File : BF108849.D
Acq On : 7 Sep 2018 10:06
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 07 18:18:58 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF090518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 05 18:03:31 2018
Response via : Initial Calibration

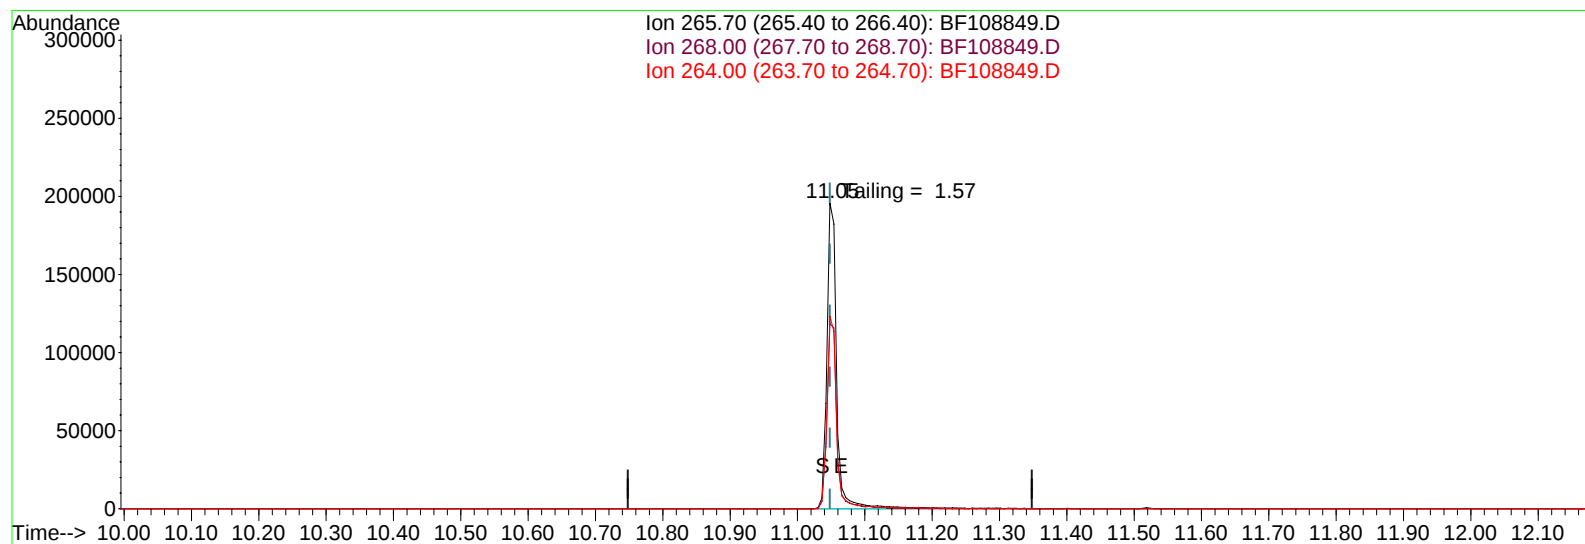

(69) Pentachlorophenol (C)




11.048min (+0.000) 68312.08ng

response 195378

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.47
264.00	61.90	62.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF090718\
Data File : BF108849.D
Acq On : 7 Sep 2018 10:06
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 07 18:18:58 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF090518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 05 18:03:31 2018
Response via : Initial Calibration

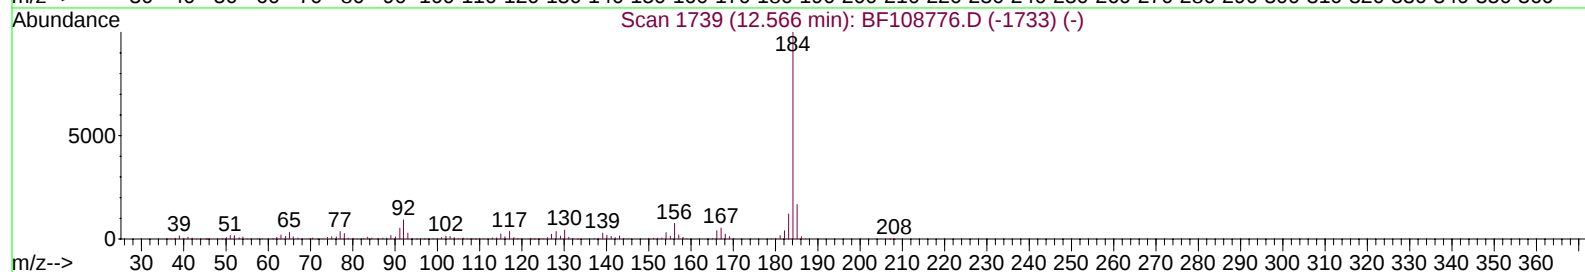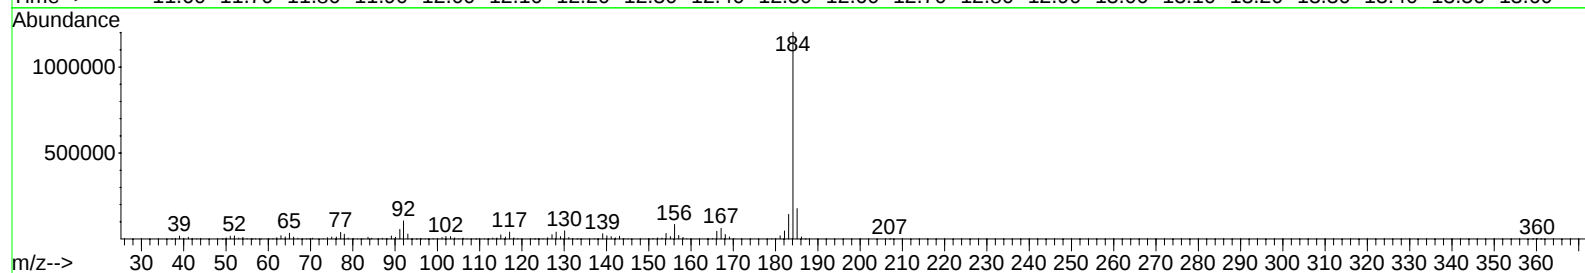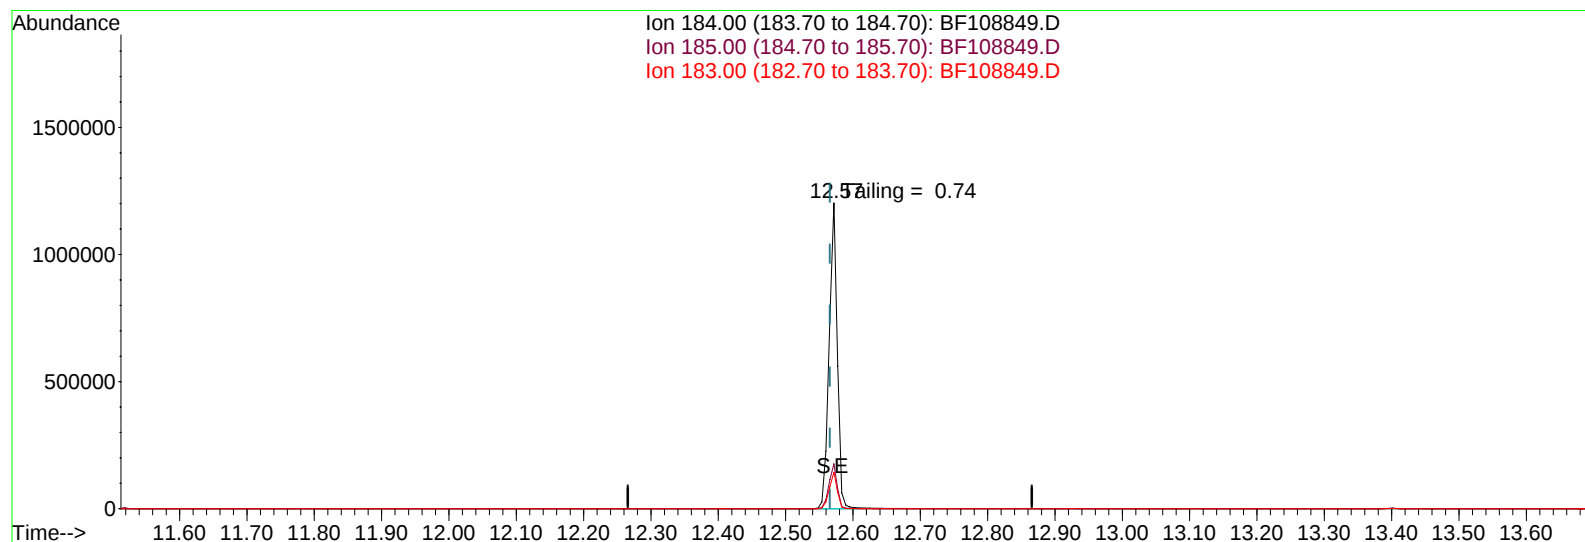

TIC: BF108849.D

(76) Benzidine

12.572min (+0.006) 6823.42ng

response 1020337

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.72
183.00	11.60	11.98
0.00	0.00	0.00