
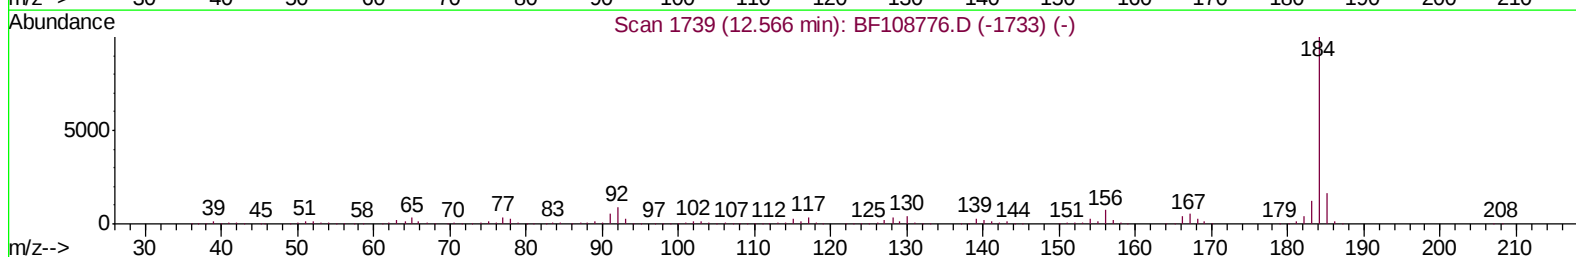
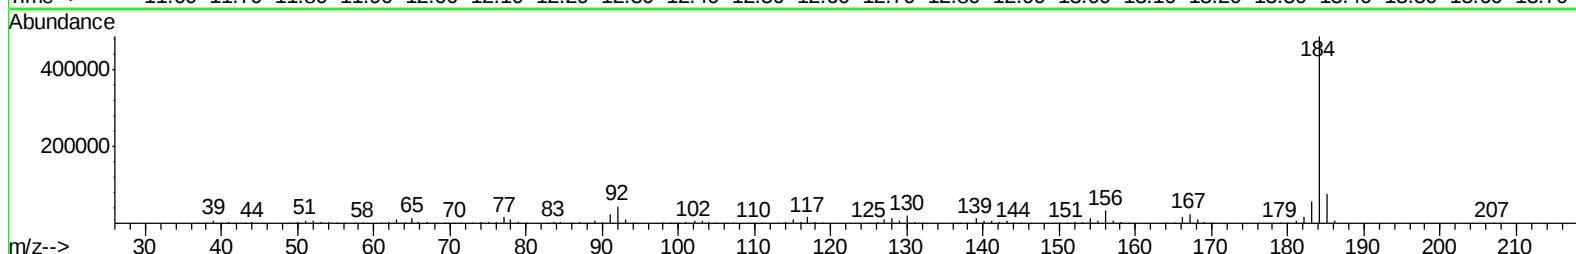


Data File : BF108876.D
Acq On : 7 Sep 2018 22:42
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 08 03:56:25 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF090518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 05 18:03:31 2018
Response via : Initial Calibration

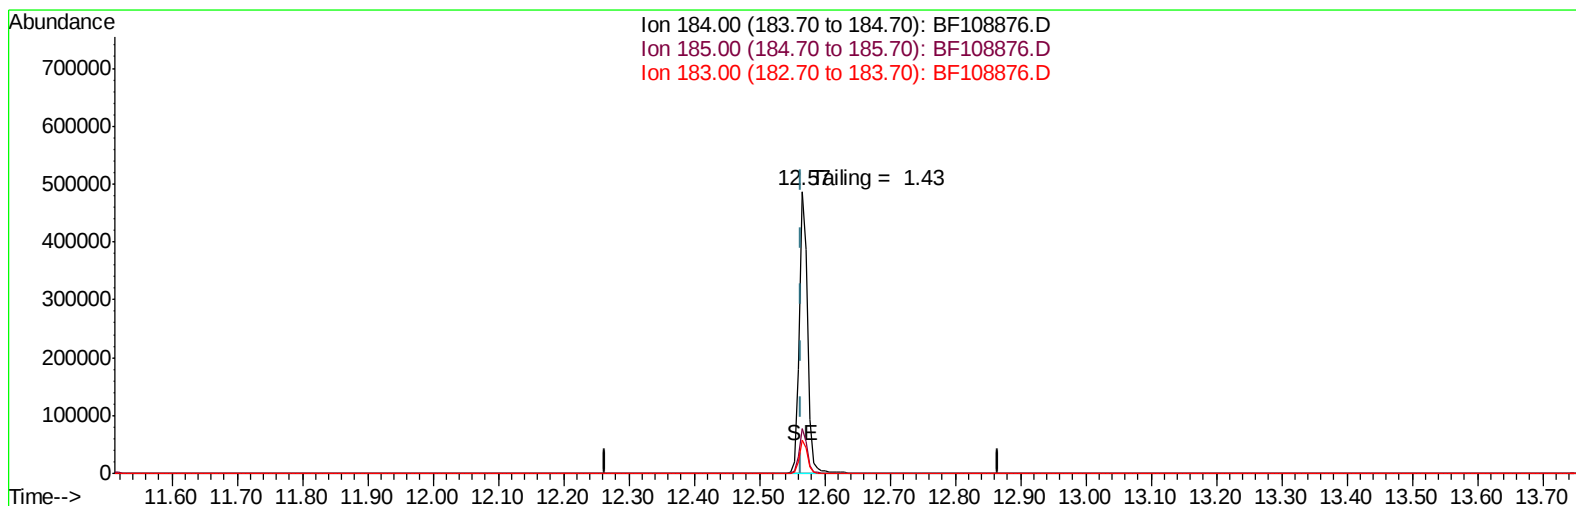

TIC: BF108876.D

(76) Benzidine

12.566min (0.000) 0.00ng m

response 432767

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.85
183.00	11.60	11.92
0.00	0.00	0.00

Data File : BF108876.D

Acq On : 7 Sep 2018 22:42

Operator : JU/SJ

Sample : DFTPP

Misc :

ALS Vial : 1 Sample Multiplier: 1




Quant Time: Sep 08 03:56:25 2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF090518.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Sep 05 18:03:31 2018

Response via : Initial Calibration

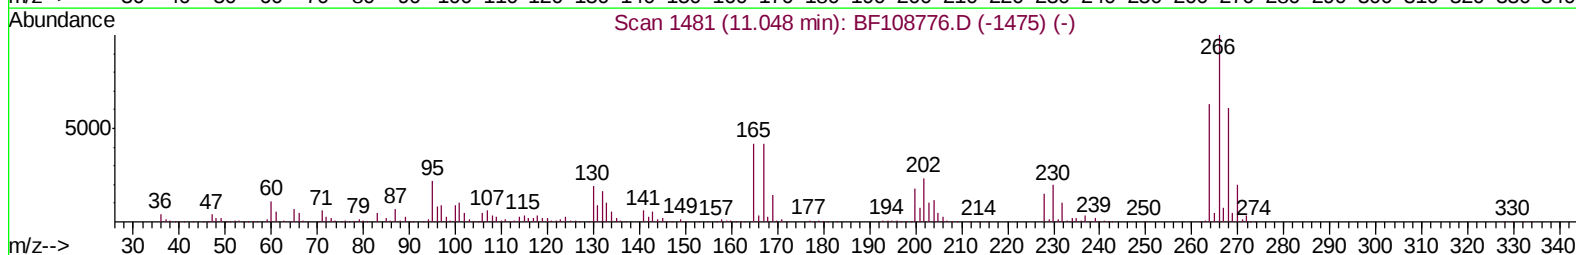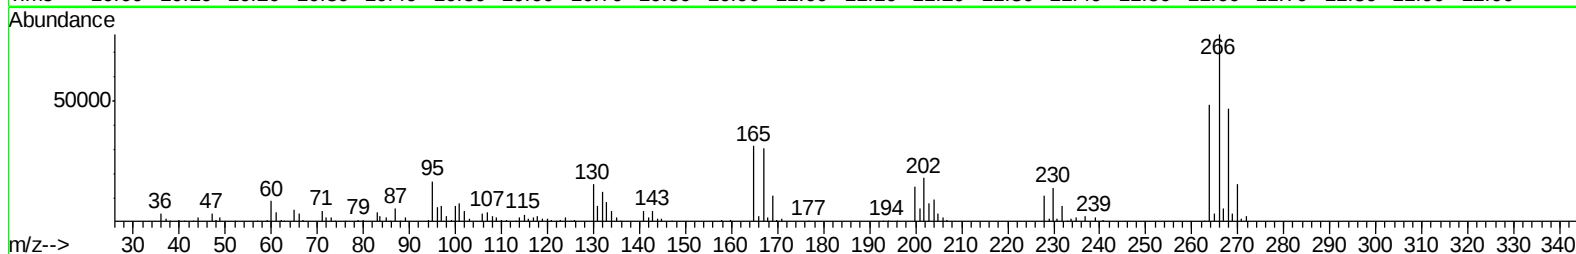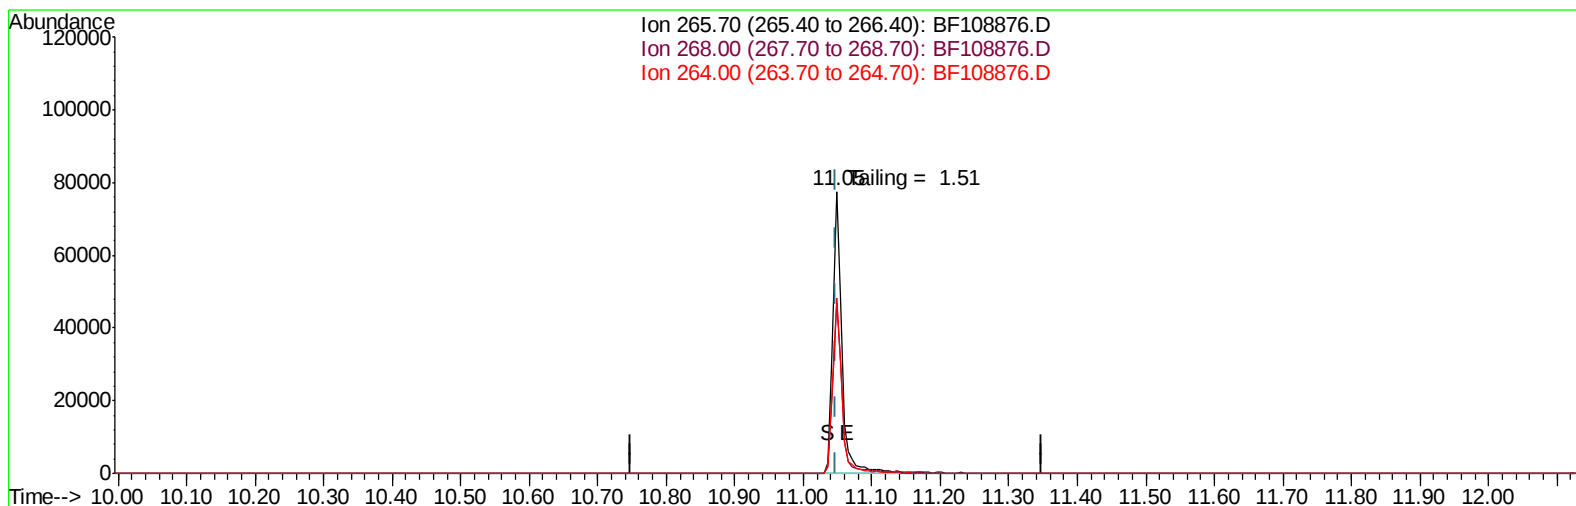

TIC: BF108876.D

(69) Pentachlorophenol (C)

11.048min (0.000) 33286.30ng

response 67966

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.35
264.00	61.90	62.42
0.00	0.00	0.00