


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090718\
 Data File : BF108849.D
 Acq On : 7 Sep 2018 10:06
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF090518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 05 18:03:31 2018

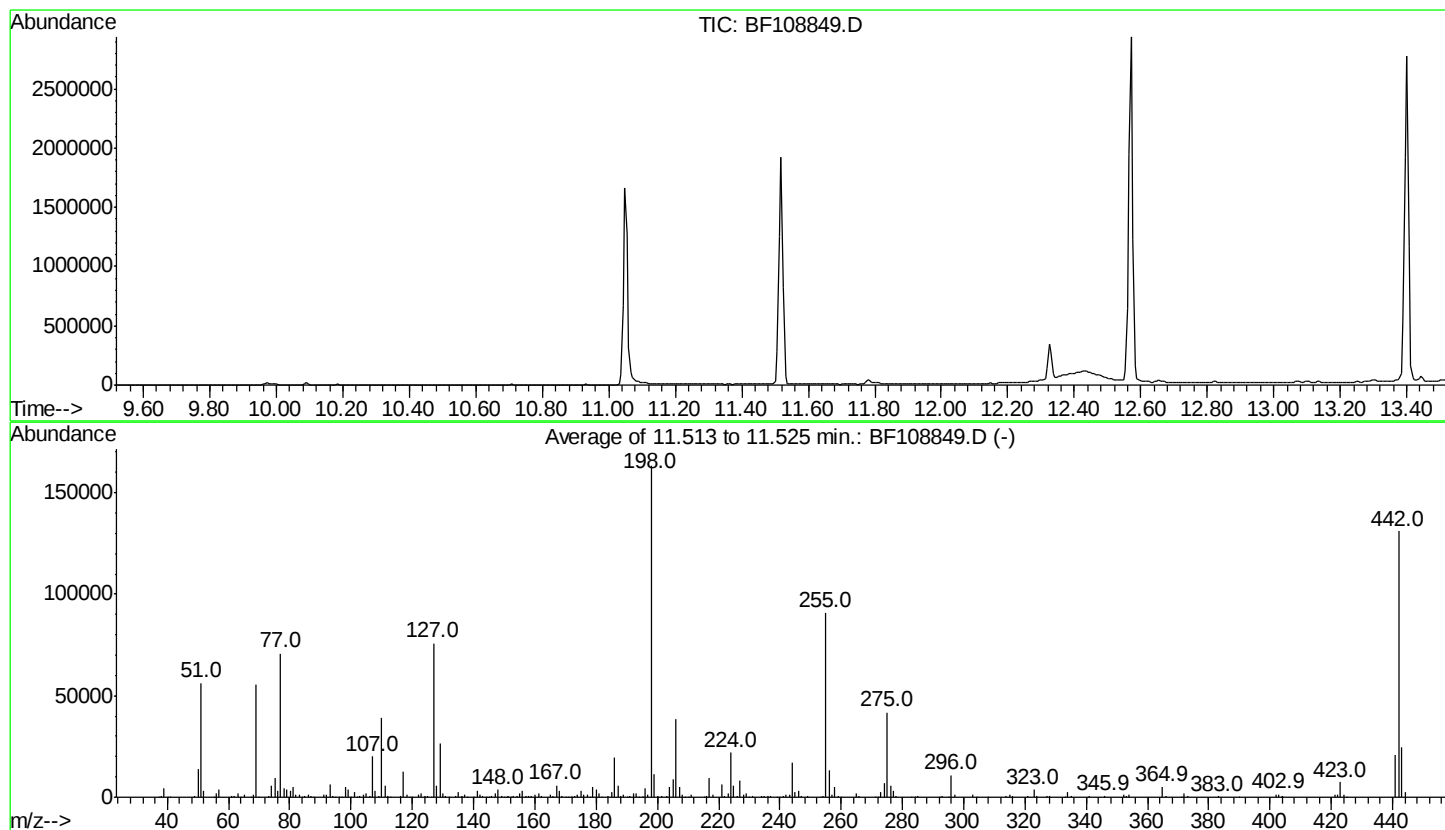

AutoFind: Scans 1560, 1561, 1562; Background Corrected with Scan 1554

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.6	56434	PASS
68	69	0.00	2	1.7	972	PASS
69	198	0.00	100	34.2	55801	PASS
70	69	0.00	2	0.6	326	PASS
127	198	10	80	46.4	75829	PASS
197	198	0.00	2	0.6	1040	PASS
198	198	100	100	100.0	163317	PASS
199	198	5	9	6.8	11109	PASS
275	198	10	60	25.6	41784	PASS
365	198	1	100	3.2	5207	PASS
441	198	0.01	100	12.7	20733	PASS
442	198	50	100	80.3	131130	PASS
443	442	15	24	18.6	24432	PASS