

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090721\
 Data File : BF125384.D
 Acq On : 7 Sep 2021 12:59
 Operator : JU/CG
 Sample : PB138943BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB138943BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF125384.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.205	13	20	27	rVB	107716	148406	2.69%	0.465%
2	5.528	580	585	588	rBV	4212025	4181654	75.79%	13.113%
3	6.534	750	756	759	rBV	3547189	4059499	73.57%	12.730%
4	6.898	814	818	821	rBV	1054127	895339	16.23%	2.808%
5	7.463	909	914	917	rBV	2780025	2701991	48.97%	8.473%
6	8.181	1032	1036	1048	rBV	1268604	1182487	21.43%	3.708%
7	9.257	1214	1219	1222	rBV	5054380	4689298	84.99%	14.705%
8	9.934	1330	1334	1347	rBV	1435042	1350140	24.47%	4.234%
9	10.728	1464	1469	1484	rBV	3317088	3301814	59.84%	10.354%
10	11.422	1583	1587	1595	rBV	1500223	1437737	26.06%	4.508%
11	13.010	1852	1857	1860	rBV	5823816	5517547	100.00%	17.302%
12	13.933	2011	2014	2020	rVB	108283	108803	1.97%	0.341%
13	14.063	2032	2036	2045	rBV	1269891	1226767	22.23%	3.847%
14	15.557	2284	2290	2300	rBV	719975	1088603	19.73%	3.414%

Sum of corrected areas: 31890085

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090721\
Data File : BF125384.D
Acq On : 7 Sep 2021 12:59
Operator : JU/CG
Sample : PB138943BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138943BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.205	3.32 ng	148406	1,4-Dichlorobenzene-d4	6.898

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	47
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
4			3-Pentanol, 2,4-dimethyl-	116	C7H16O	000600-36-2	25
5			3-Pentanol, 3-methyl-	102	C6H14O	000077-74-7	25

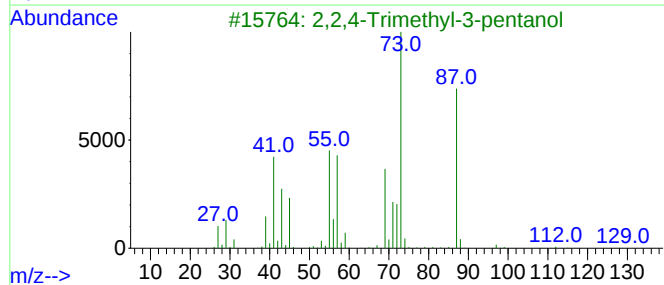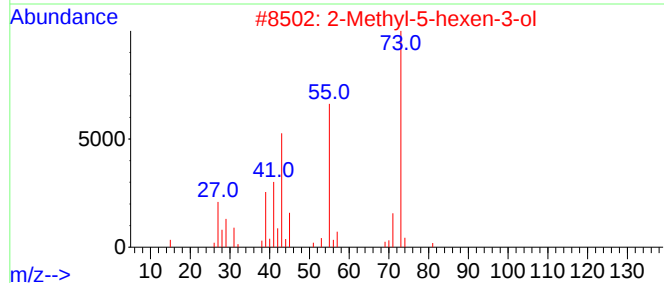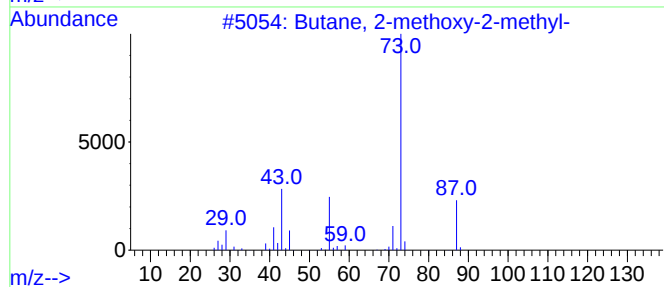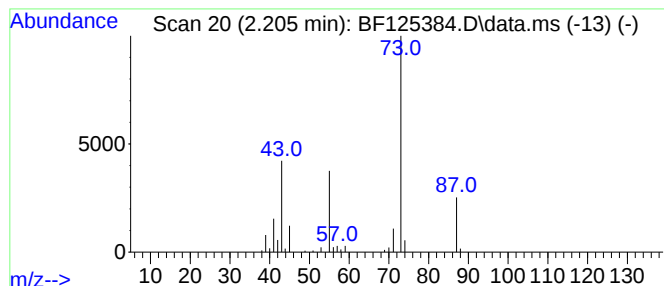

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090721\
Data File : BF125384.D
Acq On : 7 Sep 2021 12:59
Operator : JU/CG
Sample : PB138943BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138943BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.205	3.3	ng	148406	1	6.898	895339	20.0