

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF090721\  
 Data File : BF125393.D  
 Acq On : 7 Sep 2021 18:05  
 Operator : JU/CG  
 Sample : M3655-01  
 Misc :  
 ALS Vial : 15 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 CON-A

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF081821.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF125393.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 2.210       | 13            | 21          | 29           | rVB      | 1158352        | 1570973       | 54.93%          | 5.723%        |
| 2         | 3.663       | 263           | 268         | 275          | rVB      | 36195          | 54463         | 1.90%           | 0.198%        |
| 3         | 4.516       | 404           | 413         | 417          | rBV      | 2167387        | 2428859       | 84.92%          | 8.849%        |
| 4         | 5.134       | 511           | 518         | 521          | rBV      | 2292600        | 2860048       | 100.00%         | 10.420%       |
| 5         | 5.522       | 580           | 584         | 596          | rBV      | 498079         | 475799        | 16.64%          | 1.733%        |
| 6         | 5.616       | 596           | 600         | 604          | rVB      | 305657         | 241550        | 8.45%           | 0.880%        |
| 7         | 6.528       | 749           | 755         | 771          | rBV      | 1845867        | 1777797       | 62.16%          | 6.477%        |
| 8         | 6.898       | 814           | 818         | 821          | rBV      | 992969         | 790916        | 27.65%          | 2.882%        |
| 9         | 6.957       | 825           | 828         | 834          | rBV      | 177474         | 172285        | 6.02%           | 0.628%        |
| 10        | 7.222       | 870           | 873         | 878          | rBV      | 65196          | 56297         | 1.97%           | 0.205%        |
| 11        | 7.457       | 909           | 913         | 922          | rBV      | 1769036        | 1696981       | 59.33%          | 6.183%        |
| 12        | 8.081       | 1016          | 1019        | 1030         | rBV      | 183469         | 391837        | 13.70%          | 1.428%        |
| 13        | 8.181       | 1032          | 1036        | 1039         | rVV      | 1071826        | 890280        | 31.13%          | 3.244%        |
| 14        | 8.398       | 1070          | 1073        | 1081         | rVB2     | 44609          | 52204         | 1.83%           | 0.190%        |
| 15        | 8.869       | 1149          | 1153        | 1164         | rBV      | 46665          | 98055         | 3.43%           | 0.357%        |
| 16        | 9.251       | 1214          | 1218        | 1222         | rBV      | 2877456        | 2730621       | 95.47%          | 9.948%        |
| 17        | 9.328       | 1229          | 1231        | 1234         | rVB      | 41821          | 34214         | 1.20%           | 0.125%        |
| 18        | 9.581       | 1270          | 1274        | 1276         | rBV4     | 26554          | 31801         | 1.11%           | 0.116%        |
| 19        | 9.604       | 1276          | 1278        | 1282         | rVV      | 45267          | 48530         | 1.70%           | 0.177%        |
| 20        | 9.639       | 1282          | 1284        | 1288         | rVB      | 77340          | 63762         | 2.23%           | 0.232%        |
| 21        | 9.733       | 1297          | 1300        | 1310         | rBV      | 1006406        | 1812639       | 63.38%          | 6.604%        |
| 22        | 9.845       | 1316          | 1319        | 1323         | rVB2     | 98146          | 101564        | 3.55%           | 0.370%        |
| 23        | 9.933       | 1331          | 1334        | 1338         | rVB      | 996923         | 886089        | 30.98%          | 3.228%        |
| 24        | 9.969       | 1338          | 1340        | 1344         | rBV5     | 39914          | 45238         | 1.58%           | 0.165%        |
| 25        | 10.116      | 1363          | 1365        | 1371         | rVB7     | 25828          | 30845         | 1.08%           | 0.112%        |
| 26        | 10.251      | 1383          | 1388        | 1389         | rBV4     | 49703          | 53137         | 1.86%           | 0.194%        |
| 27        | 10.269      | 1389          | 1391        | 1394         | rVV3     | 61417          | 54876         | 1.92%           | 0.200%        |
| 28        | 10.304      | 1394          | 1397        | 1400         | rVV4     | 50664          | 58303         | 2.04%           | 0.212%        |
| 29        | 10.339      | 1400          | 1403        | 1407         | rVV2     | 148408         | 137468        | 4.81%           | 0.501%        |
| 30        | 10.392      | 1409          | 1412        | 1418         | rVV5     | 41331          | 83082         | 2.90%           | 0.303%        |
| 31        | 10.557      | 1437          | 1440        | 1442         | rBV3     | 42062          | 48856         | 1.71%           | 0.178%        |
| 32        | 10.727      | 1465          | 1469        | 1470         | rBV3     | 59948          | 74516         | 2.61%           | 0.271%        |
| 33        | 10.769      | 1470          | 1476        | 1477         | rBV3     | 212365         | 429052        | 15.00%          | 1.563%        |
| 34        | 11.216      | 1550          | 1552        | 1555         | rVB3     | 53893          | 42167         | 1.47%           | 0.154%        |
| 35        | 11.422      | 1584          | 1587        | 1591         | rBV      | 926305         | 849727        | 29.71%          | 3.096%        |
| 36        | 12.810      | 1818          | 1823        | 1831         | rBV2     | 72851          | 149959        | 5.24%           | 0.546%        |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF090721\  
Data File : BF125393.D  
Acq On : 7 Sep 2021 18:05  
Operator : JU/CG  
Sample : M3655-01  
Misc :  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
CON-A

Integration Parameters: rteint.p  
Integrator: RTE  
Smoothing : ON Filtering: 5  
Sampling : 1 Min Area: 3 % of largest Peak  
Start Thrs: 0.2 Max Peaks: 100  
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF081821.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

|    |        |      |      |      |      |         |         |        |        |
|----|--------|------|------|------|------|---------|---------|--------|--------|
| 37 | 13.010 | 1852 | 1857 | 1860 | rBV  | 2688279 | 2559843 | 89.50% | 9.326% |
| 38 | 13.680 | 1968 | 1971 | 1973 | rBV3 | 52916   | 58845   | 2.06%  | 0.214% |
| 39 | 13.816 | 1990 | 1994 | 1997 | rBV  | 43743   | 77542   | 2.71%  | 0.283% |
| 40 | 13.857 | 1997 | 2001 | 2004 | rVB  | 120809  | 153237  | 5.36%  | 0.558% |
| 41 | 13.892 | 2004 | 2007 | 2010 | rBV  | 187986  | 186199  | 6.51%  | 0.678% |
| 42 | 13.927 | 2010 | 2013 | 2019 | rBV  | 648010  | 644024  | 22.52% | 2.346% |
| 43 | 14.033 | 2028 | 2031 | 2033 | rBV  | 87509   | 77291   | 2.70%  | 0.282% |
| 44 | 14.063 | 2033 | 2036 | 2040 | rVB  | 866384  | 855420  | 29.91% | 3.117% |
| 45 | 14.580 | 2121 | 2124 | 2127 | rBV2 | 52377   | 44785   | 1.57%  | 0.163% |
| 46 | 15.180 | 2223 | 2226 | 2229 | rVB  | 45356   | 44893   | 1.57%  | 0.164% |
| 47 | 15.433 | 2265 | 2269 | 2276 | rVB2 | 286879  | 357783  | 12.51% | 1.303% |
| 48 | 15.562 | 2285 | 2291 | 2300 | rVB  | 714068  | 1009463 | 35.30% | 3.678% |
| 49 | 16.015 | 2365 | 2368 | 2375 | rVB  | 38505   | 53801   | 1.88%  | 0.196% |


Sum of corrected areas: 27447916

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF090721\  
Data File : BF125393.D  
Acq On : 7 Sep 2021 18:05  
Operator : JU/CG  
Sample : M3655-01  
Misc :  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
CON-A

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF081821.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

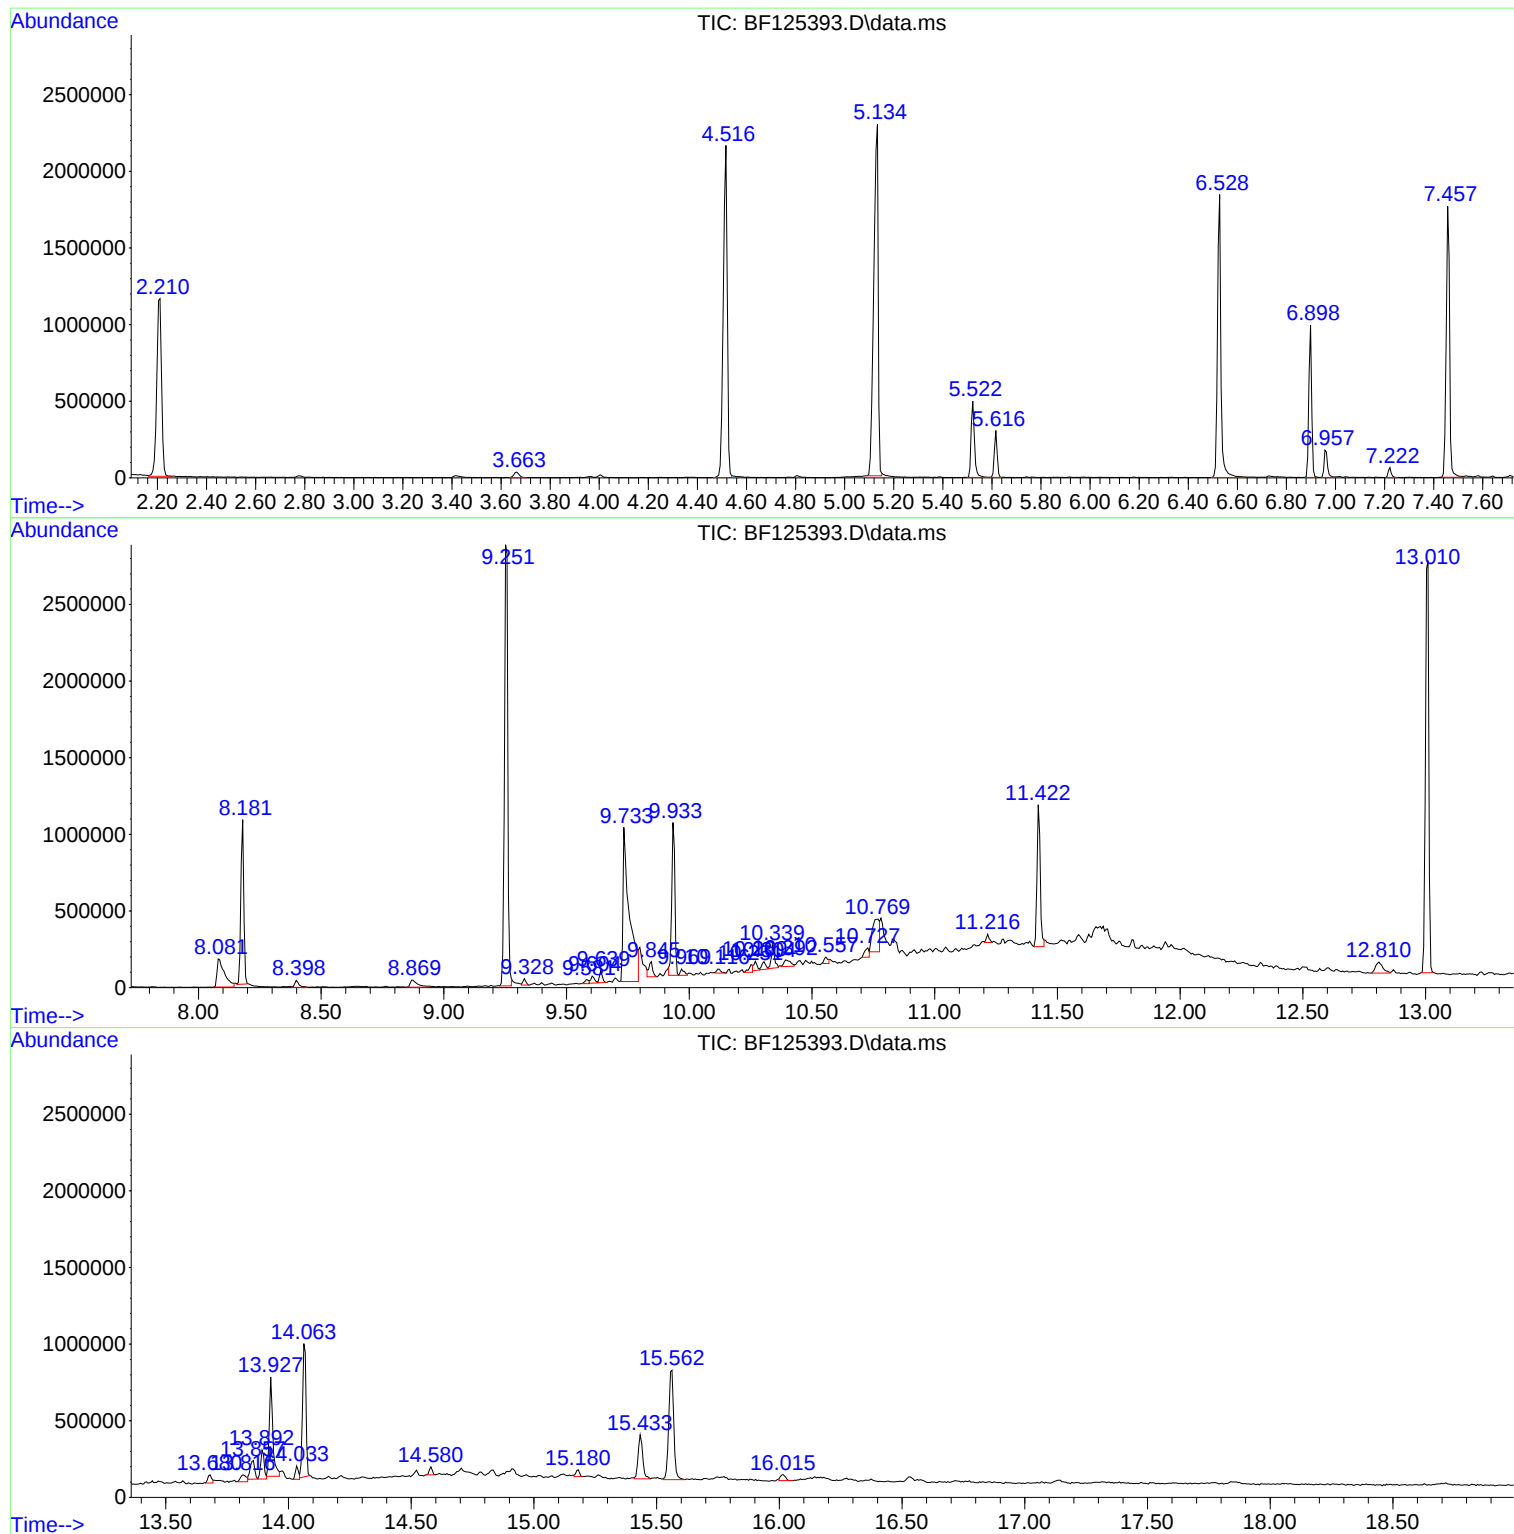

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF090721\  
Data File : BF125393.D  
Acq On : 7 Sep 2021 18:05  
Operator : JU/CG  
Sample : M3655-01  
Misc :  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
CON-A

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF081821.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF090721\  
Data File : BF125393.D  
Acq On : 7 Sep 2021 18:05  
Operator : JU/CG  
Sample : M3655-01  
Misc :  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
CON-A

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF081821.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |

-----