


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090721\
 Data File : BF125379.D
 Acq On : 7 Sep 2021 9:47
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 08 14:14:01 2021

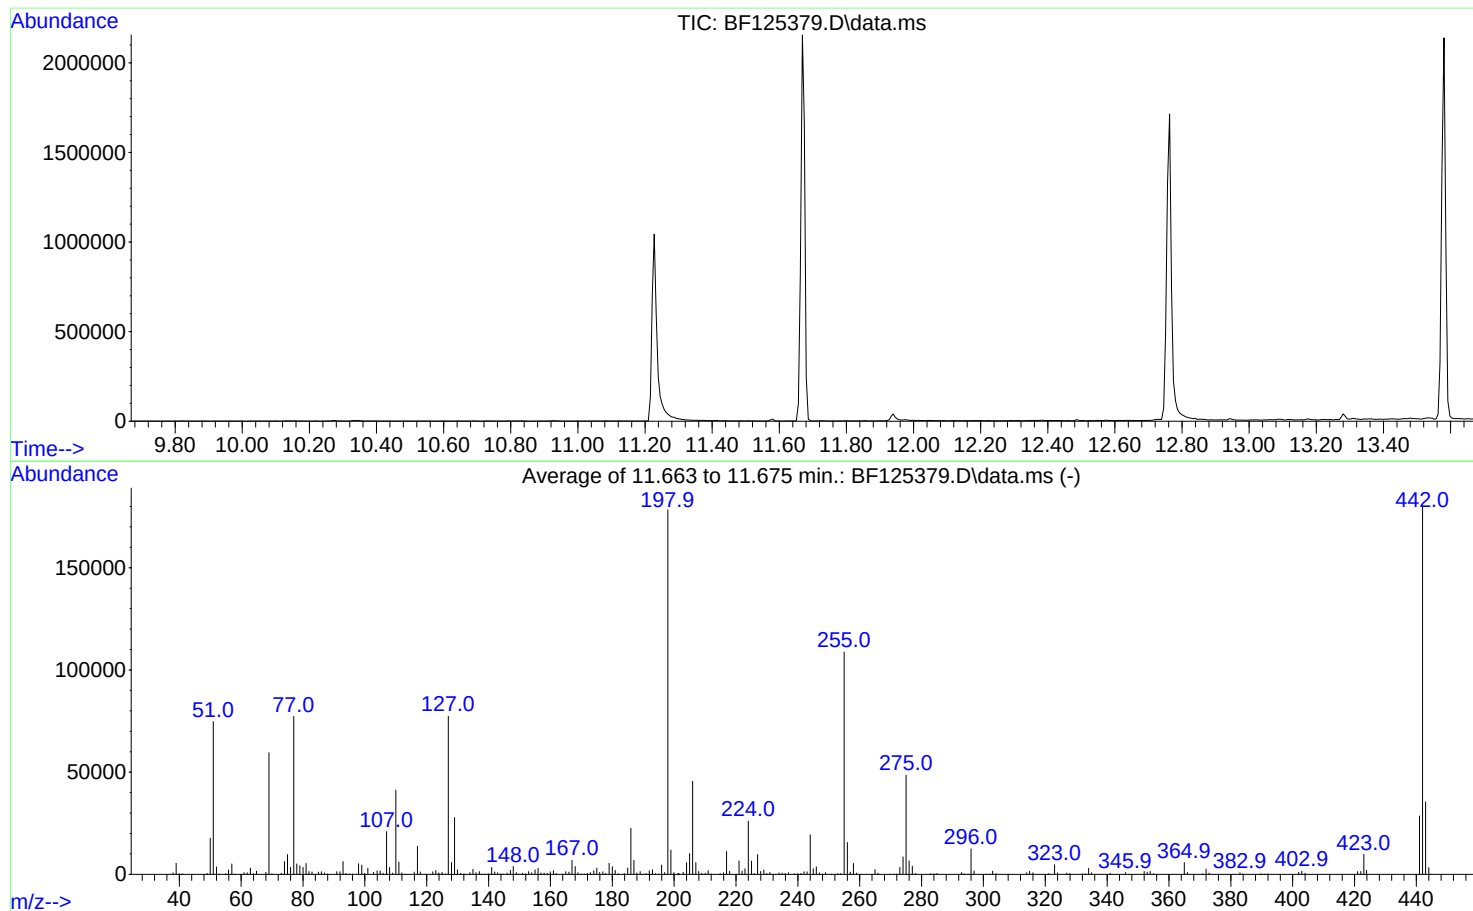




AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1623

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.9	74787	PASS
68	69	0.00	2	1.7	1027	PASS
69	198	0.00	100	33.4	59525	PASS
70	69	0.00	2	0.4	240	PASS
127	198	10	80	43.4	77365	PASS
197	198	0.00	2	0.5	876	PASS
198	198	100	100	100.0	178357	PASS
199	198	5	9	6.7	11918	PASS
275	198	10	60	27.2	48560	PASS
365	198	1	100	3.2	5733	PASS
441	198	0.01	100	16.0	28601	PASS
442	442	50	100	100.0	179979	PASS
443	442	15	24	19.7	35455	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090721\
 Data File : BF125379.D
 Acq On : 7 Sep 2021 9:47
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 07 12:01:18 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 03 11:56:34 2021
 Response via : Initial Calibration

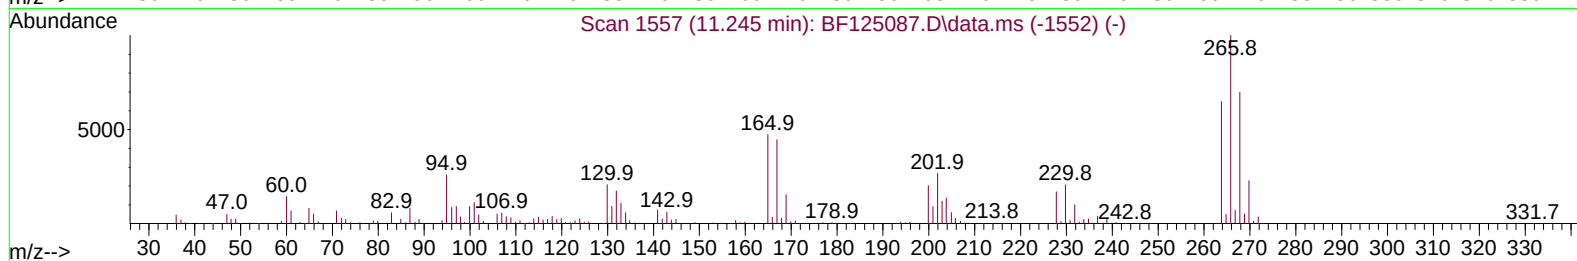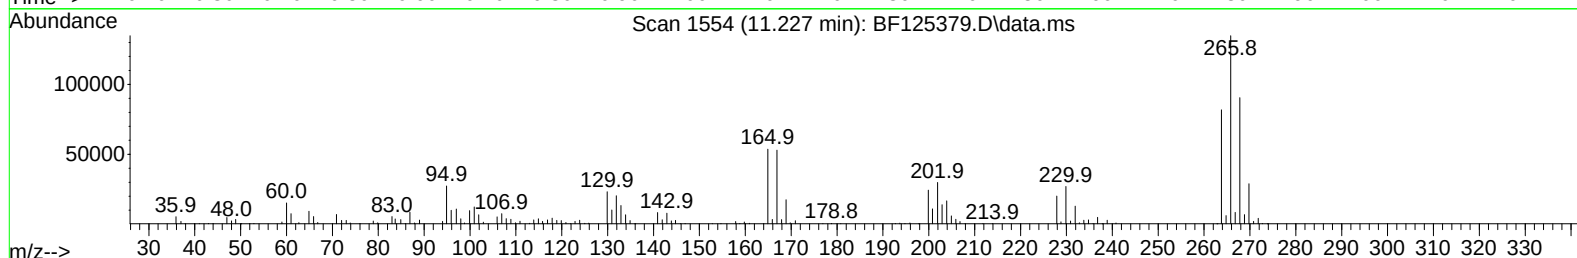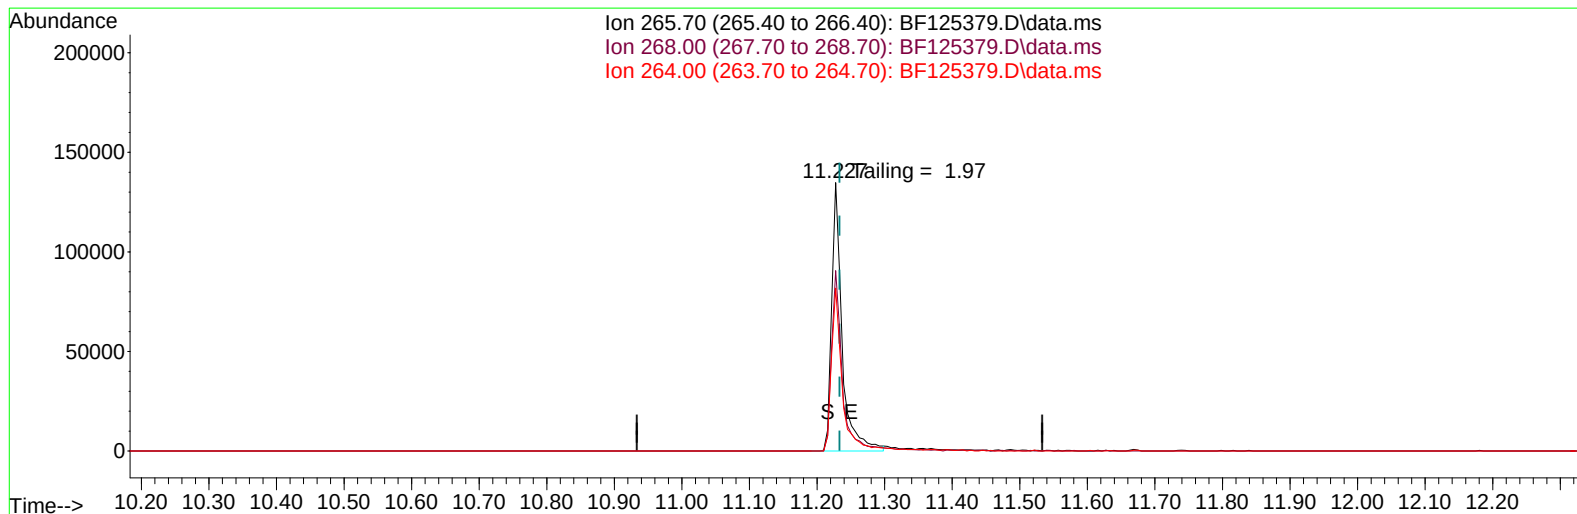

TIC: BF125379.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.006) 27595.61 ng




response 148092

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	67.17
264.00	69.90	60.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090721\
 Data File : BF125379.D
 Acq On : 7 Sep 2021 9:47
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 07 12:01:18 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 03 11:56:34 2021
 Response via : Initial Calibration

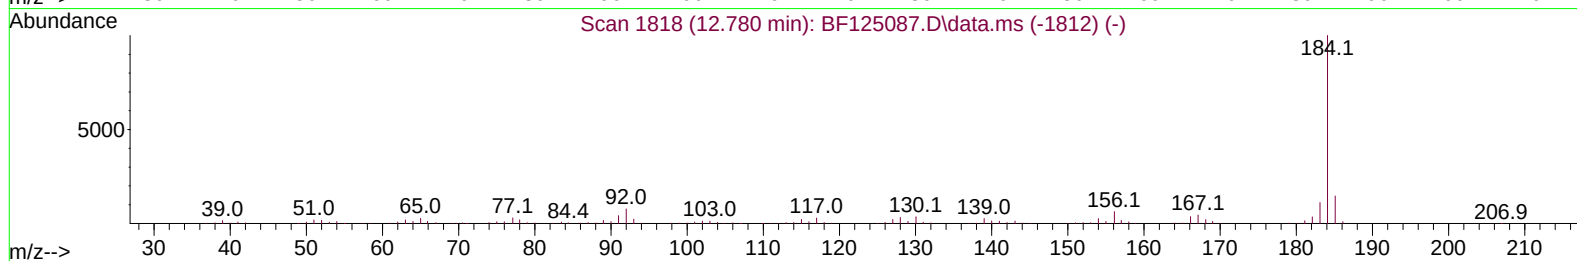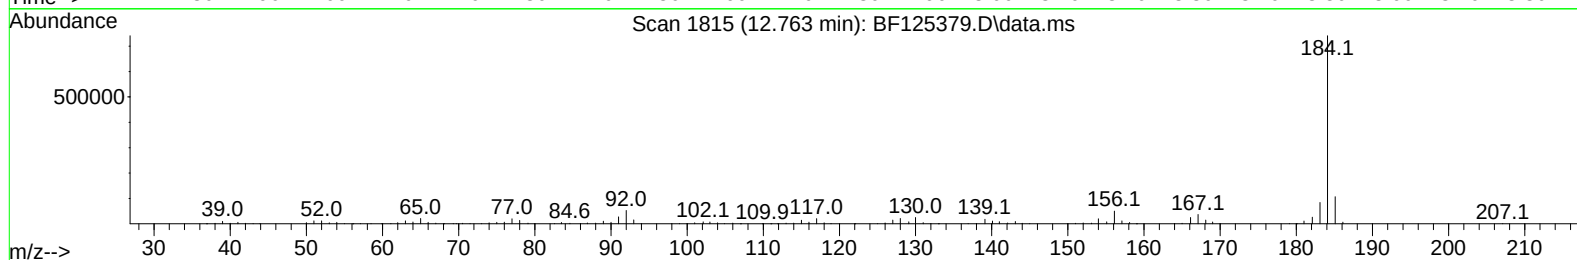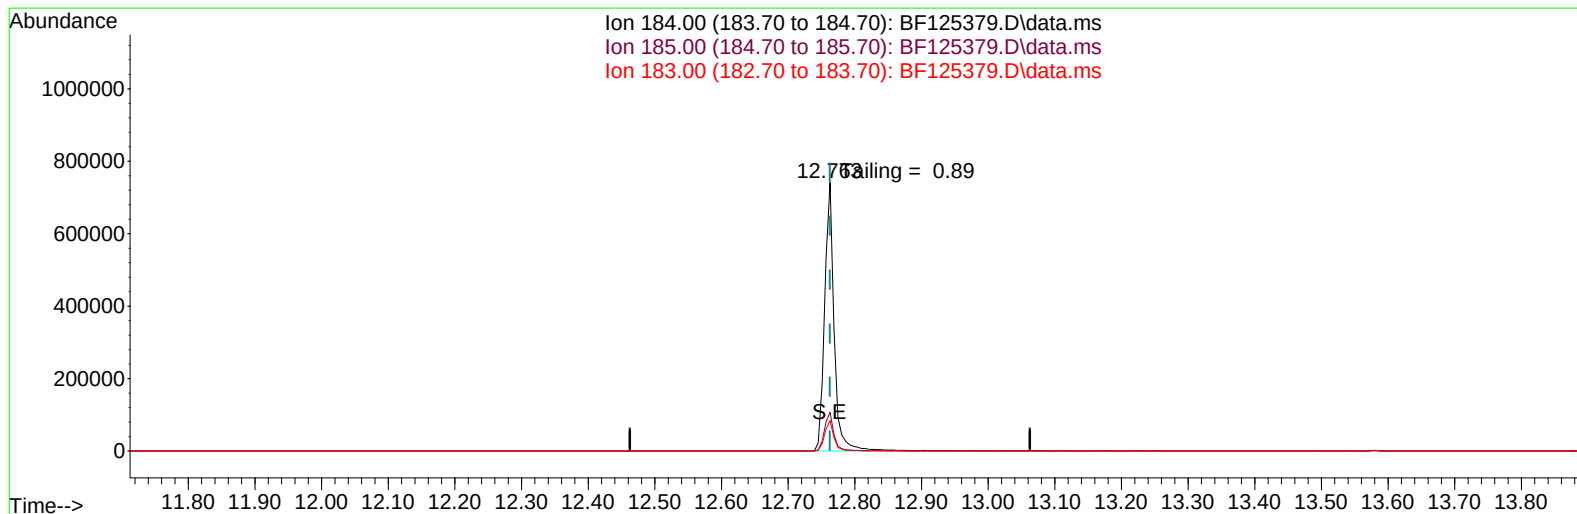

TIC: BF125379.D\data.ms

(77) Benzidine

12.763min (+ 0.000) 0.00 ng

response 735975

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.46
183.00	10.10	11.34
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/7/2021	BNA_F	<u>BF125379.D</u>
Compound Name	Response	Retention Time
DDT	359268	13.58
DDD	7101	13.28
DDE	1422	12.95
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8523	367791	2.32

Instrument :
BNA_F
ClientSampleId :
DFTPP