

Data Path : Z:\HPCHEM1\BNA F\Data\BF090815\
 Data File : BF081528.D
 Acq On : 8 Sep 2015 18:15
 Operator : UM/IZ
 Sample : G3472-02DL 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB002DL

Quant Time: Sep 08 18:45:03 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF090115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 08 15:49:53 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.34	152	49182	20.00	ng	0.00
21) Naphthalene-d8	7.63	136	195031	20.00	ng	-0.01
38) Acenaphthene-d10	9.37	164	84415	20.00	ng	-0.01
63) Phenanthrene-d10	10.83	188	165397	20.00	ng	-0.01
75) Chrysene-d12	13.45	240	107356	20.00	ng	0.00
86) Perylene-d12	14.75	264	86517	20.00	ng	0.00

System Monitoring Compounds						
5) 2-Fluorophenol	4.88	112	62086	19.59	ng	0.00
7) Phenol-d6	6.01	99	90447	21.56	ng	-0.01
23) Nitrobenzene-d5	6.92	82	53865	13.33	ng	0.00
41) 2,4,6-Tribromophenol	10.16	330	16267	21.64	ng	0.00
44) 2-Fluorobiphenyl	8.72	172	96227	14.61	ng	0.00
78) Terphenyl-d14	12.42	244	71537	15.51	ng	0.00


Target Compounds						Qvalue
19) n-Nitroso-di-n-propylamine	6.91	70	7255	2.54	ng	# 67
49) Dimethylphthalate	9.12	163	26079	3.98	ng	# 96
50) 2,6-Dinitrotoluene	9.37	165	11219	7.54	ng	# 37
51) Acenaphthene	9.40	154	11926	2.11	ng	92
55) 4-Nitrophenol	9.58	139	4561	4.28	ng	# 25
56) 2,4-Dinitrotoluene	9.37	165	11219	5.92	ng	# 31
57) Fluorene	9.92	166	13641	2.17	ng	95
70) Phenanthrene	10.87	178	190625	20.73	ng	97
71) Anthracene	10.91	178	50471	5.34	ng	98
72) Carbazole	11.07	167	23153	2.61	ng	# 96
74) Fluoranthene	12.03	202	262773	26.40	ng	90
77) Pyrene	12.26	202	218807	27.51	ng	98
80) Benzo(a)anthracene	13.44	228	121394	17.76	ng	96
82) Chrysene	13.44	228	121394	19.81	ng	97
85) Indeno(1,2,3-cd)pyrene	15.82	276	43048	9.57	ng	# 81
87) Benzo(b)fluoranthene	14.43	252	117872	19.08	ng	# 85
88) Benzo(k)fluoranthene	14.43	252	117872	23.00	ng	# 86
89) Benzo(a)pyrene	14.71	252	64619	12.35	ng	# 82
90) Dibenzo(a,h)anthracene	15.83	278	14582	3.61	ng	# 79
91) Benzo(a,h,i)perylene	16.14	276	39789	10.31	ng	# 74

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\Data\BF090815\
Data File : BF081528.D
Acq On : 8 Sep 2015 18:15
Operator : UM/IZ
Sample : G3472-02DL 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB002DL

Quant Time: Sep 08 18:45:03 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 08 15:49:53 2015
Response via : Initial Calibration

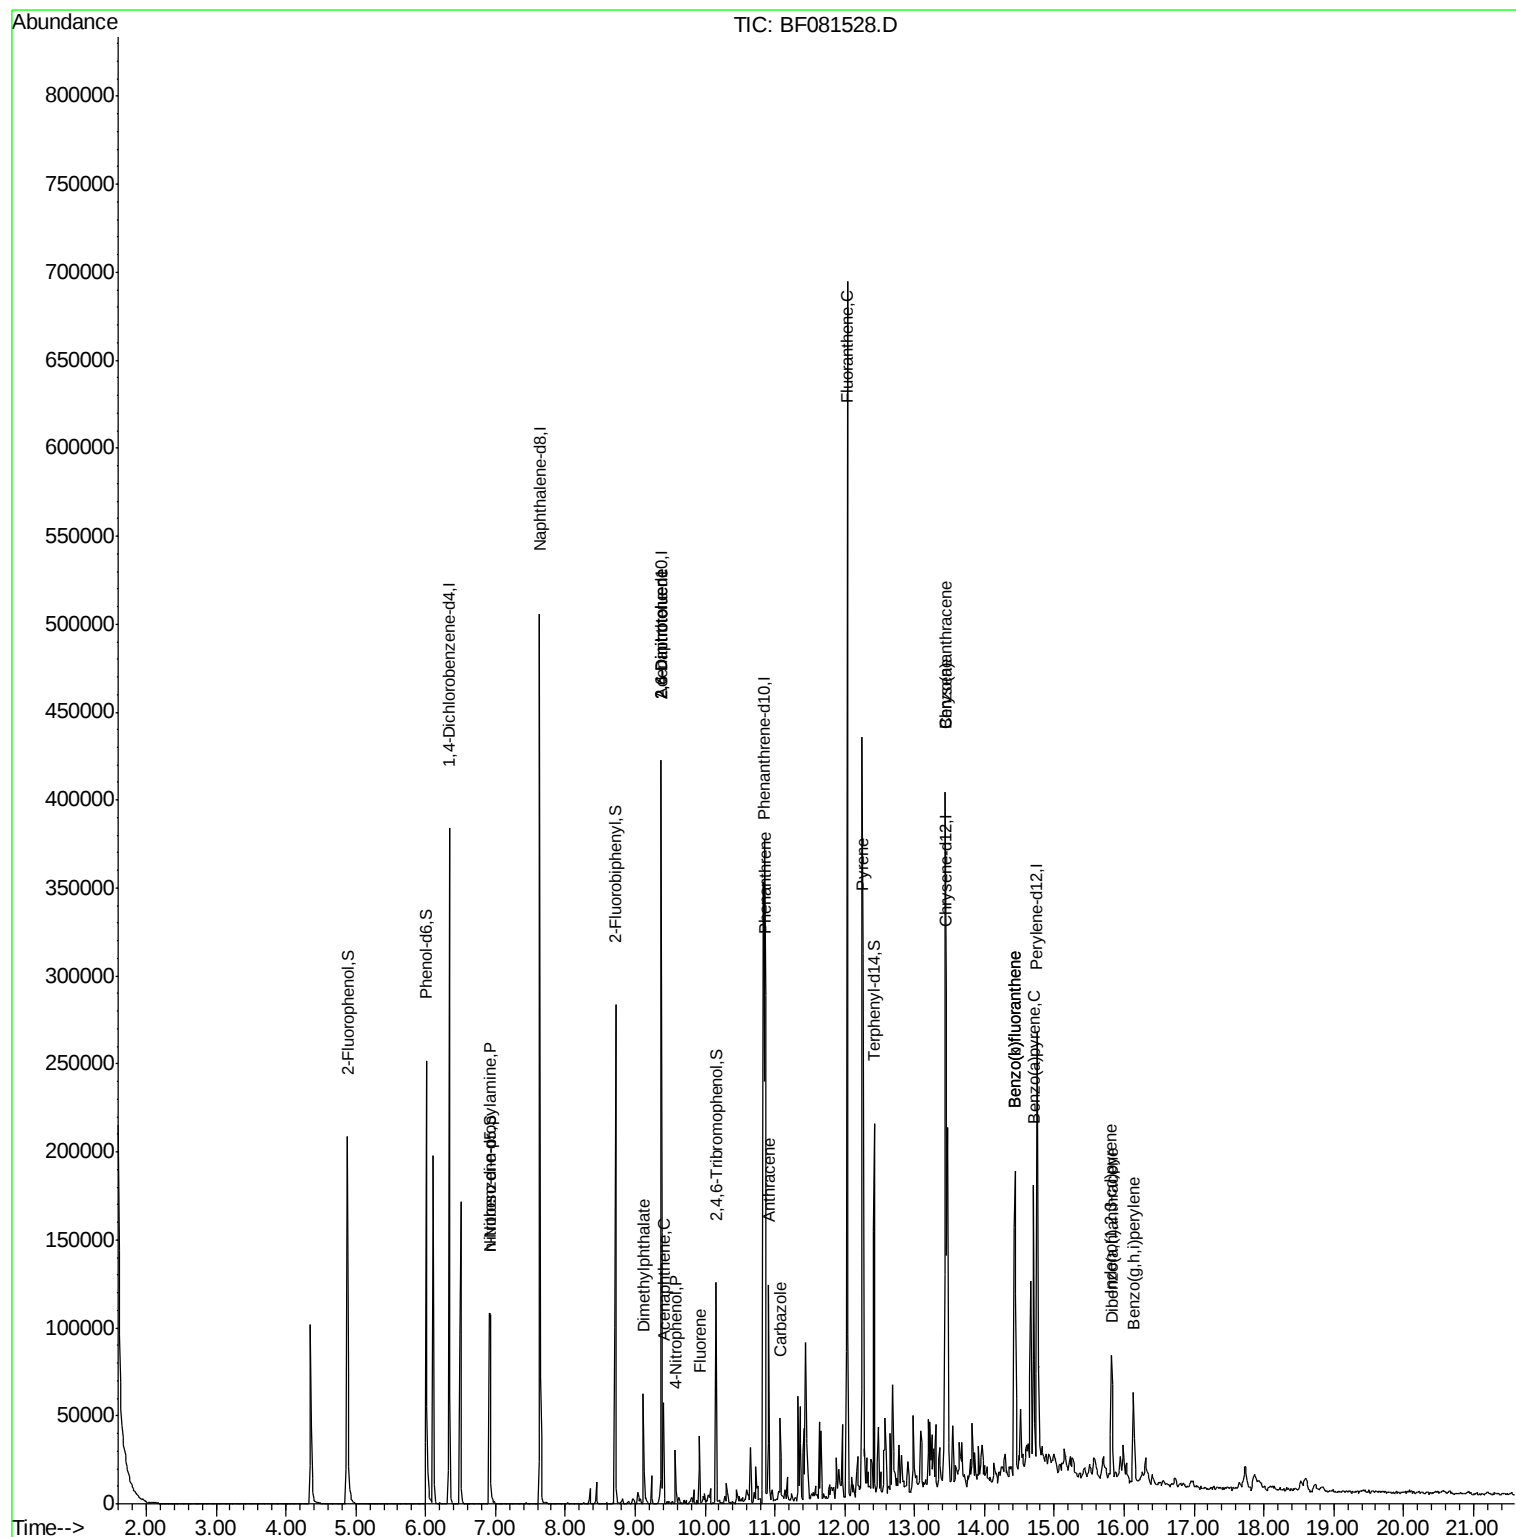




#1



1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.34 min Scan# 416
Delta R.T. -0.00 min
Lab File: BF081528.D
Acq: 8 Sep 2015 18:15

Instrument :
BNA_F
ClientSampleId :
SB002DL

Tot Ion:152 Resp: 49182
Ion Ratio Lower Upper
152 100
150 161.1 124.7 187.1
115 67.3 39.0 58.4#




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

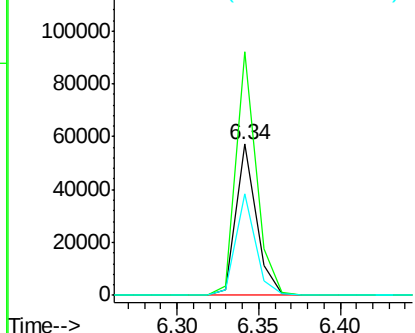



#5



2-Fluorophenol
Concen: 19.59 ng
RT: 4.88 min Scan# 288
Delta R.T. -0.00 min
Lab File: BF081528.D
Acq: 8 Sep 2015 18:15

Tgt Ion:112 Resp: 62086
Ion Ratio Lower Upper
112 100
64 74.5 39.7 59.5#
63 40.6 17.4 26.0#



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

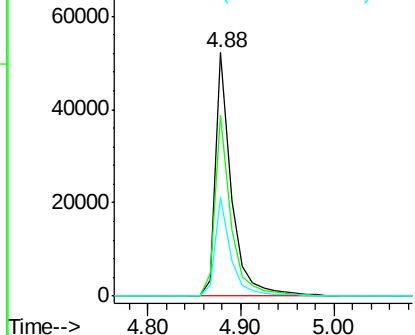

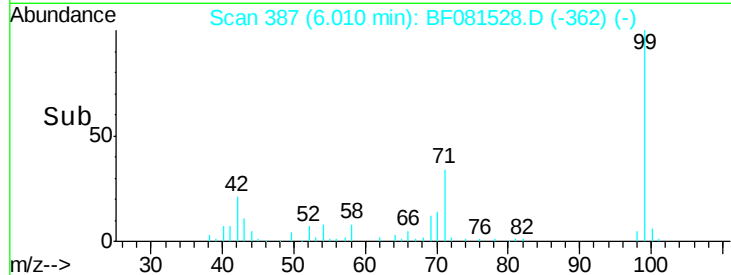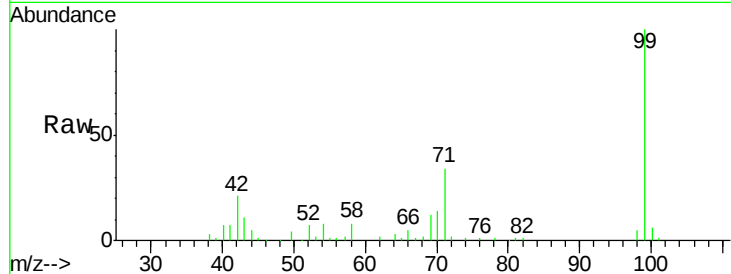

#7

Phenol-d6

Concen: 21.56 ng

RT: 6.01 min Scan# 387

Delta R.T. -0.01 min

Lab File: BF081528.D

Acq: 8 Sep 2015 18:15

Instrument :

BNA_F

ClientSampleId :

SB002DL





Tot Ion: 99 Resp: 90447

Ion Ratio Lower Upper

99 100

42 20.6 13.7 20.5#

71 34.0 14.2 21.2#

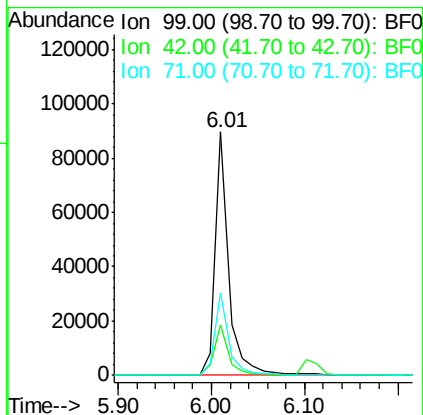

#19

n-Nitroso-di-n-propylamine

Concen: 2.54 ng

RT: 6.91 min Scan# 466

Delta R.T. 0.11 min

Lab File: BF081528.D

Acq: 8 Sep 2015 18:15

Tgt Ion: 70 Resp: 7255


Ion Ratio Lower Upper

70 100

42 59.9 63.8 95.6#

101 0.0 9.2 13.8#

130 0.0 27.3 40.9#

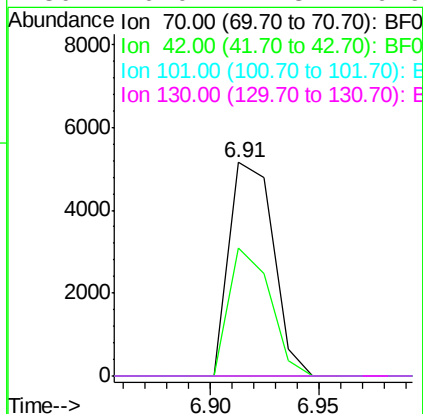



#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.63 min Scan# 529

Delta R.T. -0.01 min

Lab File: BF081528.D

Acq: 8 Sep 2015 18:15

Instrument :

BNA_F

ClientSampleId :

SB002DL

Tot Ion:136 Resp: 195031


Ion Ratio Lower Upper

136 100

137 10.6 9.0 13.6

54 12.7 8.2 12.2#

68 5.7 5.8 8.6#





Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

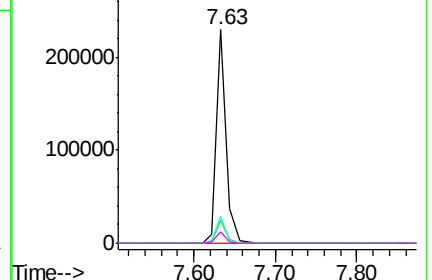

#23

Nitrobenzene-d5

Concen: 13.33 ng

RT: 6.92 min Scan# 467

Delta R.T. -0.00 min

Lab File: BF081528.D

Acq: 8 Sep 2015 18:15


Tgt Ion: 82 Resp: 53865

Ion Ratio Lower Upper

82 100

128 46.0 51.0 76.6#



54 58.1 47.5 71.3




Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

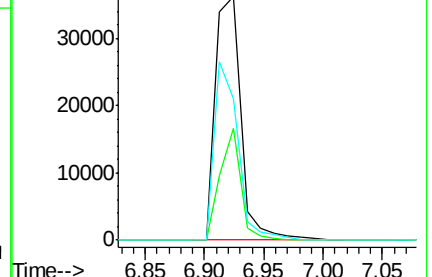







#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.37 min Scan# 681
Delta R.T. -0.01 min
Lab File: BF081528.D
Acq: 8 Sep 2015 18:15

Instrument :
BNA_F
ClientSampled :
SB002DL

Tot Ion:164 Resp: 84415
Ion Ratio Lower Upper
164 100
162 103.9 75.2 112.8
160 45.9 31.5 47.3




Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E


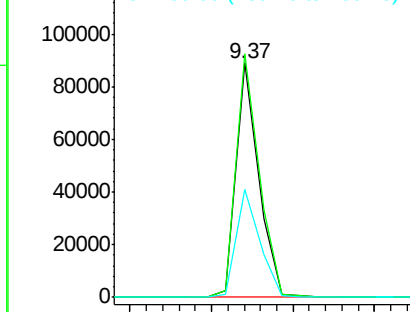



#41
2,4,6-Tribromophenol
Concen: 21.64 ng
RT: 10.16 min Scan# 750
Delta R.T. -0.00 min
Lab File: BF081528.D
Acq: 8 Sep 2015 18:15

Tgt Ion:330 Resp: 16267
Ion Ratio Lower Upper
330 100
332 94.7 76.6 114.8
141 49.2 29.7 44.5#



Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E




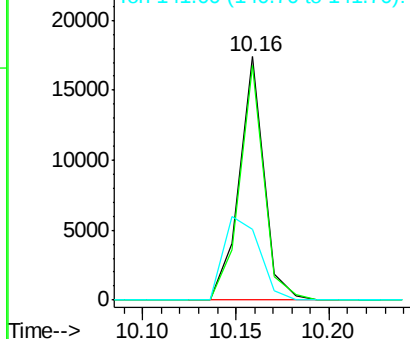


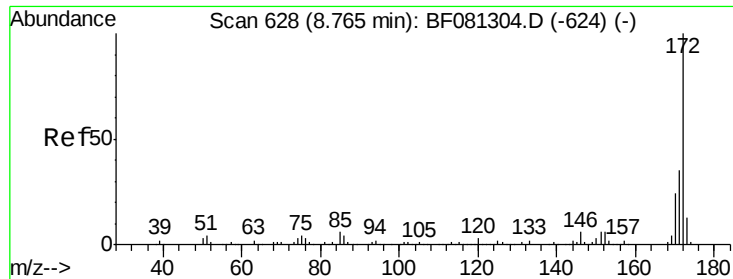

#44
2-Fluorobiphenyl
Concen: 14.61 ng
RT: 8.72 min Scan# 624
Delta R.T. -0.00 min
Lab File: BF081528.D
Acq: 8 Sep 2015 18:15




Instrument :
BNA_F
ClientSampleId :
SB002DL


Tot Ion:172 Resp: 96227
Ion Ratio Lower Upper
172 100
171 34.2 26.1 39.1
170 23.2 17.4 26.2

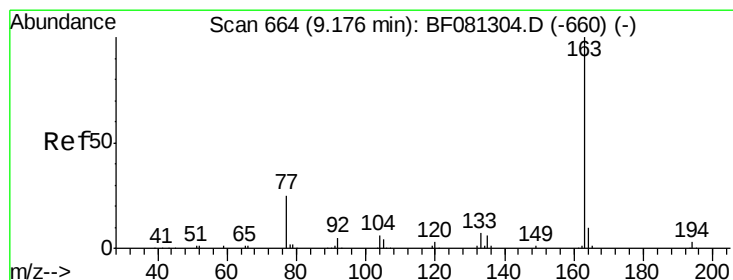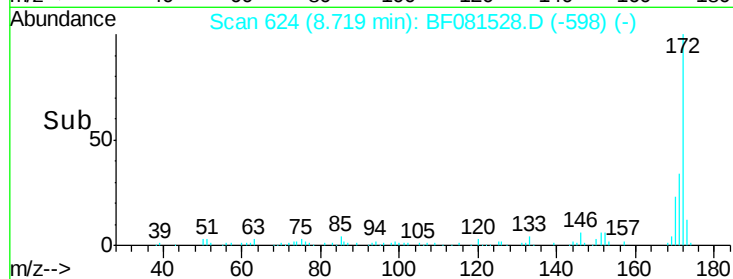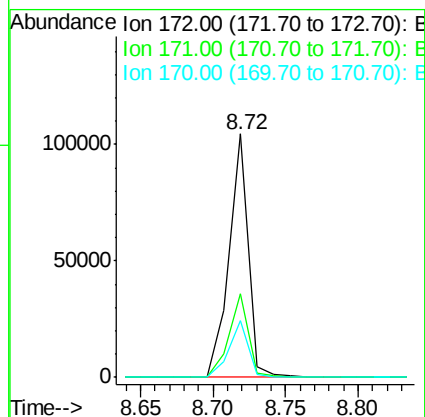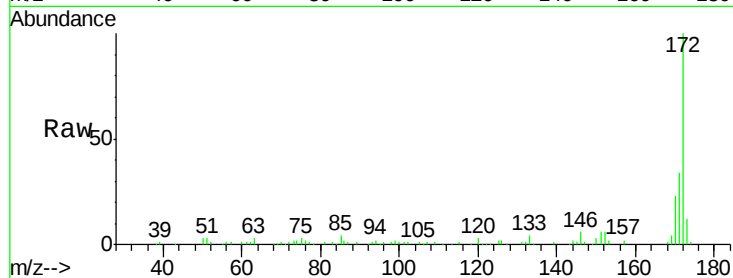

#49
Dimethylphthalate
Concen: 3.98 ng
RT: 9.12 min Scan# 659
Delta R.T. -0.02 min
Lab File: BF081528.D
Acq: 8 Sep 2015 18:15

Tgt Ion:163 Resp: 26079
Ion Ratio Lower Upper
163 100
194 2.5 4.4 6.6#
164 10.0 8.3 12.5

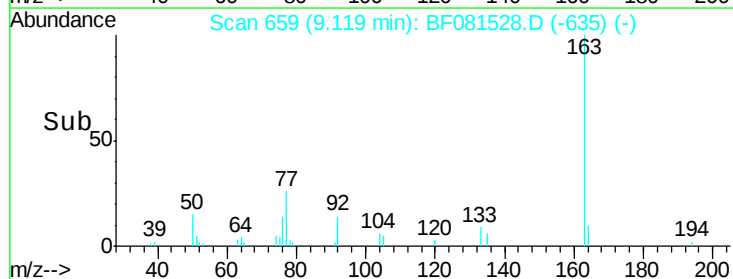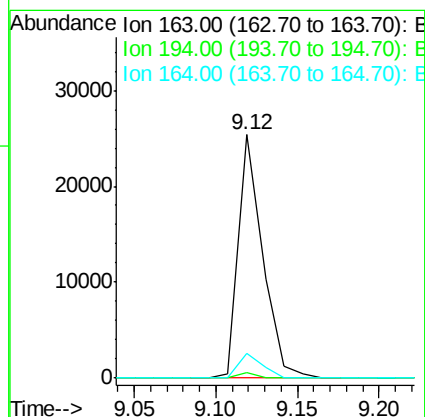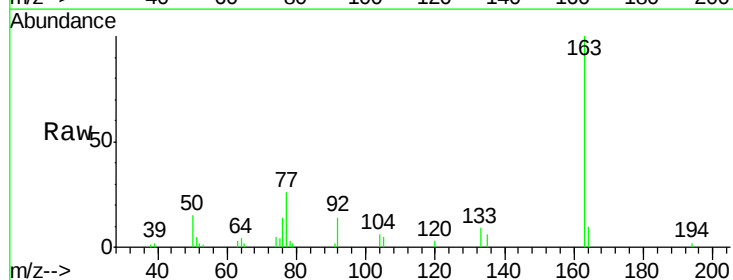



#50

2,6-Dinitrotoluene

Concen: 7.54 ng

RT: 9.37 min Scan# 681

Delta R.T. 0.17 min

Lab File: BF081528.D

Acq: 8 Sep 2015 18:15

Instrument :

BNA_F

ClientSampleId :

SB002DL


Tot Ion:165 Resp: 11219

Ion Ratio Lower Upper

165 100

63 0.0 32.3 48.5#




89 0.0 28.6 43.0#



Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

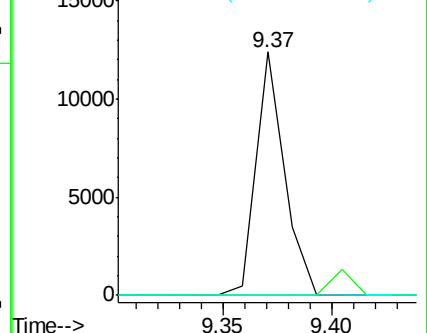

#51

Acenaphthene

Concen: 2.11 ng

RT: 9.40 min Scan# 684

Delta R.T. -0.01 min

Lab File: BF081528.D

Acq: 8 Sep 2015 18:15


Tgt Ion:154 Resp: 11926

Ion Ratio Lower Upper

154 100

153 112.4 82.1 123.1



152 51.1 37.9 56.9




Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

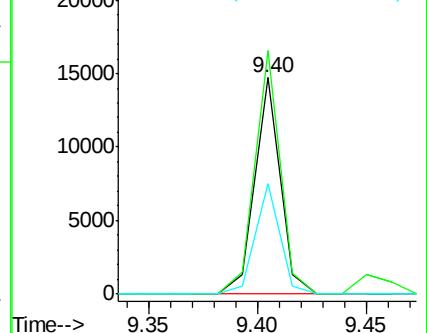







#55
4-Nitrophenol
Concen: 4.28 ng
RT: 9.58 min Scan# 699
Delta R.T. -0.01 min
Lab File: BF081528.D
Acq: 8 Sep 2015 18:15

Instrument :
BNA_F
ClientSampleId :
SB002DL

Tot Ion	Ratio	Lower	Upper
139	100		
109	0.0	12.7	52.7#
65	0.0	45.9	85.9#






Abundance Ion 139.00 (138.70 to 139.70): E
Ion 109.00 (108.70 to 109.70): E
Ion 65.00 (64.70 to 65.70): BF0

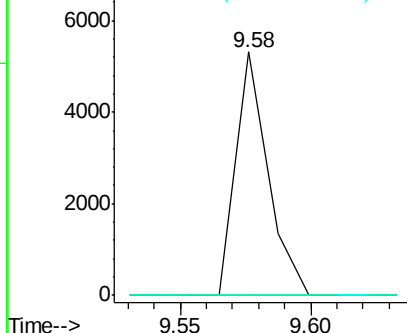


#56
2,4-Dinitrotoluene
Concen: 5.92 ng
RT: 9.37 min Scan# 681
Delta R.T. -0.22 min
Lab File: BF081528.D
Acq: 8 Sep 2015 18:15

Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	29.8	44.6#
89	0.0	44.5	66.7#
182	0.0	3.0	4.4#

Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BF0
Ion 89.00 (88.70 to 89.70): BF0
Ion 182.00 (181.70 to 182.70): E

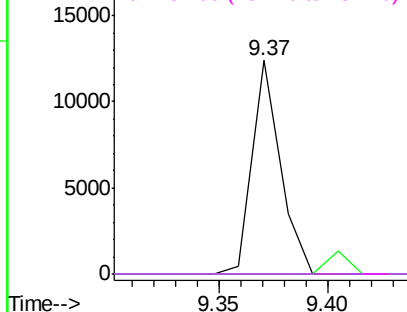


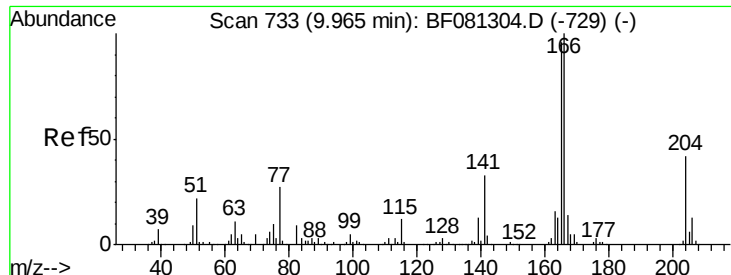




#57
Fluorene
 Concen: 2.17 ng
 RT: 9.92 min Scan# 729
 Delta R.T. -0.00 min
 Lab File: BF081528.D
 Acq: 8 Sep 2015 18:15

Instrument :
 BNA_F
 ClientSampleID :
 SB002DL

Tot Ion:166 Resp: 13641
 Ion Ratio Lower Upper
 166 100
 165 86.5 72.6 109.0
 167 15.1 10.6 16.0




Abundance Ion 166.00 (165.70 to 166.70): E
 Ion 165.00 (164.70 to 165.70): E
 Ion 167.00 (166.70 to 167.70): E

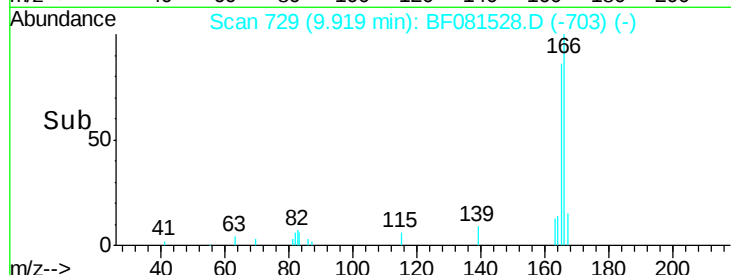
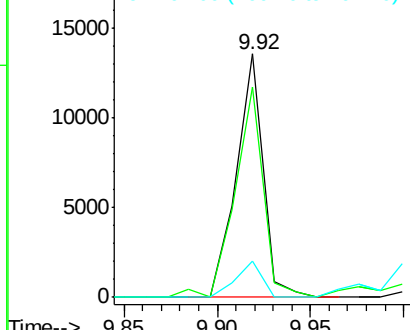



#63
Phenanthrene-d10
 Concen: 20.00 ng
 RT: 10.83 min Scan# 809
 Delta R.T. -0.01 min
 Lab File: BF081528.D
 Acq: 8 Sep 2015 18:15

Tgt Ion:188 Resp: 165397
 Ion Ratio Lower Upper
 188 100
 94 10.8 11.1 16.7#
 80 12.3 11.0 16.4



Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF0
 Ion 80.00 (79.70 to 80.70): BF0

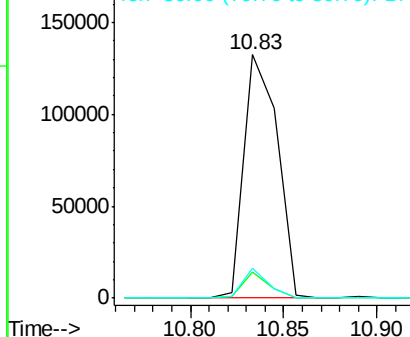







#70
Phenanthrene
Concen: 20.73 ng
RT: 10.87 min Scan# 812
Delta R.T. -0.00 min
Lab File: BF081528.D
Acq: 8 Sep 2015 18:15

Instrument :
BNA_F
ClientSampleId :
SB002DL

Tot Ion:178 Resp: 190625
Ion Ratio Lower Upper
178 100
176 19.0 13.8 20.8
179 14.5 12.2 18.2




Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E

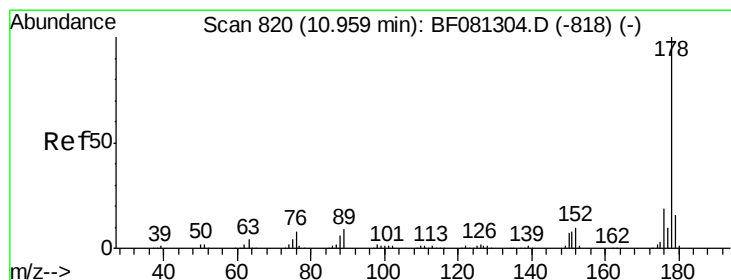
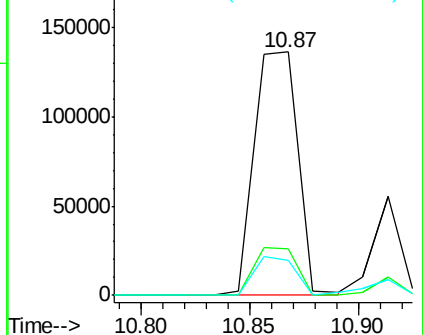



#71
Anthracene
Concen: 5.34 ng
RT: 10.91 min Scan# 816
Delta R.T. -0.00 min
Lab File: BF081528.D
Acq: 8 Sep 2015 18:15

Tgt Ion:178 Resp: 50471
Ion Ratio Lower Upper
178 100
176 18.1 14.1 21.1
179 16.3 12.2 18.2

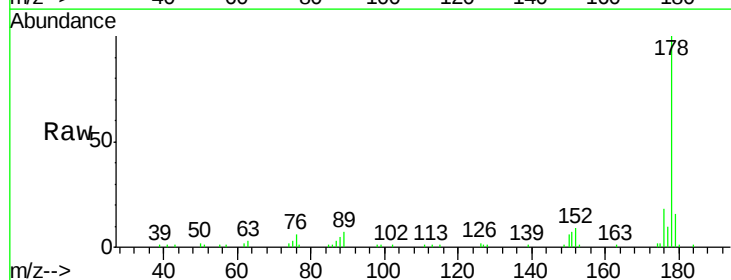

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E

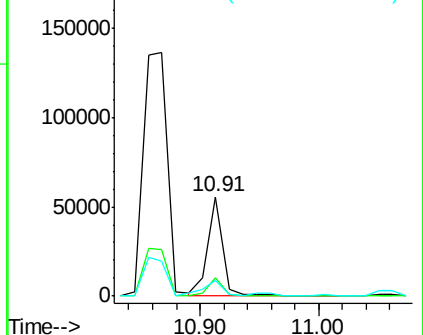

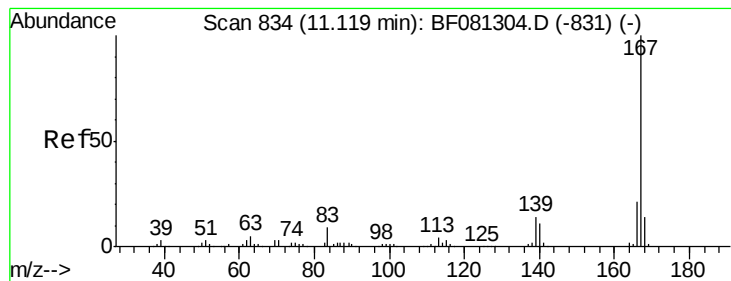

#72

Carbazole

Concen: 2.61 ng

RT: 11.07 min Scan# 830

Delta R.T. -0.01 min

Lab File: BF081528.D

Acq: 8 Sep 2015 18:15

Instrument :

BNA_F

ClientSampleId :

SB002DL


Tot Ion:167 Resp: 23153

Ion Ratio Lower Upper

167 100

166 20.0 15.7 23.5




139 16.0 9.5 14.3#

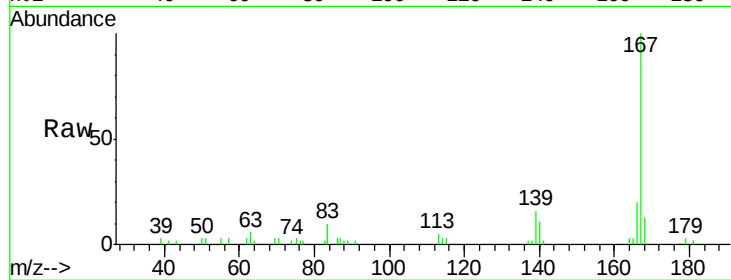

Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

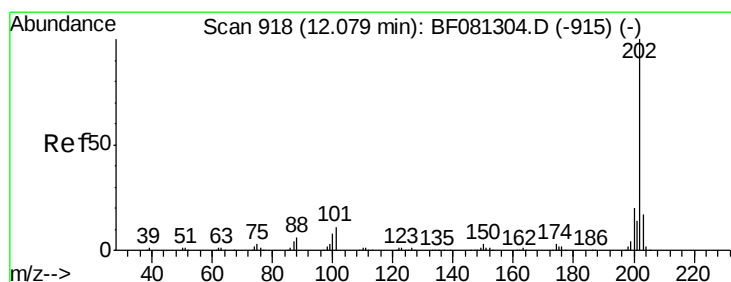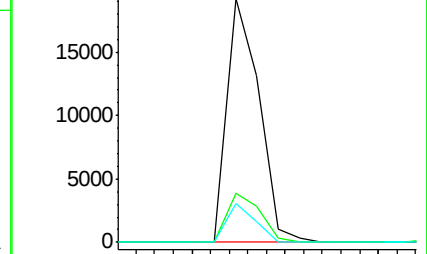

#74

Fluoranthene

Concen: 26.40 ng

RT: 12.03 min Scan# 914

Delta R.T. -0.00 min

Lab File: BF081528.D

Acq: 8 Sep 2015 18:15


Tgt Ion:202 Resp: 262773

Ion Ratio Lower Upper

202 100

101 9.7 0.0 38.3



203 17.5 0.0 37.3

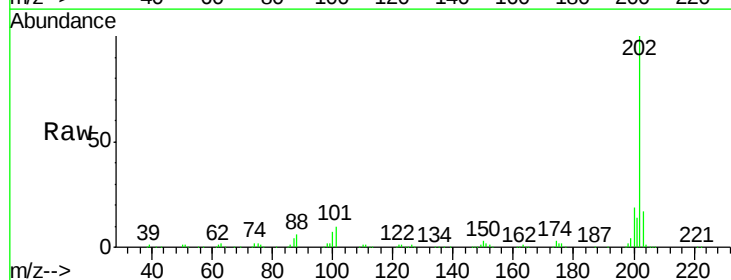


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

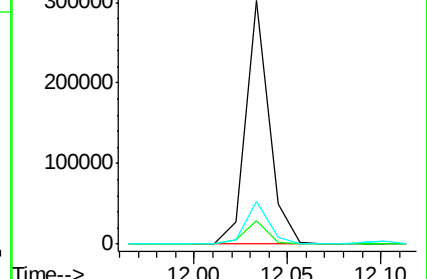







#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.45 min Scan# 1038
Delta R.T. -0.00 min
Lab File: BF081528.D
Acq: 8 Sep 2015 18:15

Instrument :
BNA_F
ClientSampleId :
SB002DL

Tot Ion:240 Resp: 107356
Ion Ratio Lower Upper
240 100
120 5.6 16.2 24.2#
236 25.7 18.4 27.6




Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

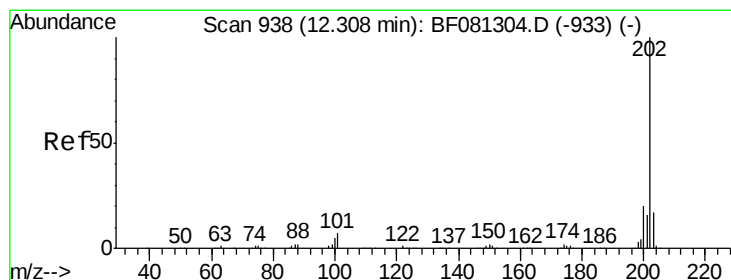
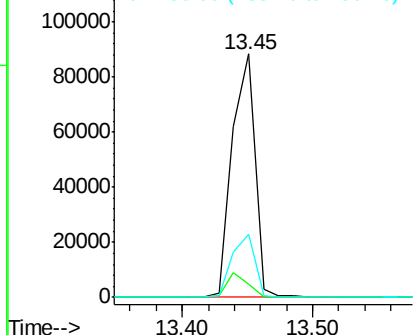



#77
Pyrene
Concen: 27.51 ng
RT: 12.26 min Scan# 934
Delta R.T. -0.00 min
Lab File: BF081528.D
Acq: 8 Sep 2015 18:15

Tgt Ion:202 Resp: 218807
Ion Ratio Lower Upper
202 100
200 19.9 15.0 22.4
203 16.9 14.1 21.1



Abundance Ion 202.00 (201.70 to 202.70): E
Ion 200.00 (199.70 to 200.70): E
Ion 203.00 (202.70 to 203.70): E

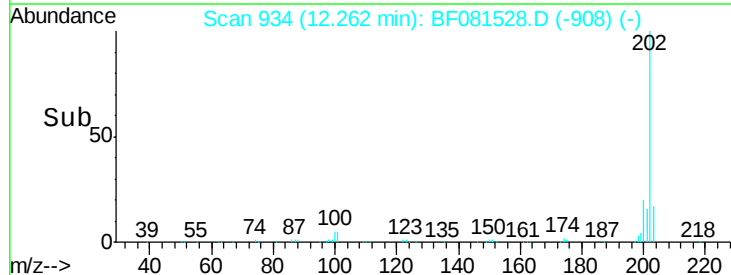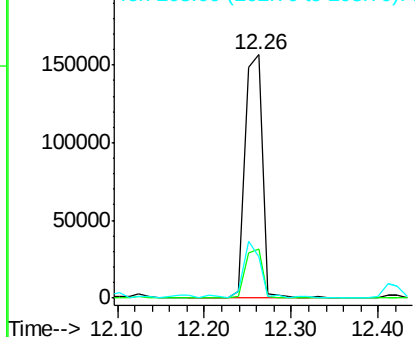



#78

Terphenyl-d14

Concen: 15.51 ng

RT: 12.42 min Scan# 948

Delta R.T. -0.00 min

Lab File: BF081528.D

Acq: 8 Sep 2015 18:15

Instrument :

BNA_F

ClientSampleId :

SB002DL


Tot Ion:244 Resp: 71537

Ion Ratio Lower Upper

244 100

212 7.3 4.3 6.5#




122 6.5 17.4 26.2#



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

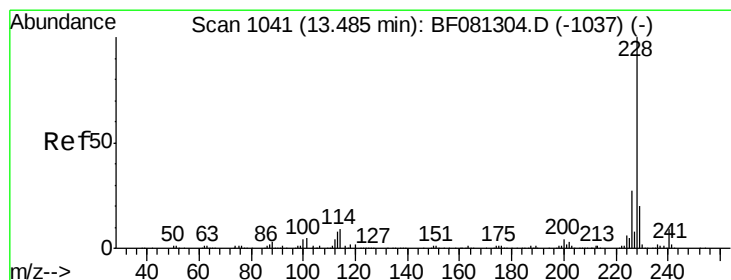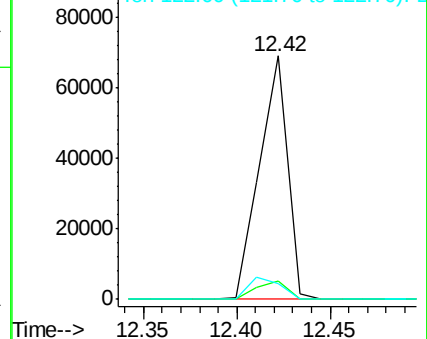

#80

Benzo(a)anthracene

Concen: 17.76 ng

RT: 13.44 min Scan# 1037

Delta R.T. -0.00 min

Lab File: BF081528.D

Acq: 8 Sep 2015 18:15


Tgt Ion:228 Resp: 121394

Ion Ratio Lower Upper

228 100

226 27.9 20.0 30.0



229 20.5 15.4 23.2




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

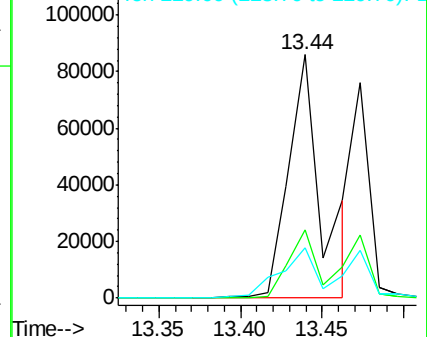



#82

Chrysene

Concen: 19.81 ng

RT: 13.44 min Scan# 1037

Delta R.T. -0.03 min

Lab File: BF081528.D

Acq: 8 Sep 2015 18:15

Instrument :

BNA_F

ClientSampleID :

SB002DL


Tot Ion:228 Resp: 121394

Ion Ratio Lower Upper

228 100

226 27.9 21.0 31.4




229 20.5 15.6 23.4



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

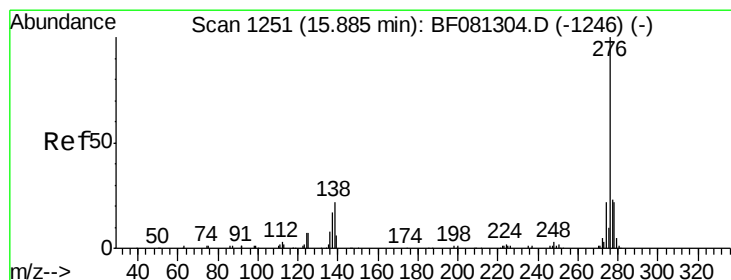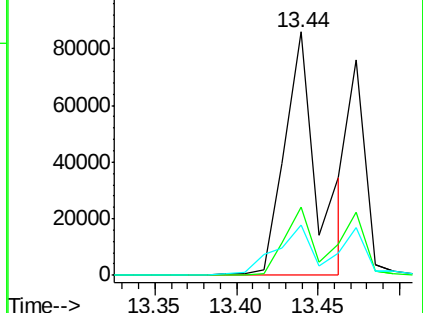

#85

Indeno(1,2,3-cd)pyrene

Concen: 9.57 ng

RT: 15.82 min Scan# 1245

Delta R.T. -0.01 min

Lab File: BF081528.D

Acq: 8 Sep 2015 18:15


Tgt Ion:276 Resp: 43048

Ion Ratio Lower Upper

276 100

138 21.6 25.7 38.5#



277 28.7 15.6 23.4#




Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E



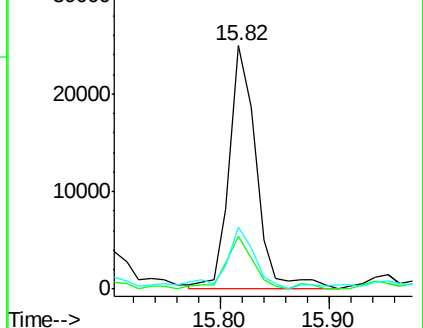



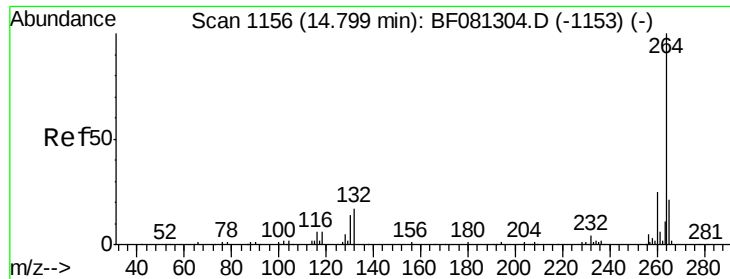

#86
Pervlene-d12
Concen: 20.00 ng
RT: 14.75 min Scan# 1152
Delta R.T. -0.00 min
Lab File: BF081528.D
Acq: 8 Sep 2015 18:15




Instrument :
BNA_F
ClientSampleId :
SB002DL


Tot Ion:264 Resp: 86517
Ion Ratio Lower Upper
264 100
260 24.7 16.7 25.1
265 22.1 17.2 25.8

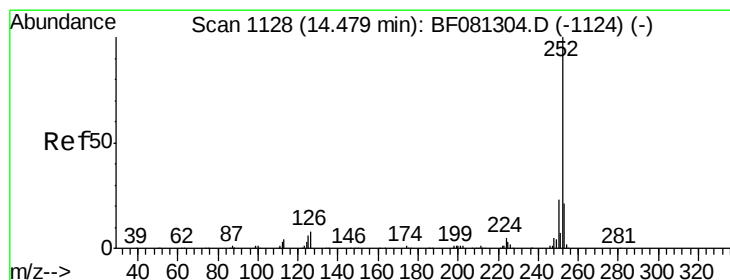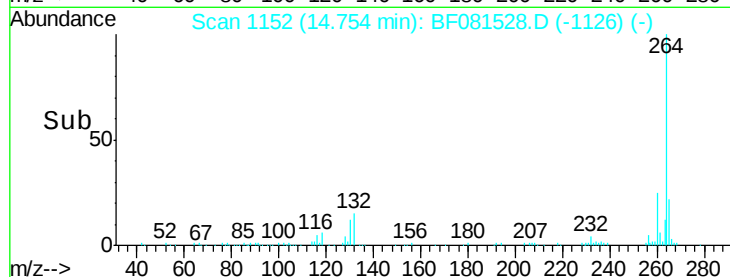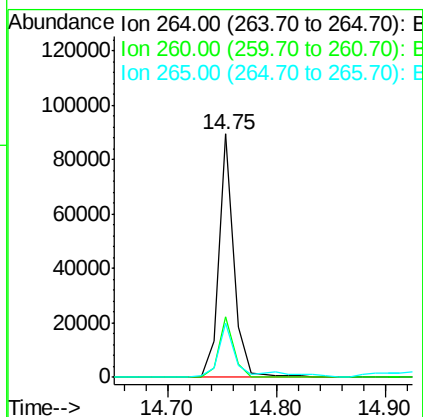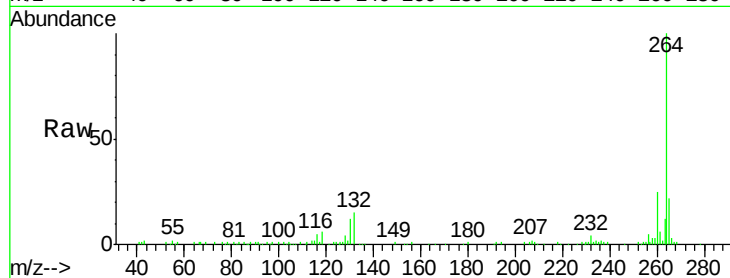

#87
Benzo(b)fluoranthene
Concen: 19.08 ng
RT: 14.43 min Scan# 1124
Delta R.T. -0.00 min
Lab File: BF081528.D
Acq: 8 Sep 2015 18:15

Tgt Ion:252 Resp: 117872
Ion Ratio Lower Upper
252 100
253 23.1 17.5 26.3
125 8.5 17.1 25.7#


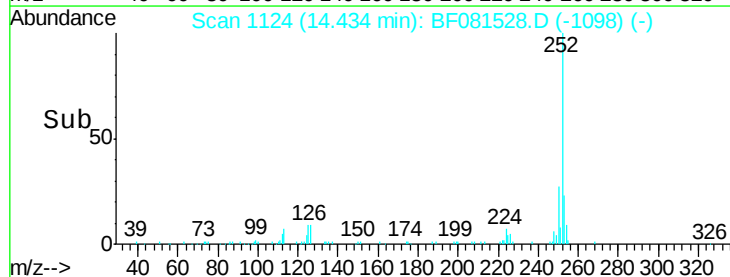
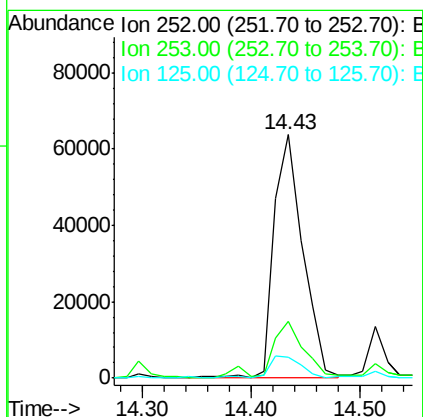
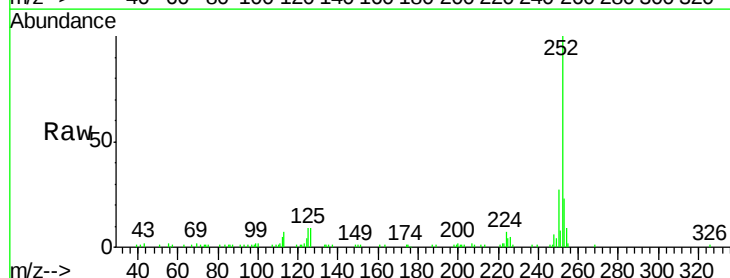




#88
Benzo(k)fluoranthene
Concen: 23.00 ng
RT: 14.43 min Scan# 1124
Delta R.T. -0.02 min
Lab File: BF081528.D
Acq: 8 Sep 2015 18:15




Instrument :
BNA_F
ClientSampleId :
SB002DL


Tot Ion:252 Resp: 117872
Ion Ratio Lower Upper
252 100
253 23.1 17.0 25.4
125 8.5 16.0 24.0#

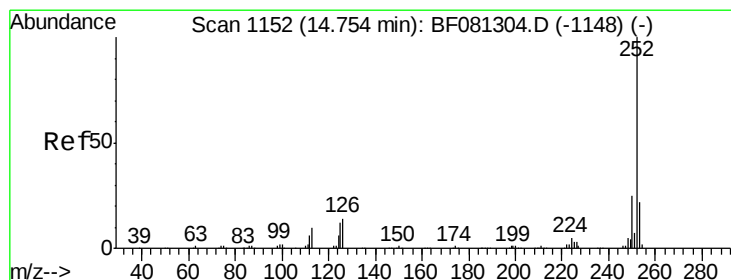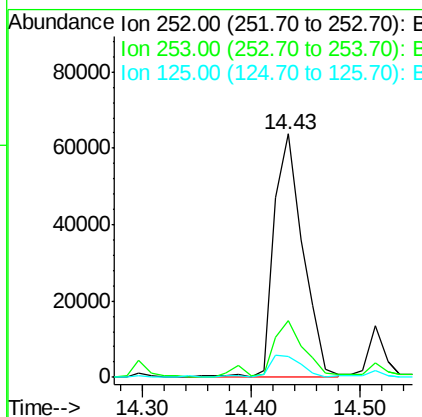

#89
Benzo(a)pyrene
Concen: 12.35 ng
RT: 14.71 min Scan# 1148
Delta R.T. -0.00 min
Lab File: BF081528.D
Acq: 8 Sep 2015 18:15

Tgt Ion:252 Resp: 64619
Ion Ratio Lower Upper
252 100
253 23.1 17.2 25.8
125 7.0 18.0 27.0#


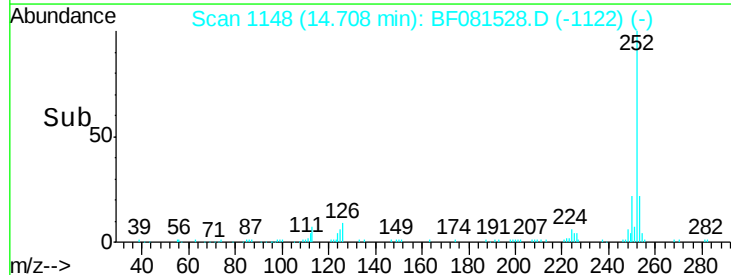
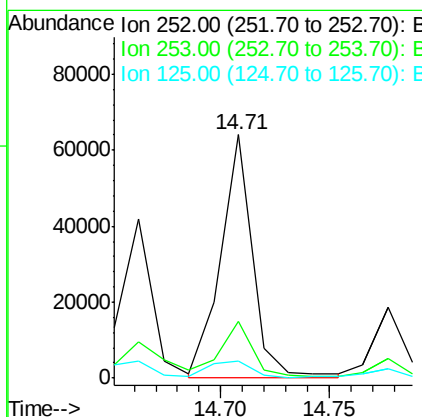





#90
Dibenzo(a,h)anthracene
Concen: 3.61 ng
RT: 15.83 min Scan# 1246
Delta R.T. -0.01 min
Lab File: BF081528.D
Acq: 8 Sep 2015 18:15

Instrument :
BNA_F
ClientSampleId :
SB002DL

Tot Ion:278 Resp: 14582
Ion Ratio Lower Upper
278 100
139 19.5 26.3 39.5#
279 31.0 18.2 27.4#

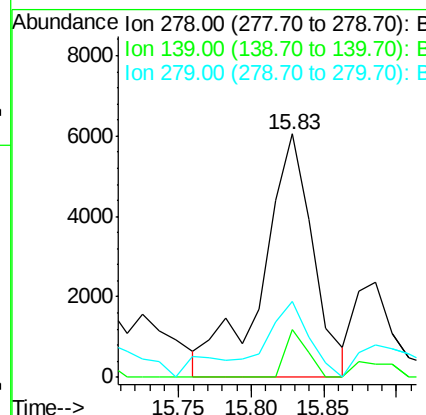

#91
Benzo(g,h,i)perylene
Concen: 10.31 ng
RT: 16.14 min Scan# 1273
Delta R.T. -0.00 min
Lab File: BF081528.D
Acq: 8 Sep 2015 18:15

Tgt Ion:276 Resp: 39789
Ion Ratio Lower Upper
276 100
277 24.0 17.8 26.6
138 19.2 34.6 51.8#

