

Data Path : Z:\HPCHEM1\BNA F\DATA\BF090815\
 Data File : BF081541.D
 Acq On : 9 Sep 2015 2:37
 Operator : UM/IZ
 Sample : G3585-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MGP212BR-20-23

Quant Time: Sep 09 03:33:34 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF090115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 09 03:32:15 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.34	152	50038	20.00	ng	-0.01
21) Naphthalene-d8	7.63	136	190721	20.00	ng	-0.01
38) Acenaphthene-d10	9.37	164	84001	20.00	ng	-0.01
63) Phenanthrene-d10	10.83	188	149017	20.00	ng	-0.01
75) Chrysene-d12	13.44	240	104447	20.00	ng	-0.01
86) Perylene-d12	14.75	264	101373	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	4.89	112	392782	121.79	ng	0.01
7) Phenol-d6	6.02	99	620766	145.41	ng	0.00
23) Nitrobenzene-d5	6.92	82	349429	88.40	ng	-0.01
41) 2,4,6-Tribromophenol	10.16	330	88310	118.07	ng	0.00
44) 2-Fluorobiphenyl	8.72	172	495769	75.63	ng	0.00
78) Terphenyl-d14	12.42	244	324866	72.40	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	6.92	70	48265	16.61	ng	# 64
25) Isophorone	6.92	82	270839	36.84	ng	# 58
49) Dimethylphthalate	9.12	163	139755	21.41	ng	# 97
56) 2,4-Dinitrotoluene	9.37	165	11326	6.00	ng	# 31
66) 4-Bromophenyl-phenylether	10.16	248	7190	4.77	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF090815\
Data File : BF081541.D
Acq On : 9 Sep 2015 2:37
Operator : UM/IZ
Sample : G3585-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MGP212BR-20-23

Quant Time: Sep 09 03:33:34 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 09 03:32:15 2015
Response via : Initial Calibration

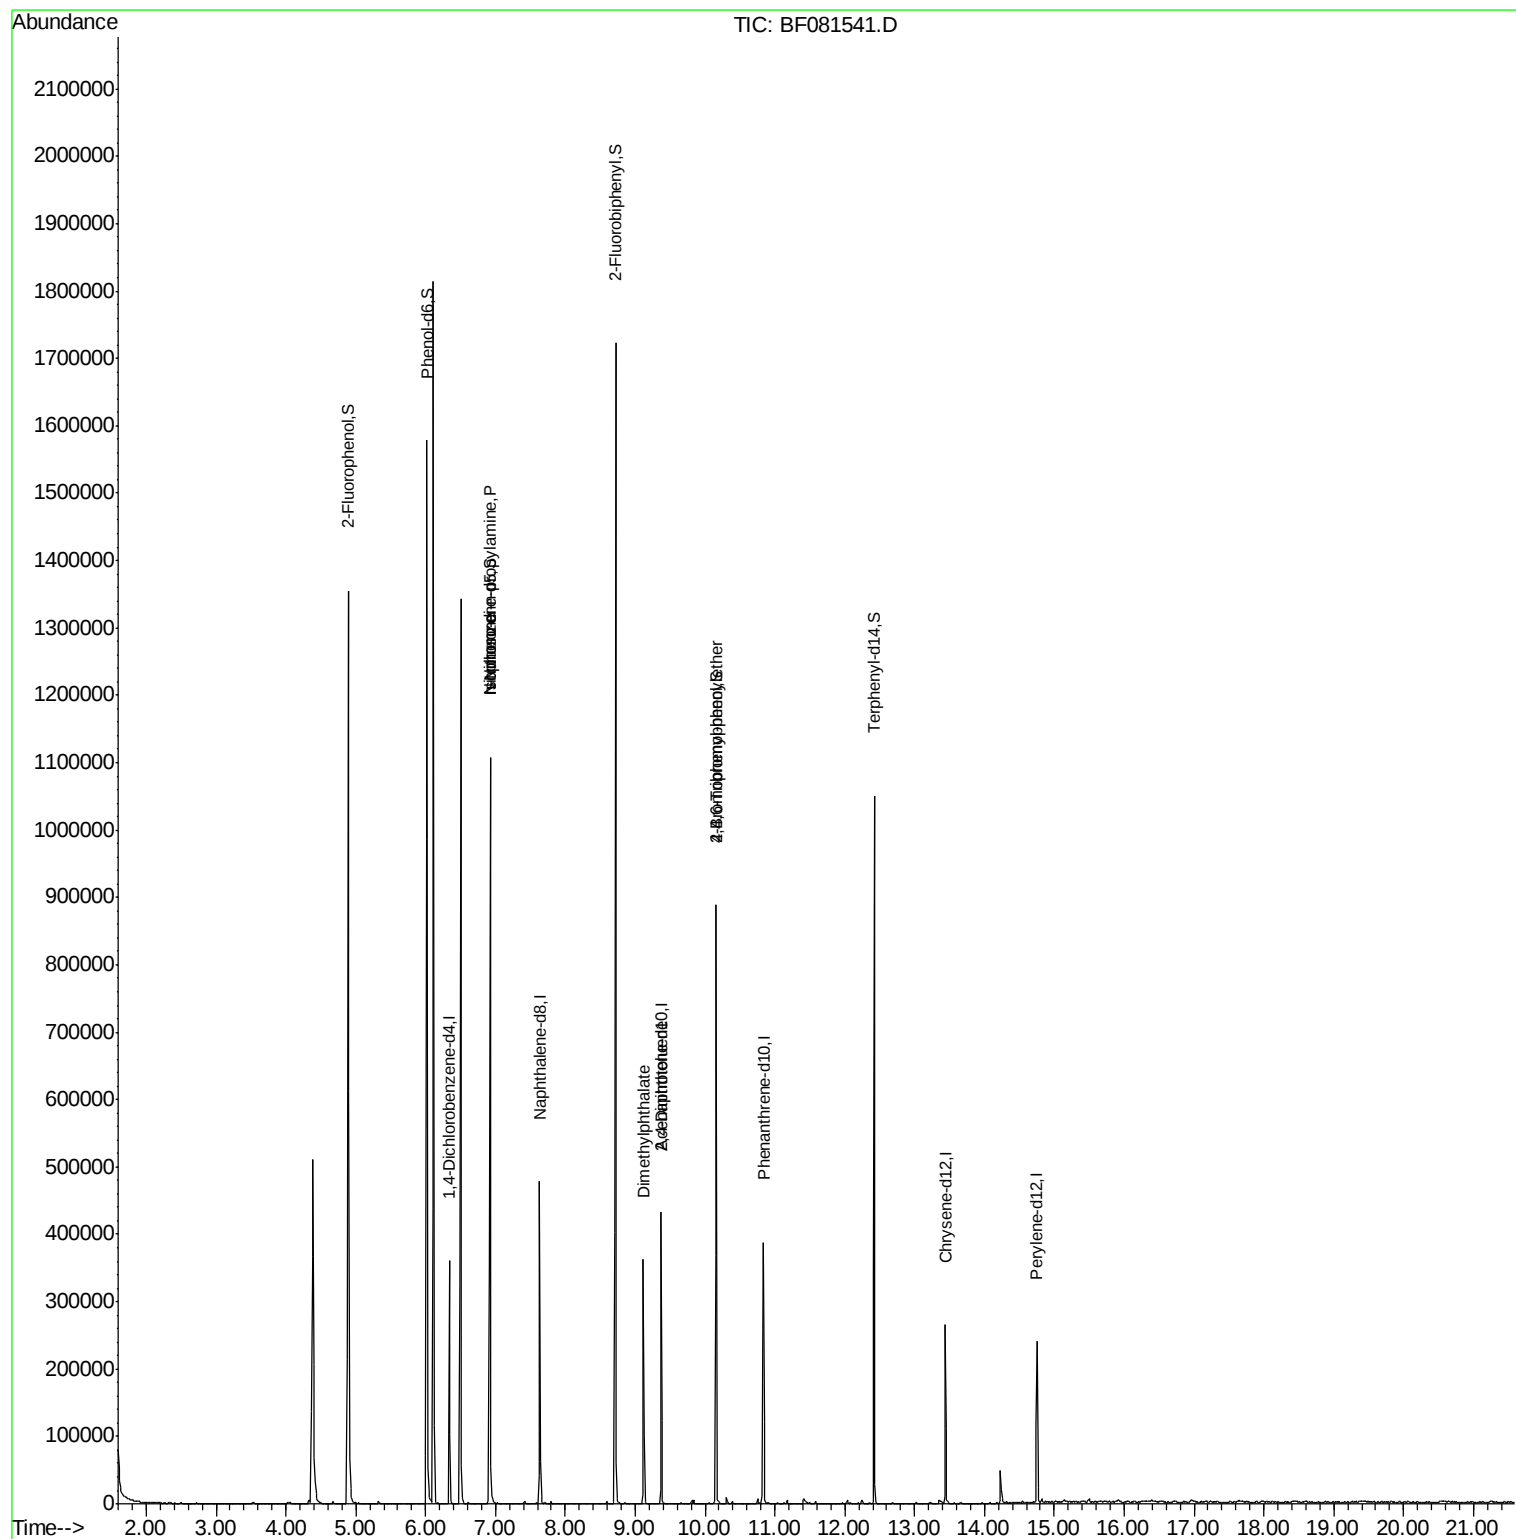

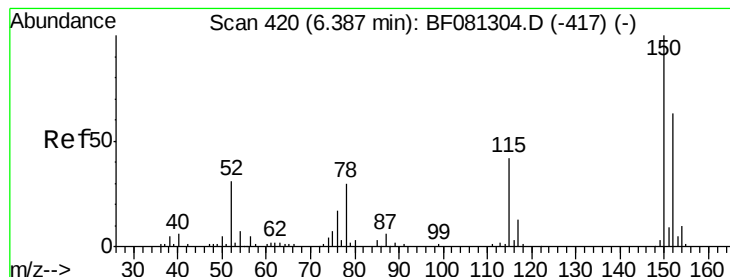

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.34 min Scan# 416

Delta R.T. -0.01 min

Lab File: BF081541.D

Acq: 9 Sep 2015 2:37

Instrument :

BNA_F

ClientSampleId :

MGP212BR-20-23


Tot Ion:152 Resp: 50038

Ion Ratio Lower Upper

152 100

150 159.0 124.7 187.1




115 70.6 39.0 58.4#

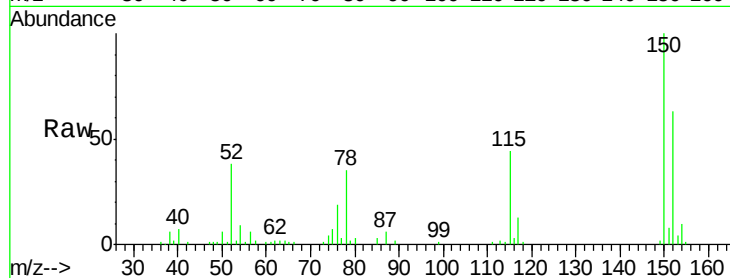

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

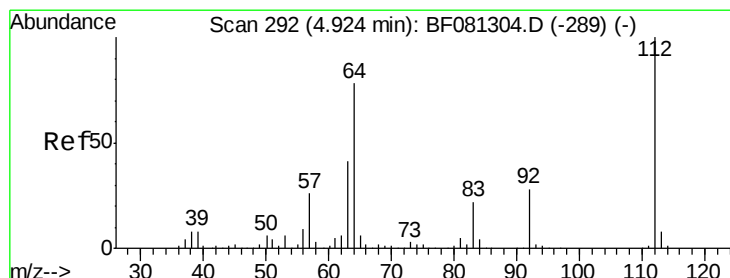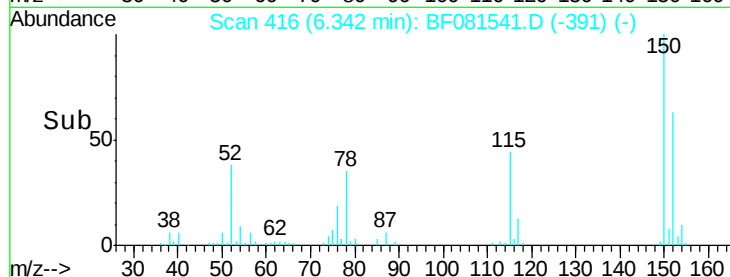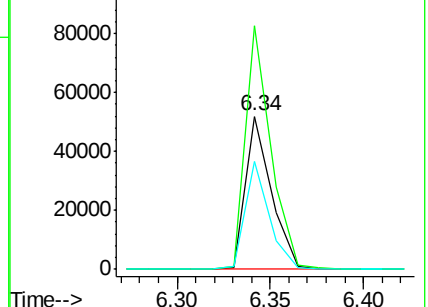

#5

2-Fluorophenol

Concen: 121.79 ng

RT: 4.89 min Scan# 289

Delta R.T. 0.01 min

Lab File: BF081541.D

Acq: 9 Sep 2015 2:37


Tgt Ion:112 Resp: 392782

Ion Ratio Lower Upper

112 100

64 79.8 39.7 59.5#



63 43.1 17.4 26.0#

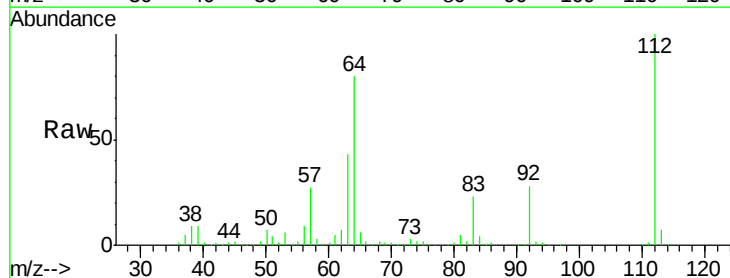


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

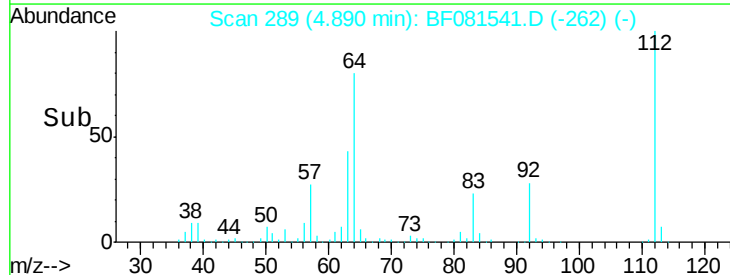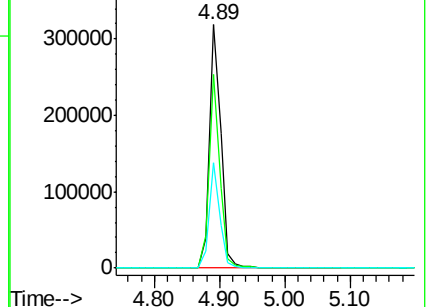

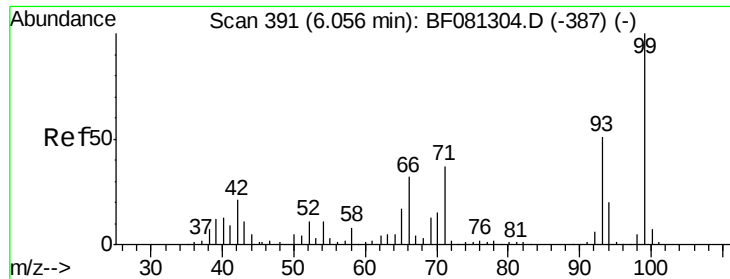

#7

Phenol-d6

Concen: 145.41 ng

RT: 6.02 min Scan# 388

Delta R.T. 0.00 min

Lab File: BF081541.D

Acq: 9 Sep 2015 2:37

Instrument :

BNA_F

ClientSampleId :

MGP212BR-20-23


Tot Ion: 99 Resp: 620766

Ion Ratio Lower Upper

99 100

42 20.5 13.7 20.5




71 35.6 14.2 21.2#

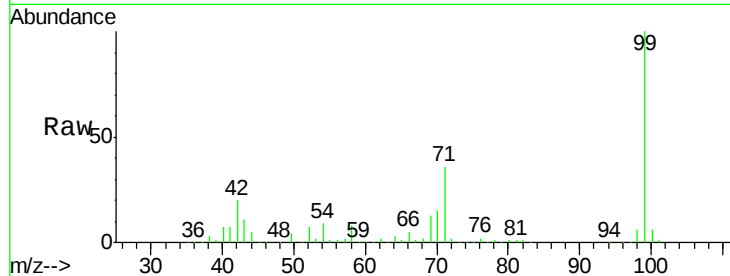

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

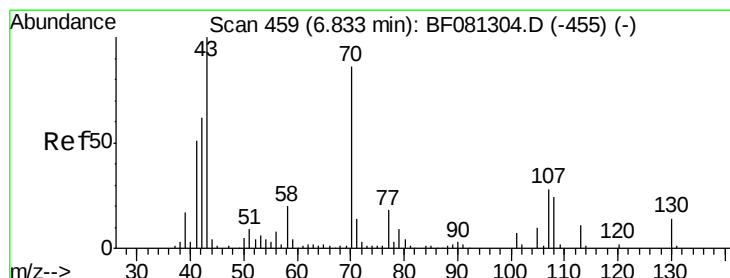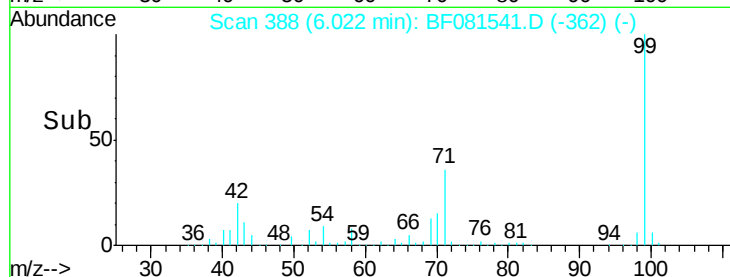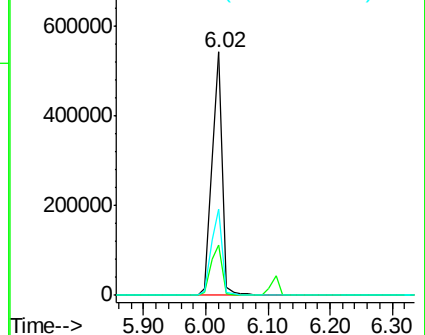

#19

n-Nitroso-di-n-propylamine

Concen: 16.61 ng

RT: 6.92 min Scan# 467

Delta R.T. 0.13 min

Lab File: BF081541.D

Acq: 9 Sep 2015 2:37

Tgt Ion: 70 Resp: 48265


Ion Ratio Lower Upper

70 100

42 55.6 63.8 95.6#

101 0.0 9.2 13.8#

130 1.5 27.3 40.9#


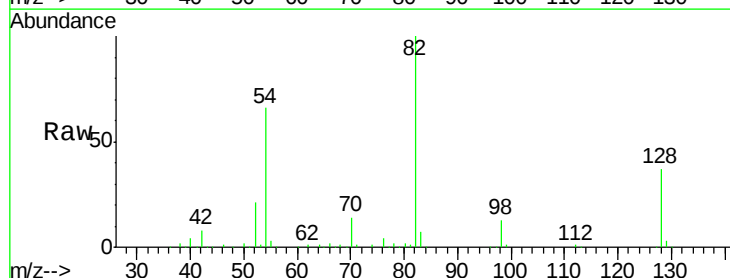



Abundance Ion 70.00 (69.70 to 70.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 101.00 (100.70 to 101.70): BF0

Ion 130.00 (129.70 to 130.70): BF0

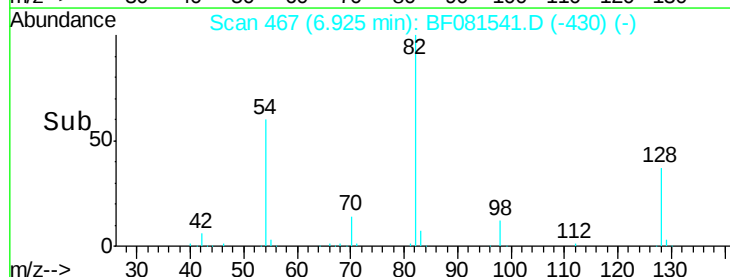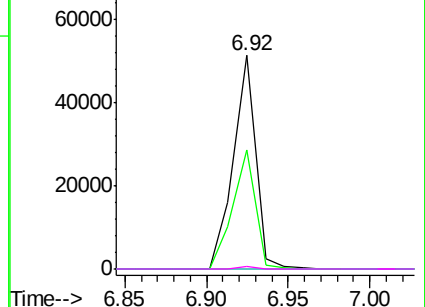

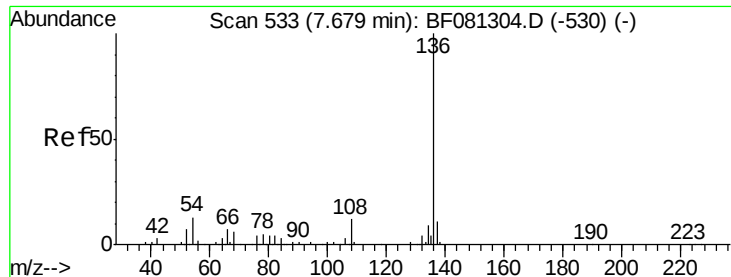

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.63 min Scan# 529

Delta R.T. -0.01 min

Lab File: BF081541.D

Acq: 9 Sep 2015 2:37

Instrument :

BNA_F

ClientSampleId :

MGP212BR-20-23

Tot Ion:136 Resp: 190721


Ion Ratio Lower Upper

136 100

137 11.1 9.0 13.6

54 12.4 8.2 12.2#

68 4.9 5.8 8.6#



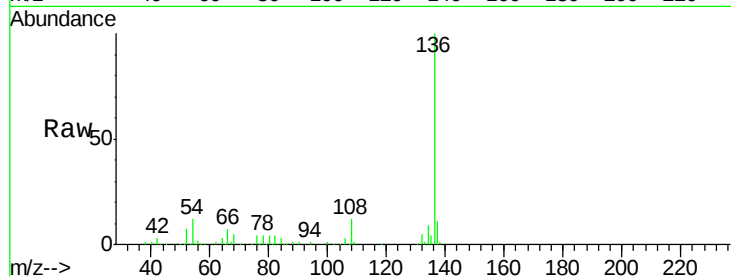


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

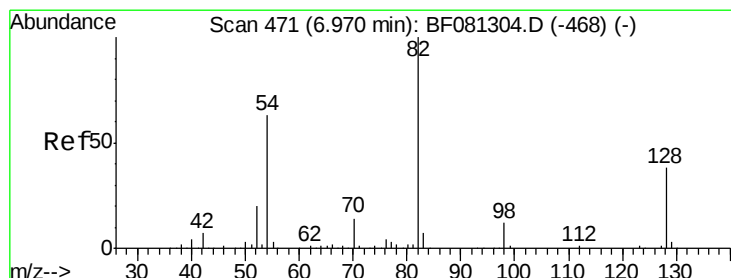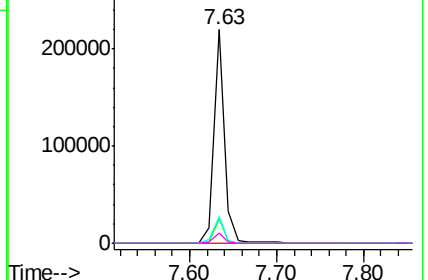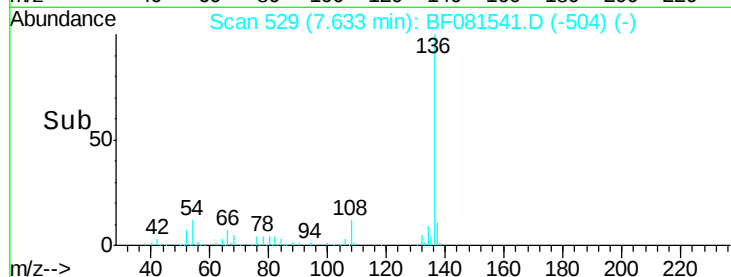

#23

Nitrobenzene-d5

Concen: 88.40 ng

RT: 6.92 min Scan# 467

Delta R.T. -0.01 min

Lab File: BF081541.D

Acq: 9 Sep 2015 2:37


Tgt Ion: 82 Resp: 349429

Ion Ratio Lower Upper

82 100

128 37.2 51.0 76.6#



54 65.9 47.5 71.3

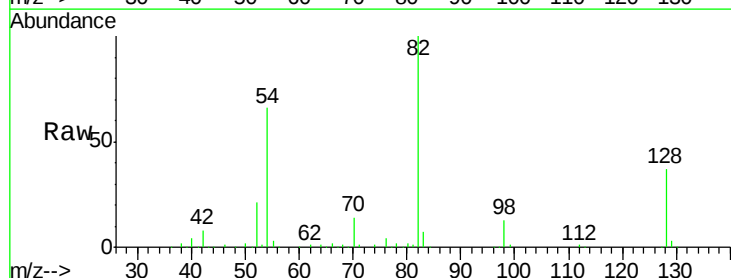


Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

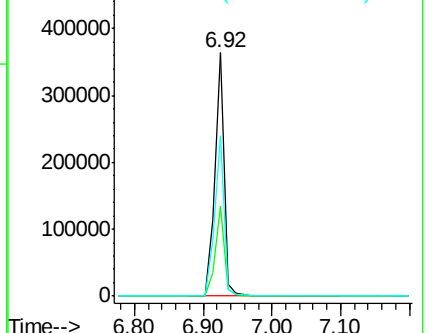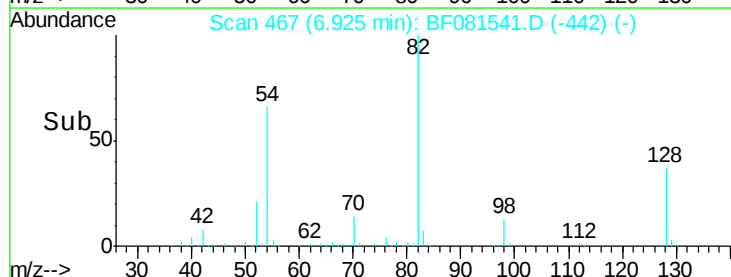

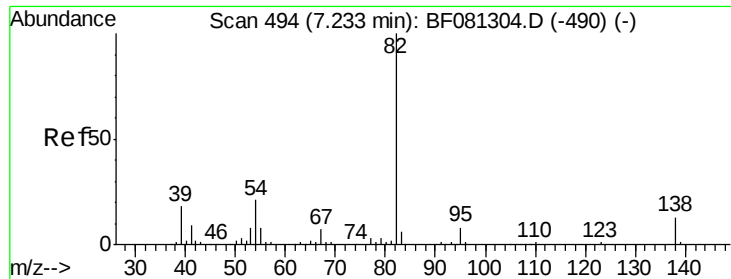

#25

Isophorone

Concen: 36.84 ng

RT: 6.92 min Scan# 467

Delta R.T. -0.27 min

Lab File: BF081541.D

Acq: 9 Sep 2015 2:37

Instrument :

BNA_F

ClientSampleId :

MGP212BR-20-23


Tot Ion: 82 Resp: 270839

Ion Ratio Lower Upper

82 100

95 0.0 4.0 6.0#




138 0.0 18.3 27.5#

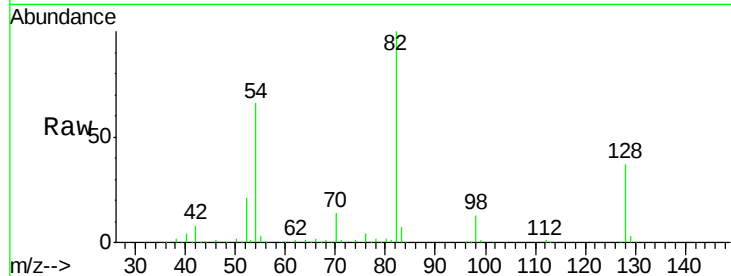

Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 95.00 (94.70 to 95.70): BF0

Ion 138.00 (137.70 to 138.70): BF0

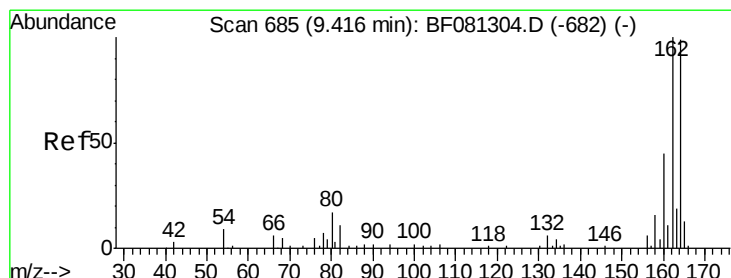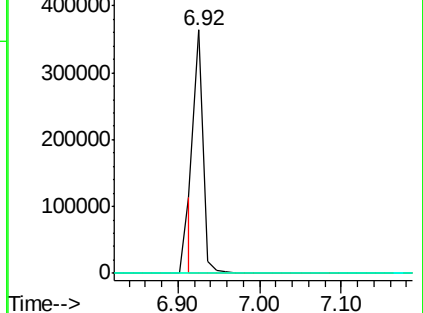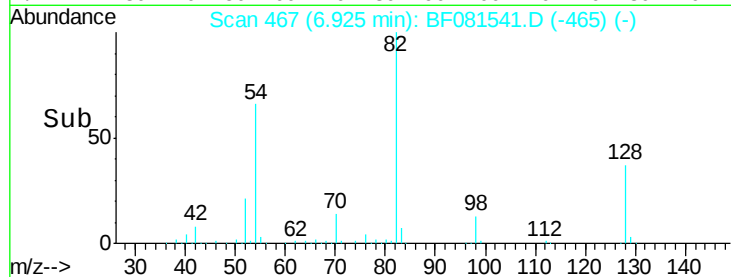

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.37 min Scan# 681

Delta R.T. -0.01 min

Lab File: BF081541.D

Acq: 9 Sep 2015 2:37


Tgt Ion: 164 Resp: 84001

Ion Ratio Lower Upper

164 100

162 104.9 75.2 112.8



160 46.6 31.5 47.3

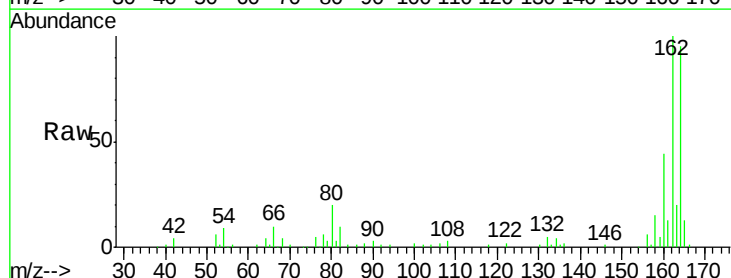


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

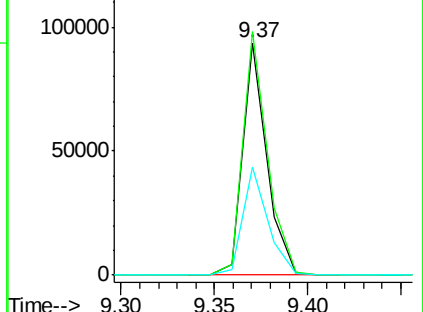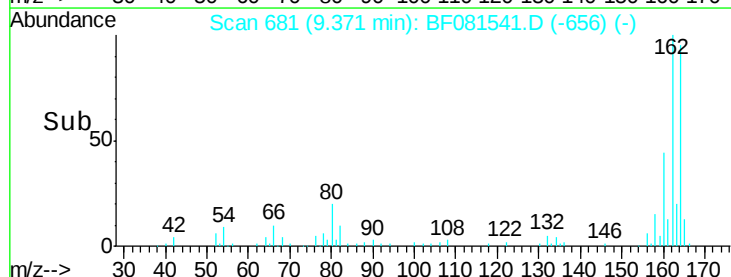


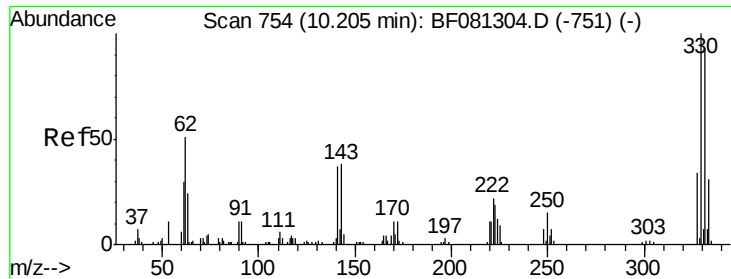




#41
 2,4,6-Tribromophenol
 Concen: 118.07 ng
 RT: 10.16 min Scan# 750
 Delta R.T. 0.00 min
 Lab File: BF081541.D
 Acq: 9 Sep 2015 2:37

Instrument :
 BNA_F
 ClientSampleId :
 MGP212BR-20-23

Tot Ion:330 Resp: 88310
 Ion Ratio Lower Upper
 330 100
 332 99.7 76.6 114.8
 141 50.9 29.7 44.5#

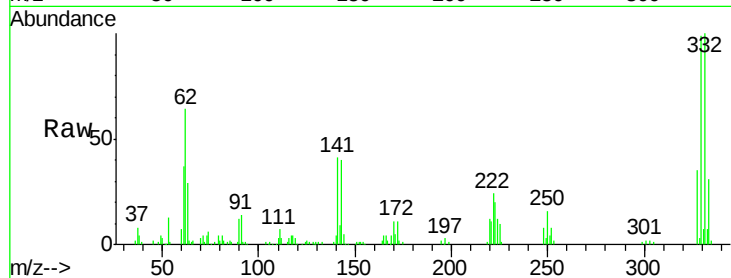


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

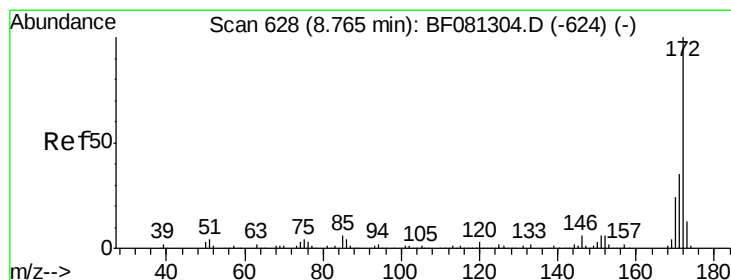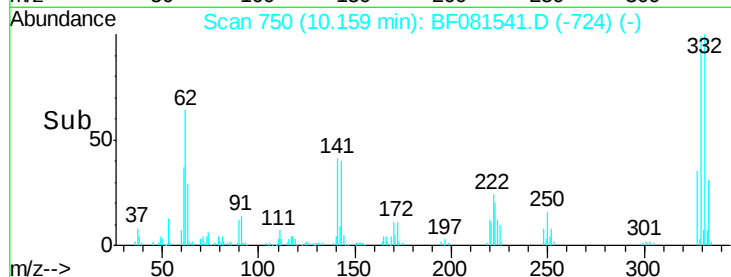
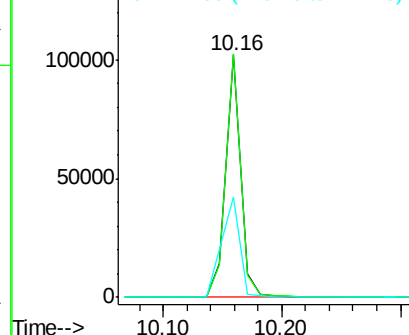



#44
 2-Fluorobiphenyl
 Concen: 75.63 ng
 RT: 8.72 min Scan# 624
 Delta R.T. 0.00 min
 Lab File: BF081541.D
 Acq: 9 Sep 2015 2:37

Tgt Ion:172 Resp: 495769
 Ion Ratio Lower Upper
 172 100
 171 35.5 26.1 39.1
 170 24.2 17.4 26.2

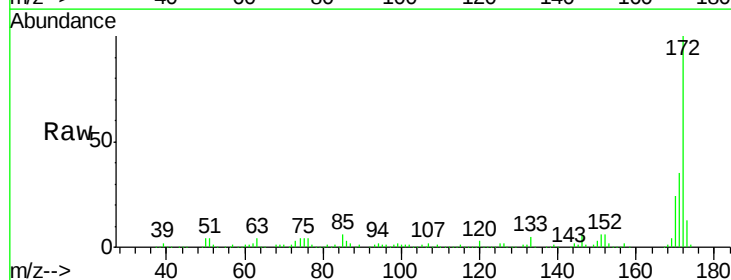

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

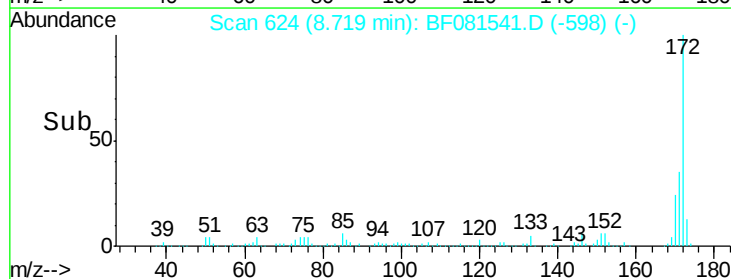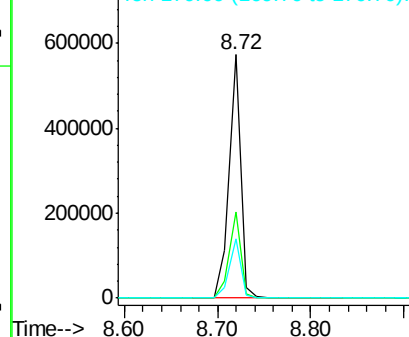

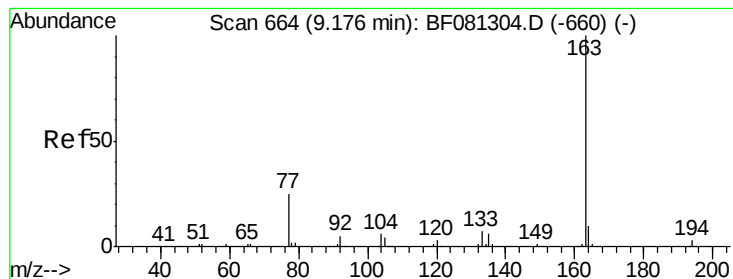

#49

Dimethylphthalate

Concen: 21.41 ng

RT: 9.12 min Scan# 659

Delta R.T. -0.01 min

Lab File: BF081541.D

Acq: 9 Sep 2015 2:37

Instrument :

BNA_F

ClientSampleId :

MGP212BR-20-23


Tot Ion:163 Resp: 139755

Ion Ratio Lower Upper

163 100

194 2.9 4.4 6.6#




164 10.7 8.3 12.5

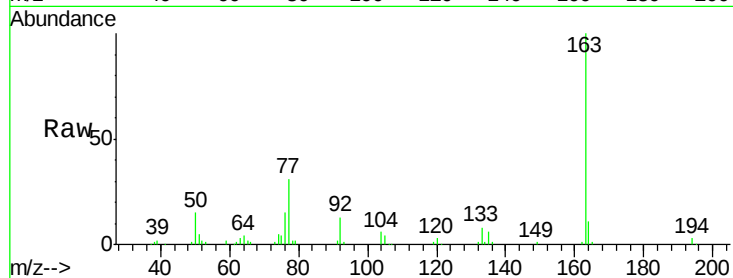

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

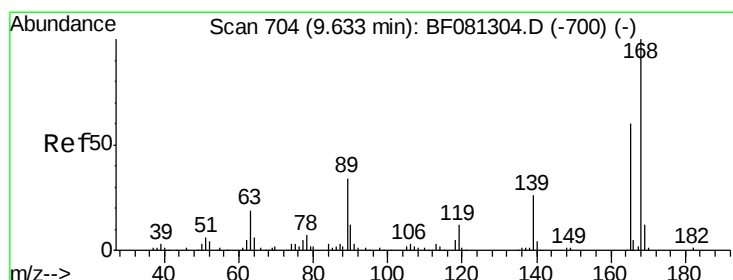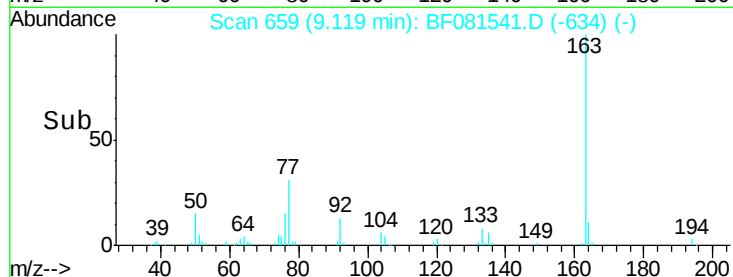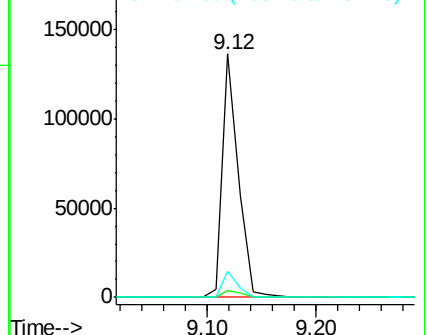

#56

2,4-Dinitrotoluene

Concen: 6.00 ng

RT: 9.37 min Scan# 681

Delta R.T. -0.22 min

Lab File: BF081541.D

Acq: 9 Sep 2015 2:37

Tgt Ion:165 Resp: 11326


Ion Ratio Lower Upper

165 100

63 0.0 29.8 44.6#

89 0.0 44.5 66.7#

182 0.0 3.0 4.4#


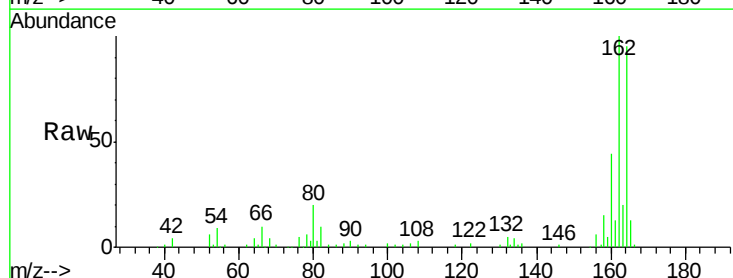



Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

Ion 182.00 (181.70 to 182.70): E

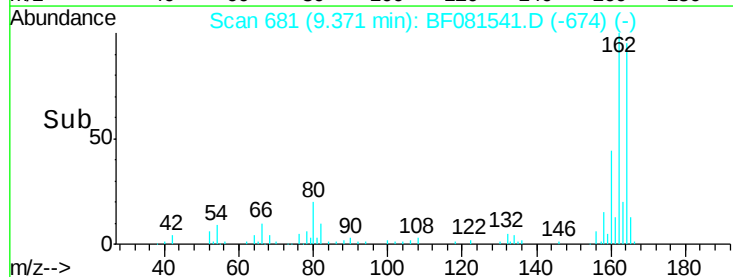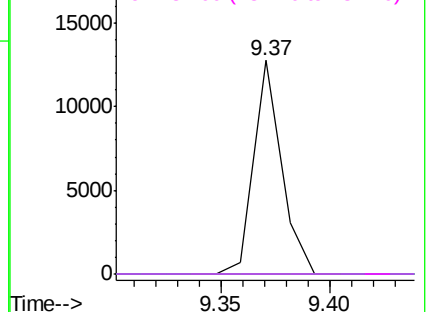


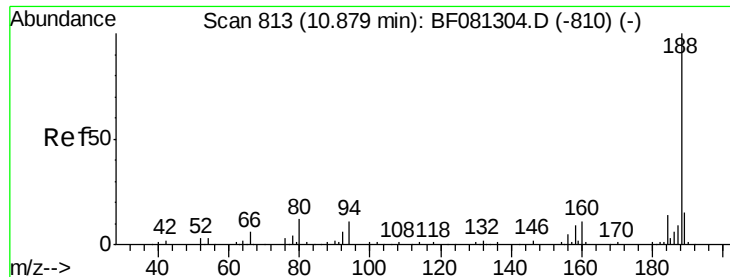




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 10.83 min Scan# 809
Delta R.T. -0.01 min
Lab File: BF081541.D
Acq: 9 Sep 2015 2:37

Instrument :
BNA_F
ClientSampleId :
MGP212BR-20-23

Tot Ion:188 Resp: 149017
Ion Ratio Lower Upper
188 100
94 9.8 11.1 16.7#
80 10.7 11.0 16.4#

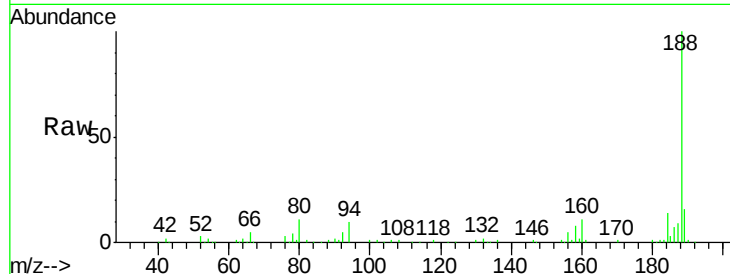


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

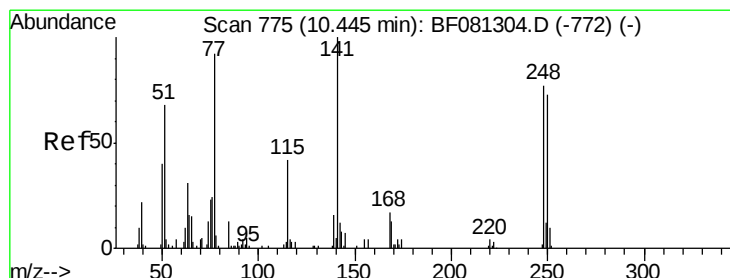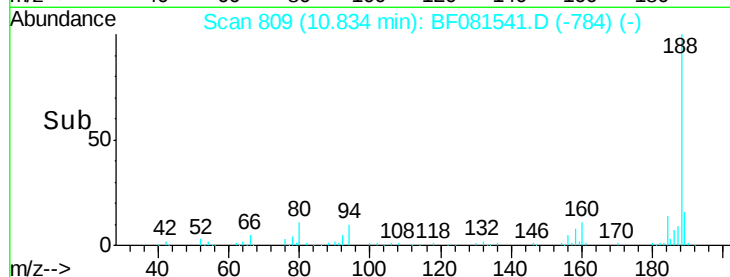
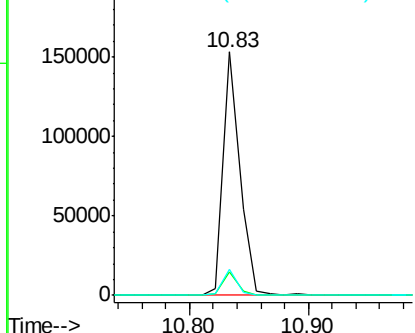



#66
4-Bromophenyl-phenylether
Concen: 4.77 ng
RT: 10.16 min Scan# 750
Delta R.T. -0.25 min
Lab File: BF081541.D
Acq: 9 Sep 2015 2:37

Tgt Ion:248 Resp: 7190
Ion Ratio Lower Upper
248 100
250 202.9 78.5 117.7#
141 515.3 59.0 88.6#

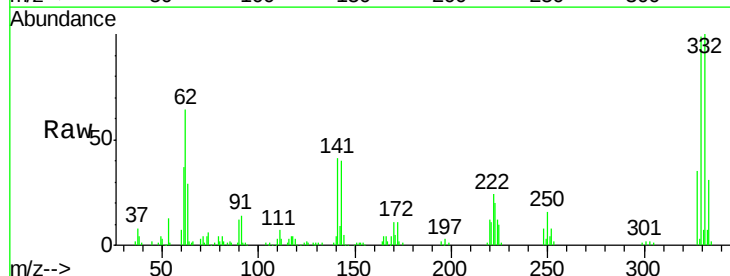

Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

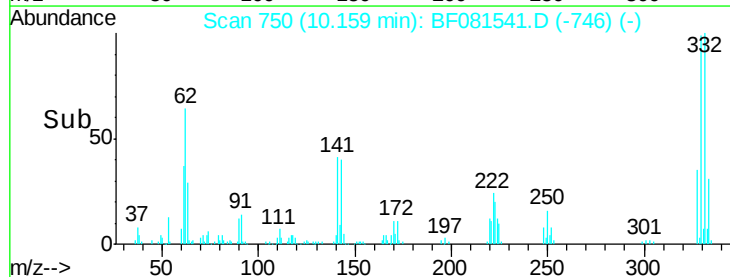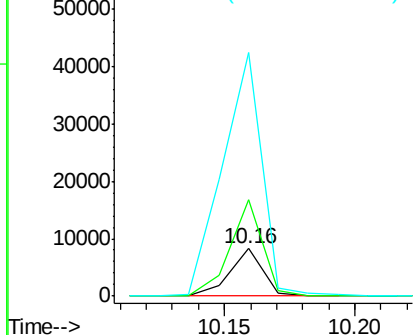

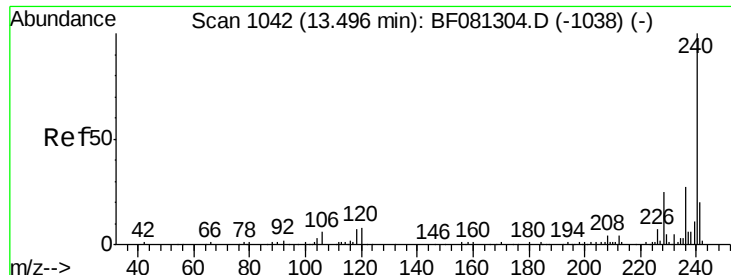

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.44 min Scan# 1037

Delta R.T. -0.01 min

Lab File: BF081541.D

Acq: 9 Sep 2015 2:37

Instrument :

BNA_F

ClientSampleId :

MGP212BR-20-23


Tot Ion:240 Resp: 104447

Ion Ratio Lower Upper

240 100

120 13.3 16.2 24.2#




236 26.3 18.4 27.6

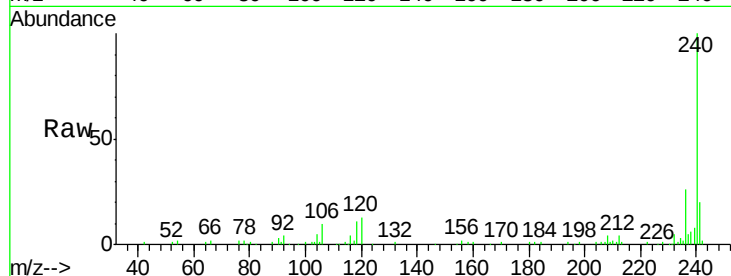

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

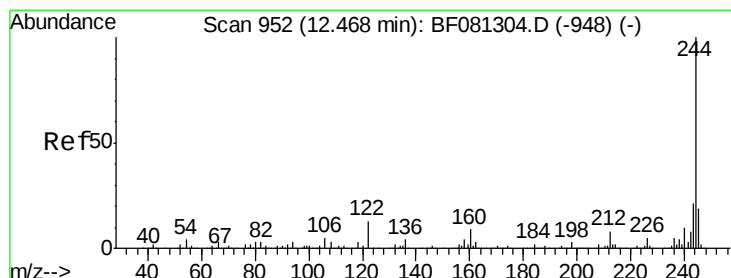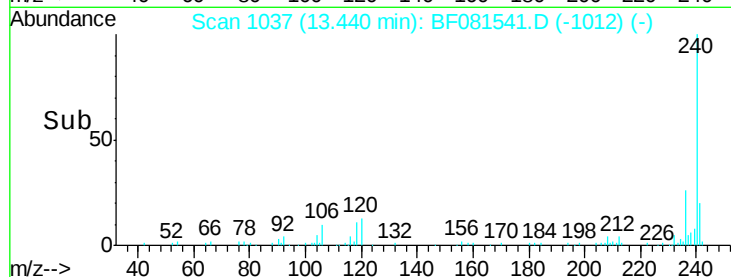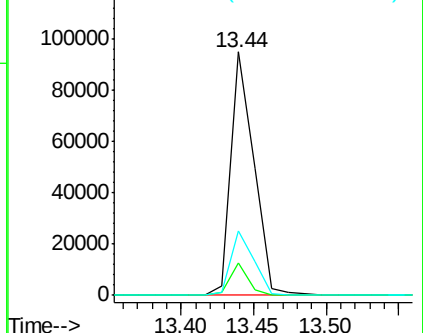

#78

Terphenyl-d14

Concen: 72.40 ng

RT: 12.42 min Scan# 948

Delta R.T. 0.00 min

Lab File: BF081541.D

Acq: 9 Sep 2015 2:37


Tgt Ion:244 Resp: 324866

Ion Ratio Lower Upper

244 100

212 7.3 4.3 6.5#



122 8.7 17.4 26.2#



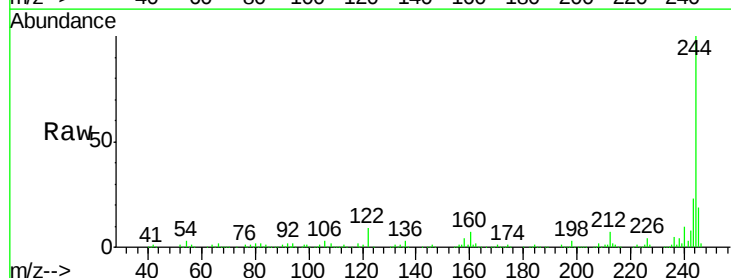


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

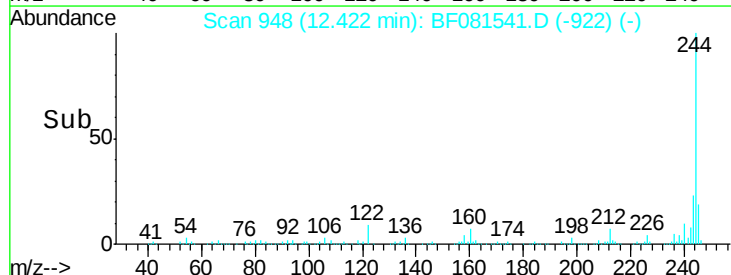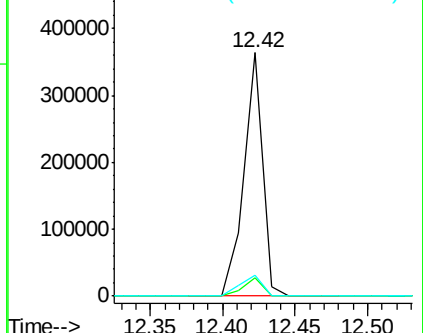

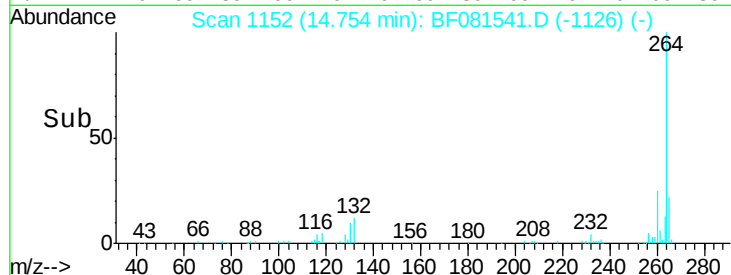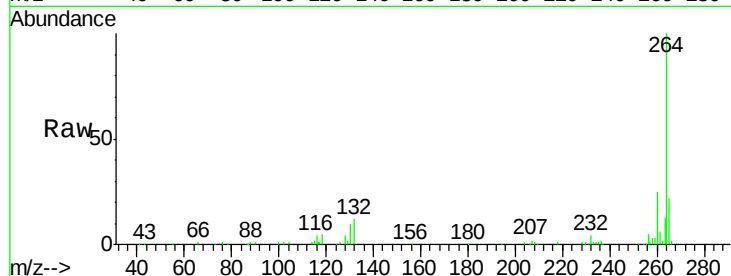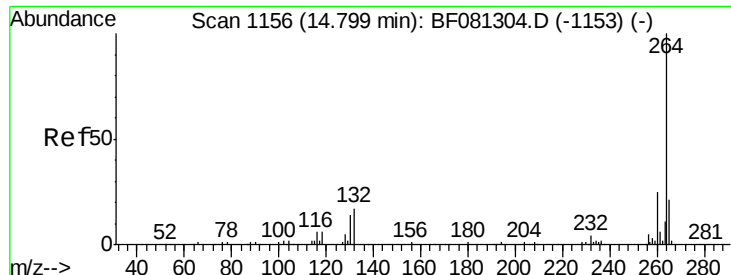

#86
Pervlene-d12
Concen: 20.00 ng
RT: 14.75 min Scan# 1152
Delta R.T. 0.00 min
Lab File: BF081541.D
Acq: 9 Sep 2015 2:37

Instrument :
BNA_F
ClientSampleId :
MGP212BR-20-23

Tot Ion:	264	Resp:	101373
Ion	Ratio	Lower	Upper
264	100		
260	24.8	16.7	25.1
265	21.5	17.2	25.8

