
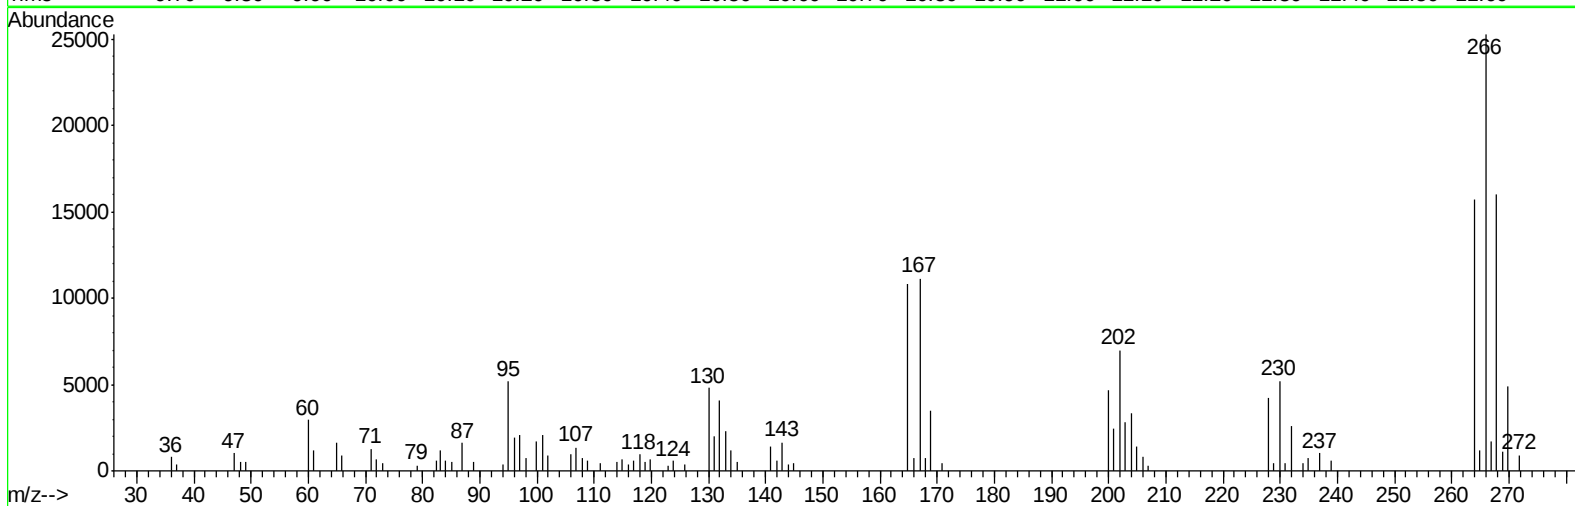


Data Path : Z:\HPCHEM1\BNA F\Data\BF090815\
Data File : BF081520.D
Acq On : 8 Sep 2015 13:49
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 08 18:58:30 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 08 15:49:53 2015
Response via : Initial Calibration

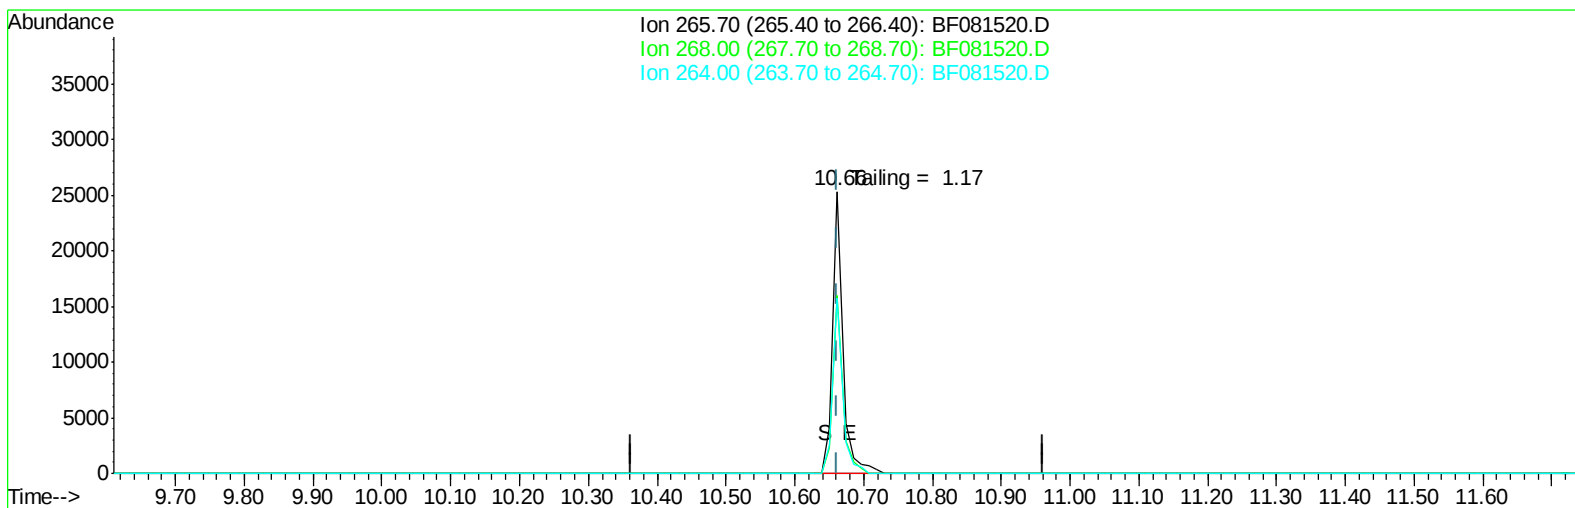

TIC: BF081520.D

(69) Pentachlorophenol (C)



10.662min (-0.000) 0.00ng

response 25362

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	63.29
264.00	62.70	62.08
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF090815\
Data File : BF081520.D
Acq On : 8 Sep 2015 13:49
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 08 18:58:30 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 08 15:49:53 2015
Response via : Initial Calibration

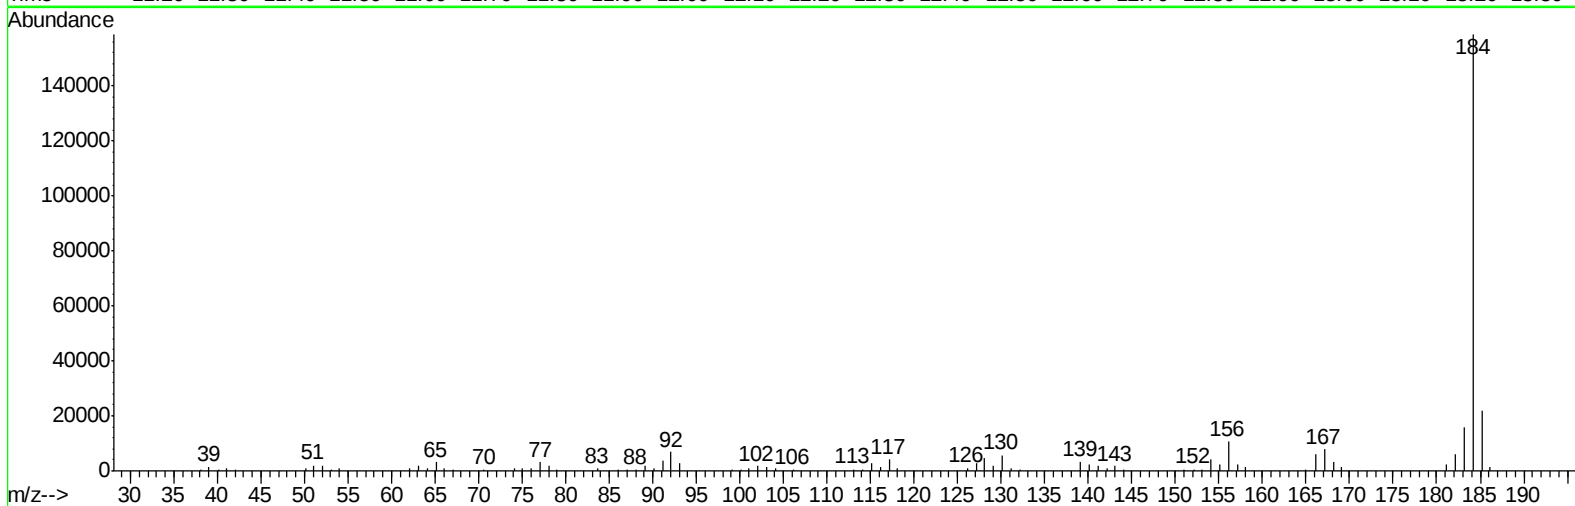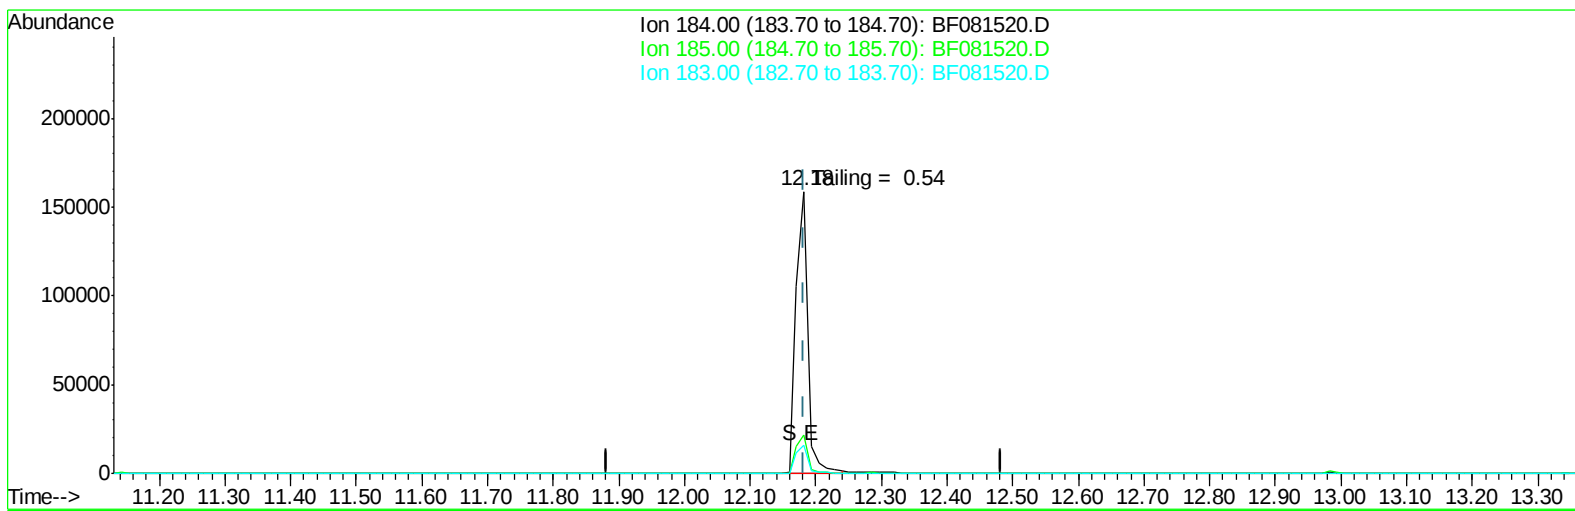

TIC: BF081520.D

(76) Benzidine

12.182min (-0.000) 0.00ng

response 204032

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	13.83
183.00	9.50	10.11
0.00	0.00	0.00