
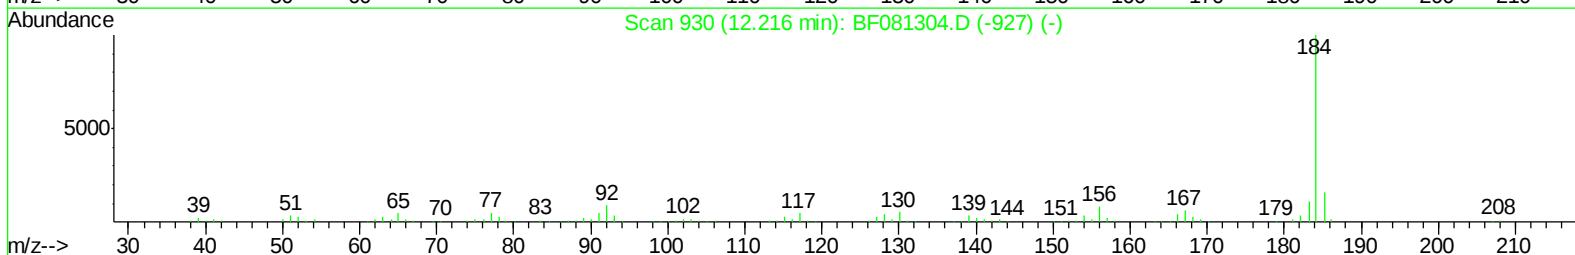
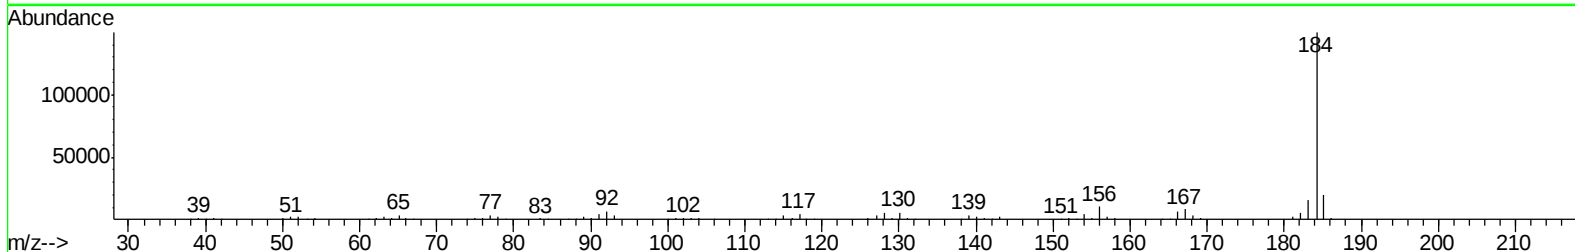


Data Path : Z:\HPCHEM1\BNA F\DATA\BF090815\
Data File : BF081539.D
Acq On : 9 Sep 2015 1:32
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 09 06:41:04 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 09 03:32:15 2015
Response via : Initial Calibration

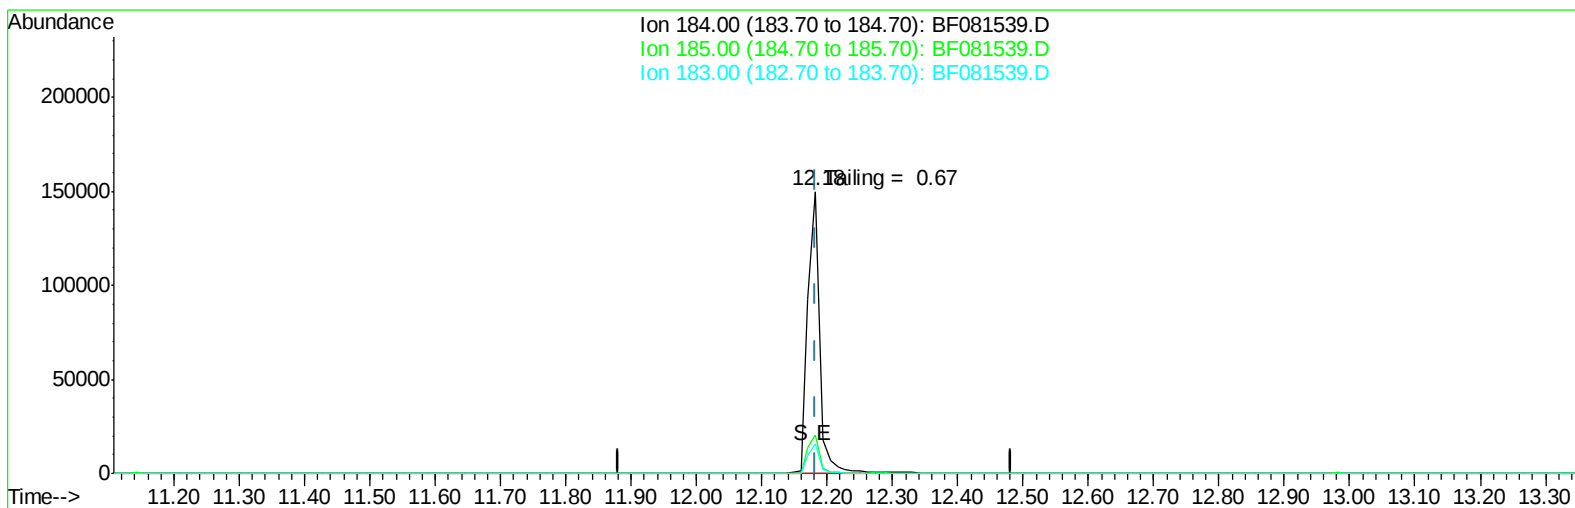

TIC: BF081539.D

(76) Benzidine




12.182min (+0.000) 0.00ng

response 192777

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	13.50
183.00	9.50	10.66
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF090815\
Data File : BF081539.D
Acq On : 9 Sep 2015 1:32
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 09 06:41:04 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 09 03:32:15 2015
Response via : Initial Calibration

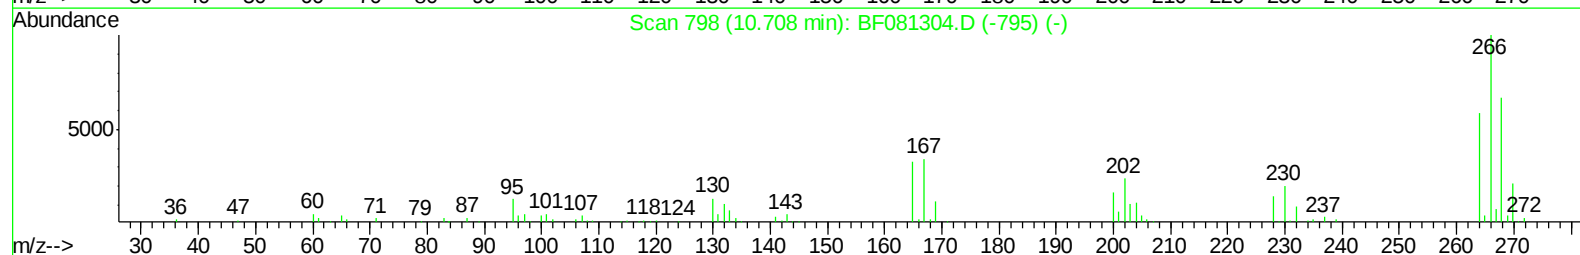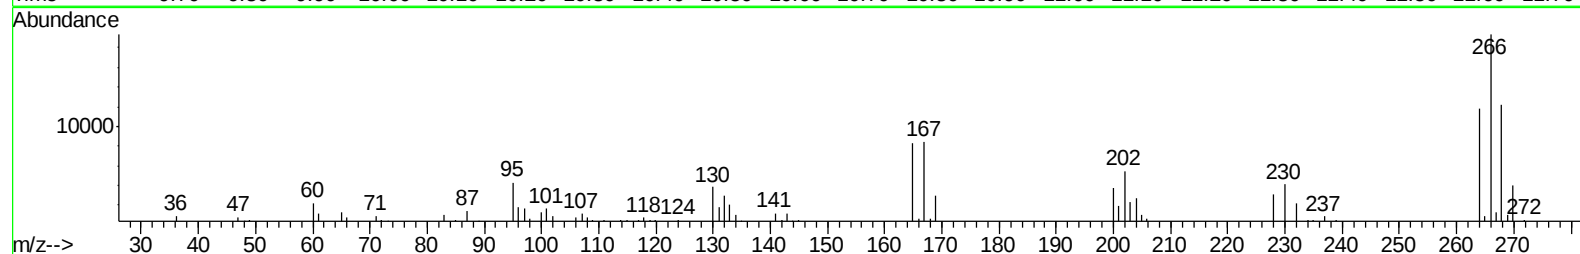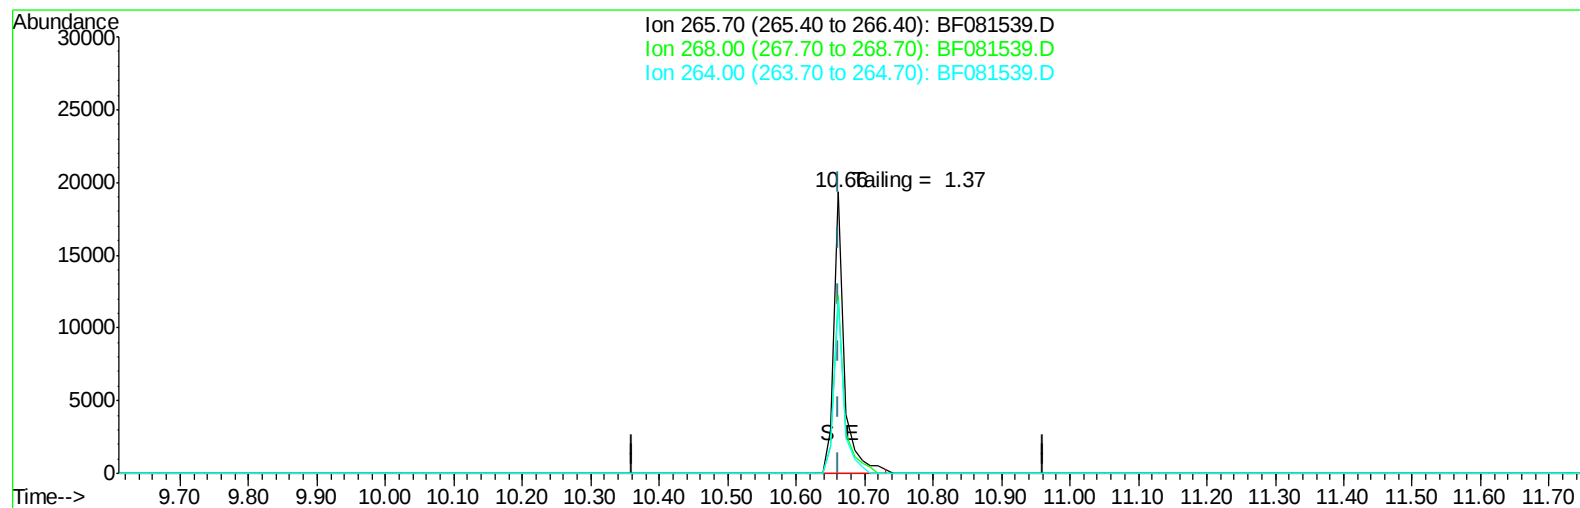

TIC: BF081539.D

(69) Pentachlorophenol (C)

10.662min (+0.000) 0.00ng

response 20734

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	63.21
264.00	62.70	61.27
0.00	0.00	0.00