


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF090815\
 Data File : BF081520.D
 Acq On : 8 Sep 2015 13:49
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 08 15:49:53 2015

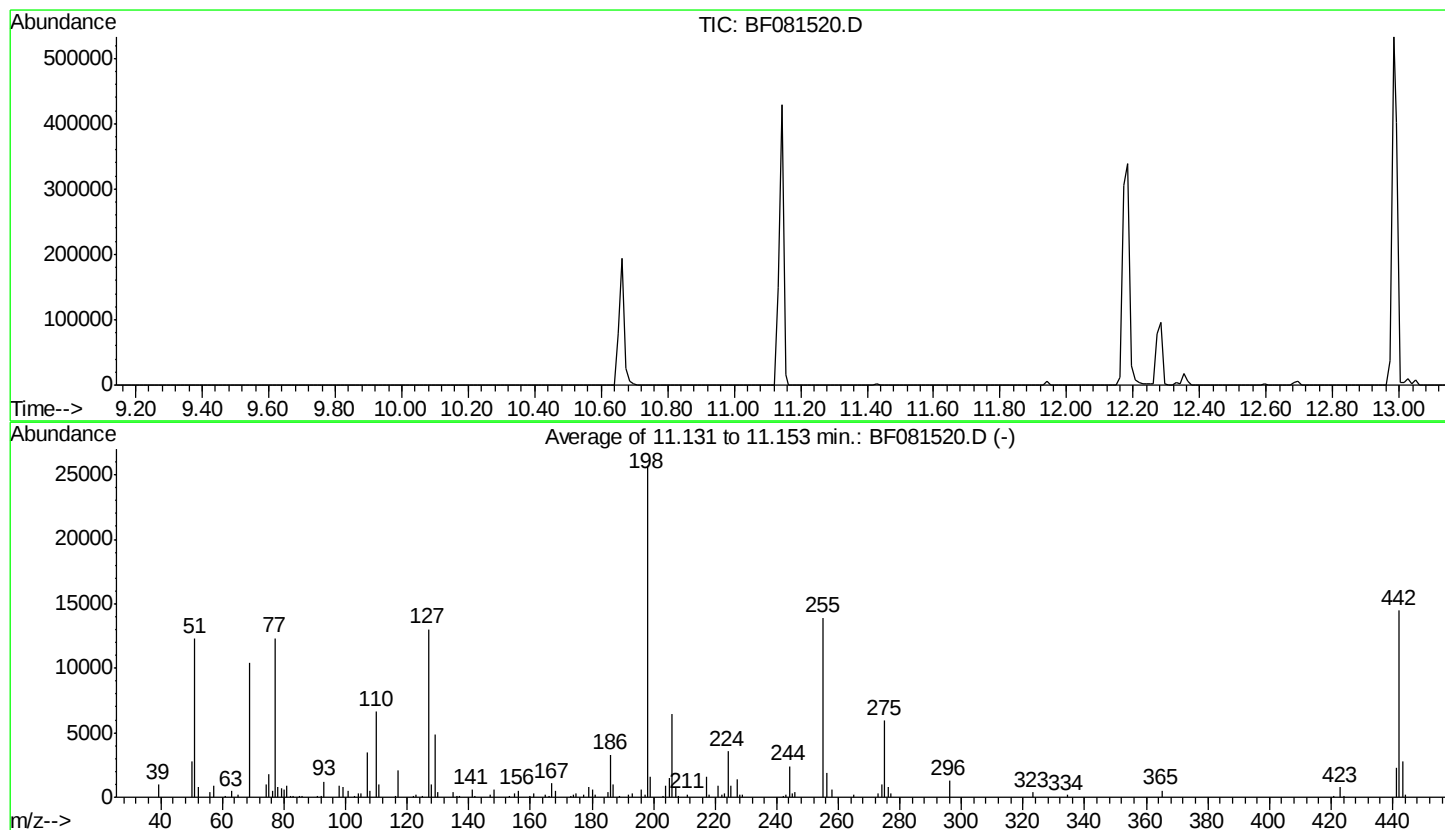

AutoFind: Scans 835, 836, 837; Background Corrected with Scan 832

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.7	12269	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	40.6	10435	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.7	13047	PASS
197	198	0.00	2	0.6	152	PASS
198	198	100	100	100.0	25709	PASS
199	198	5	9	6.2	1588	PASS
275	198	10	60	23.1	5926	PASS
365	198	1	100	2.0	525	PASS
441	442	0.01	24	16.0	2311	PASS
442	198	50	100	56.2	14459	PASS
443	442	15	24	19.1	2757	PASS