


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF090815\
 Data File : BF081539.D
 Acq On : 9 Sep 2015 1:32
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 08 15:49:53 2015

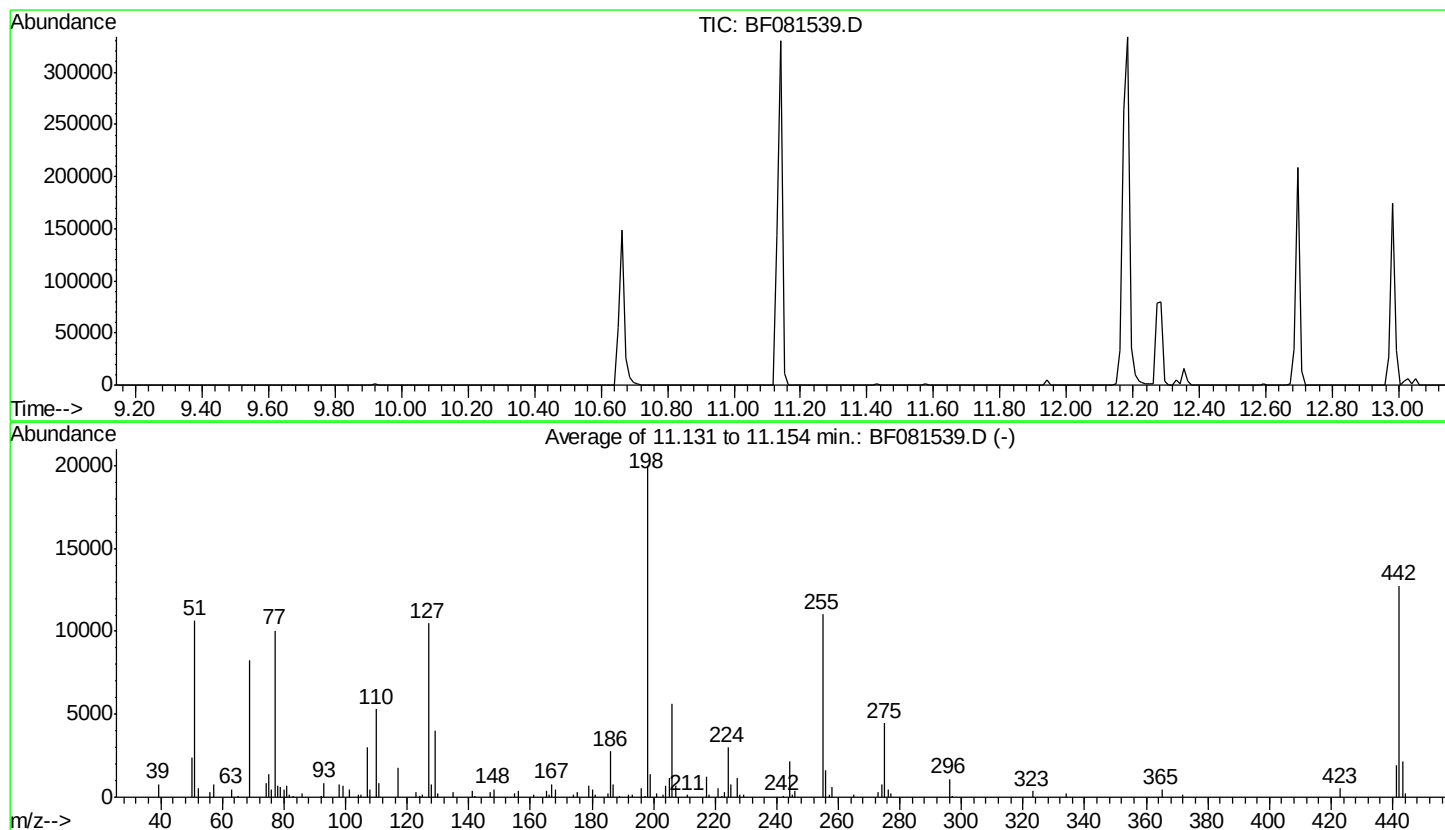

AutoFind: Scans 835, 836, 837; Background Corrected with Scan 832

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.1	10617	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	41.4	8277	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.4	10473	PASS
197	198	0.00	2	0.5	101	PASS
198	198	100	100	100.0	19995	PASS
199	198	5	9	7.0	1395	PASS
275	198	10	60	22.3	4465	PASS
365	198	1	100	2.3	460	PASS
441	442	0.01	24	15.2	1938	PASS
442	198	50	100	63.8	12762	PASS
443	442	15	24	16.8	2144	PASS