
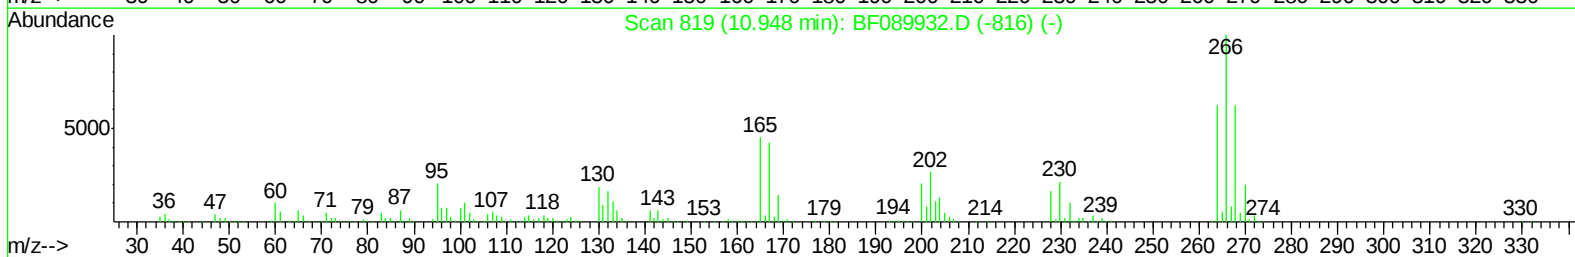
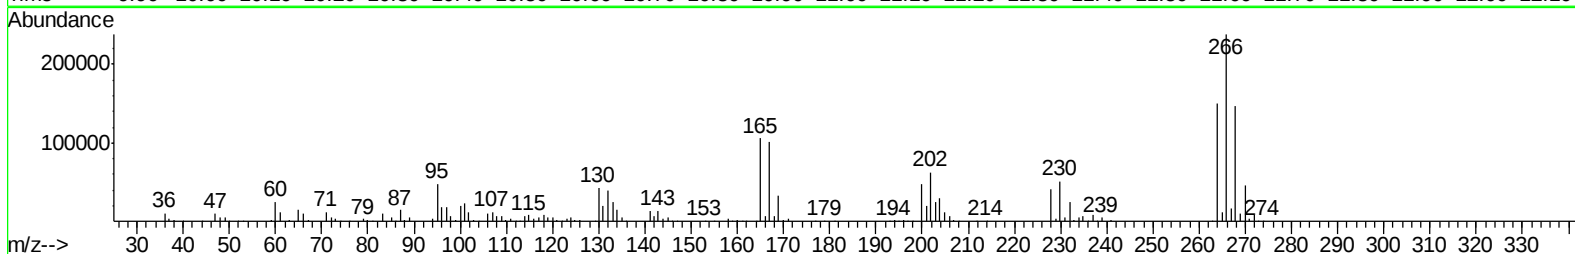


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF090816\
Data File : BF090022.D
Acq On : 8 Sep 2016 14:02
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 09 08:54:22 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 08 16:07:52 2016
Response via : Initial Calibration

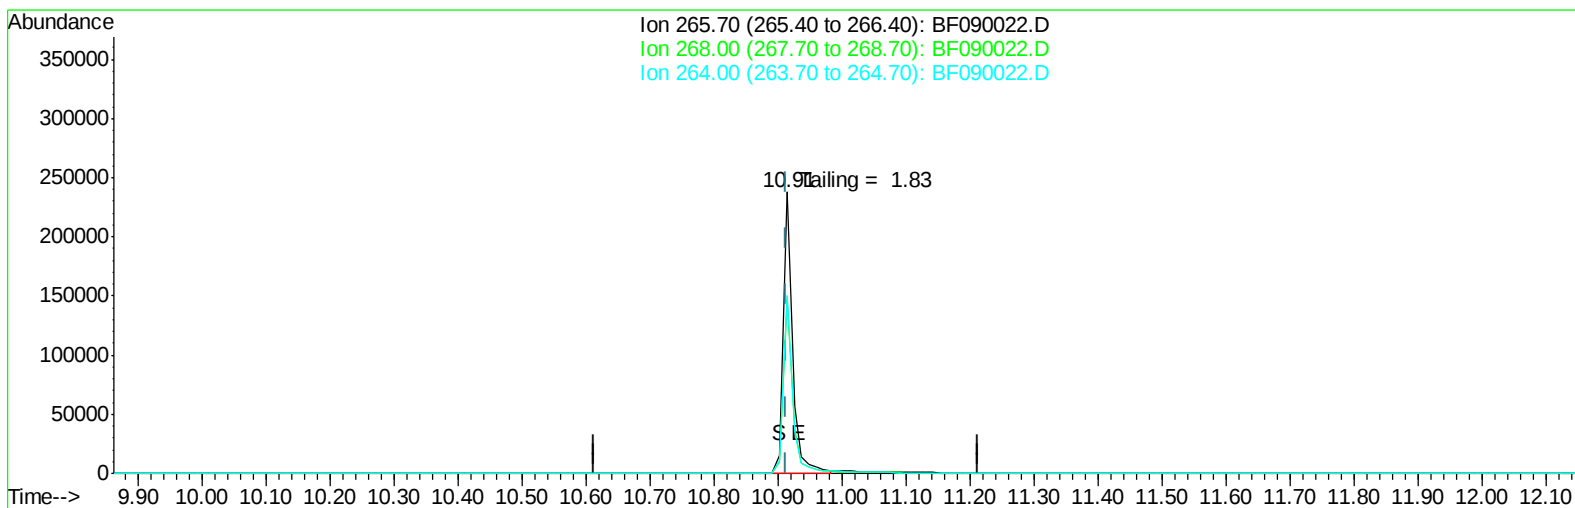

TIC: BF090022.D

(69) Pentachlorophenol (C)




10.913min (-0.000) 37805.91ng

response 246051

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	62.02
264.00	63.20	62.98
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF090816\
Data File : BF090022.D
Acq On : 8 Sep 2016 14:02
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 09 08:54:22 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 08 16:07:52 2016
Response via : Initial Calibration

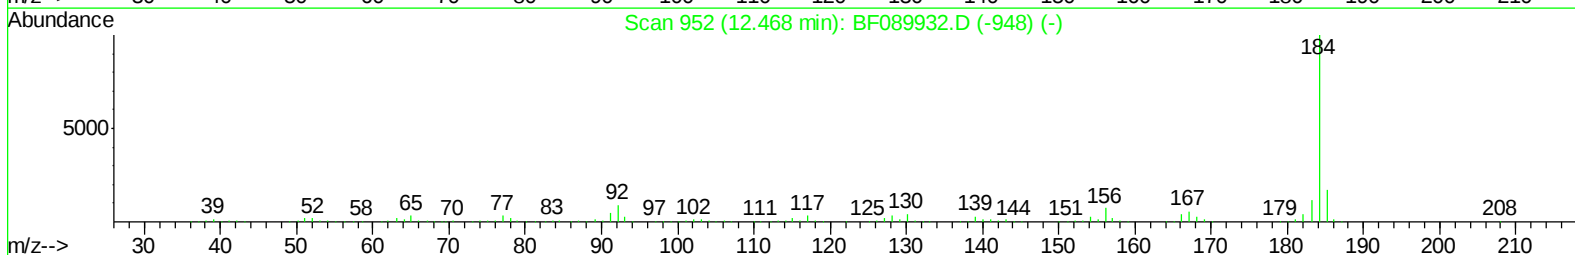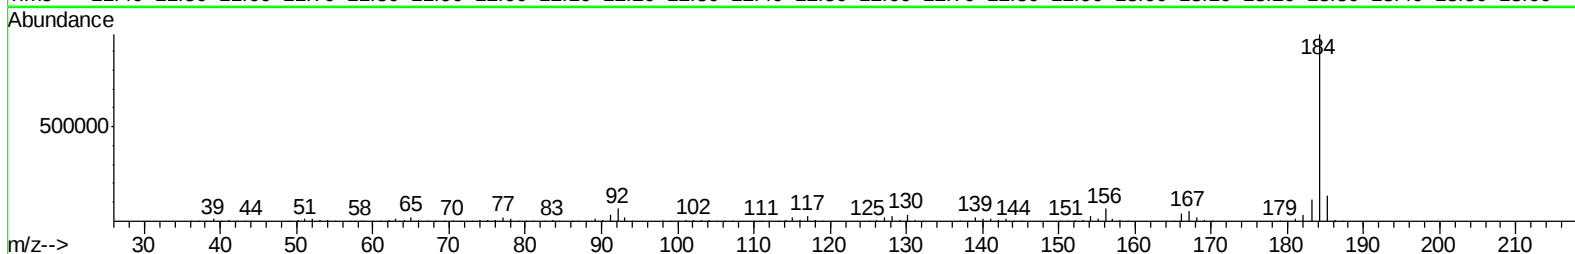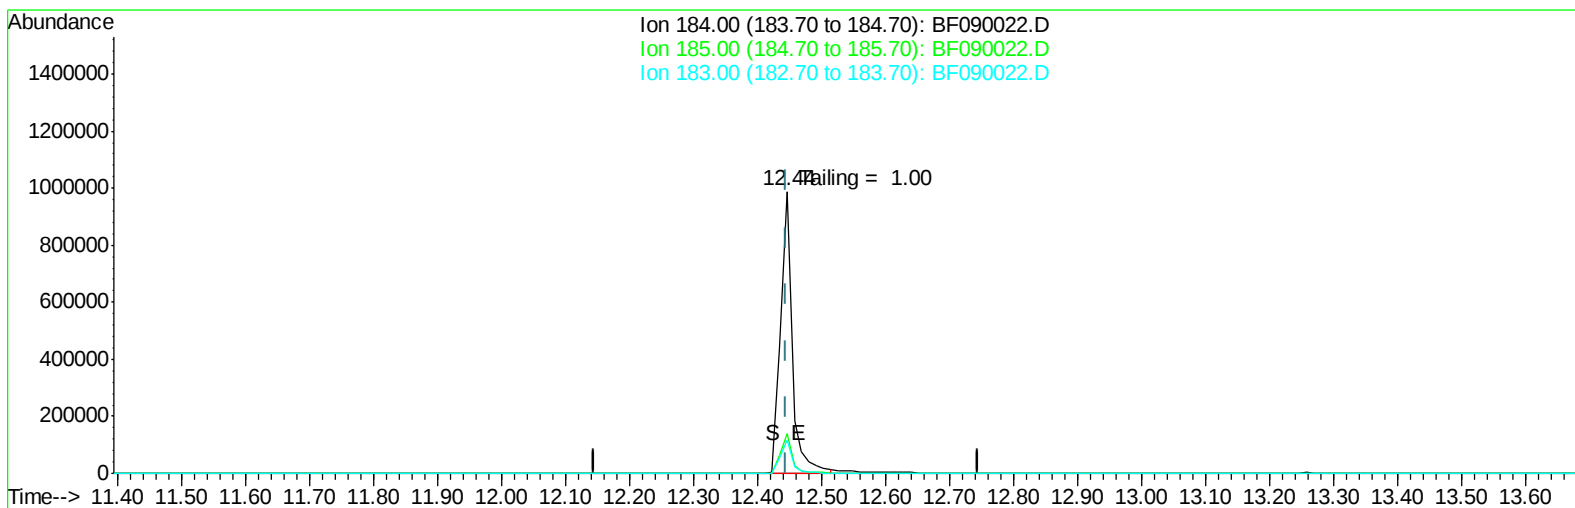

TIC: BF090022.D

(76) Benzidine

12.445min (-0.000) 21005.35ng

response 1269218

Ion	Exp%	Act%
184.00	100	100
185.00	17.30	14.05
183.00	12.00	11.80
0.00	0.00	0.00