

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF090816\
 Data File : BF090043.D
 Acq On : 9 Sep 2016 00:05
 Operator : UM/SJ
 Sample : H4688-03 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SS-AST3

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF083116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.724	11	12	68	rVB	4490706	14048878	100.00%	56.865%
2	5.164	310	313	324	rBV	203166	322760	2.30%	1.306%
3	6.239	404	407	415	rBV	255672	380831	2.71%	1.541%
4	6.364	415	418	420	rBV	275719	393041	2.80%	1.591%
5	6.593	436	438	441	rBV	922489	1071677	7.63%	4.338%
6	6.753	450	452	454	rBV	321561	302617	2.15%	1.225%
7	7.164	485	488	504	rBV	154107	253462	1.80%	1.026%
8	7.885	549	551	553	rBV	1661160	1446799	10.30%	5.856%
9	8.959	643	645	652	rBV	527634	550123	3.92%	2.227%
10	9.359	678	680	689	rVB	191654	187839	1.34%	0.760%
11	9.633	701	704	706	rBV	1373172	1504912	10.71%	6.091%
12	10.411	769	772	775	rBV	229976	256228	1.82%	1.037%
13	11.096	830	832	835	rBV	1153876	1260642	8.97%	5.103%
14	12.674	968	970	982	rVB	298535	446188	3.18%	1.806%
15	13.714	1059	1061	1074	rBV	1191047	1331371	9.48%	5.389%
16	15.051	1175	1178	1182	rBV	757282	948446	6.75%	3.839%




Sum of corrected areas: 24705814

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF090816\
Data File : BF090043.D
Acq On : 9 Sep 2016 00:05
Operator : UM/SJ
Sample : H4688-03 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SS-AST3

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

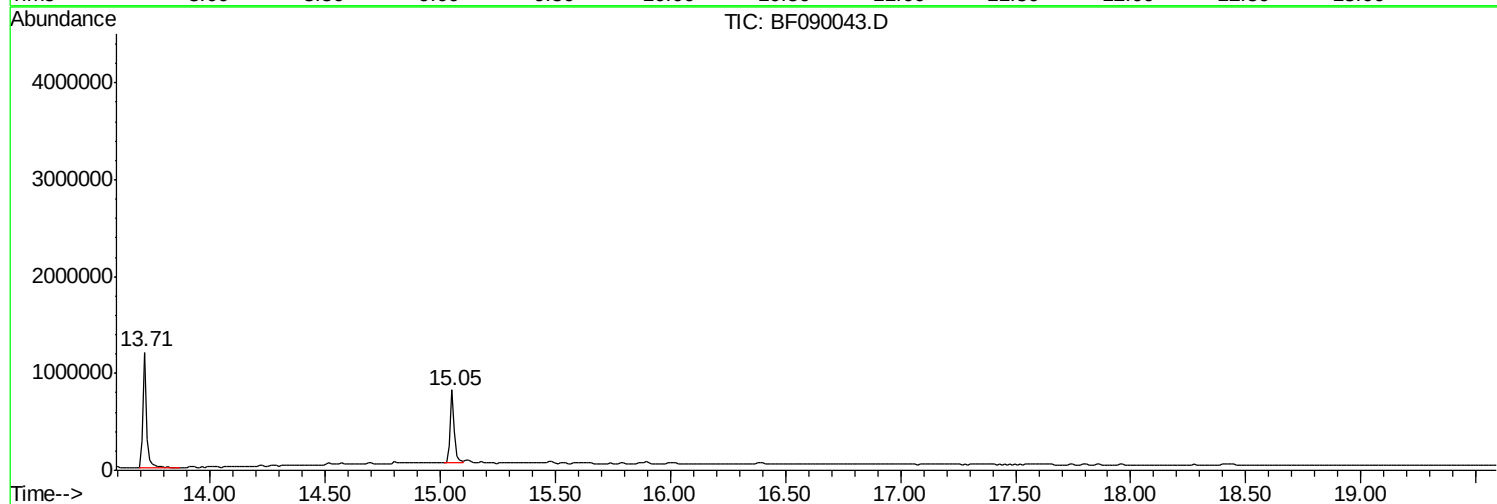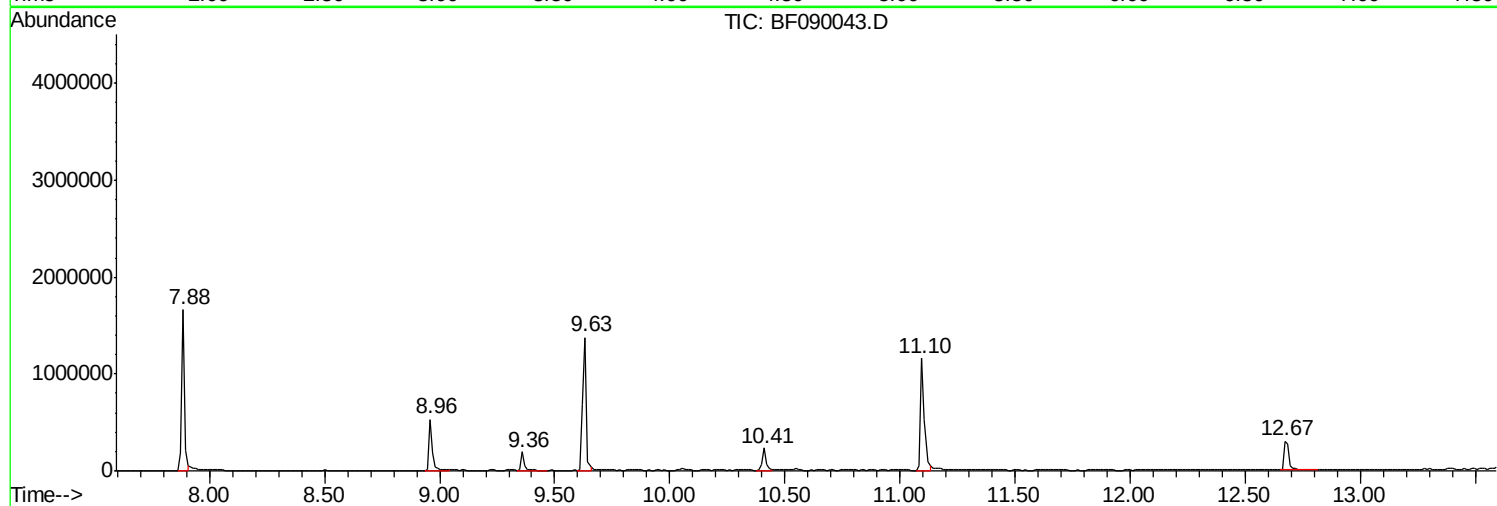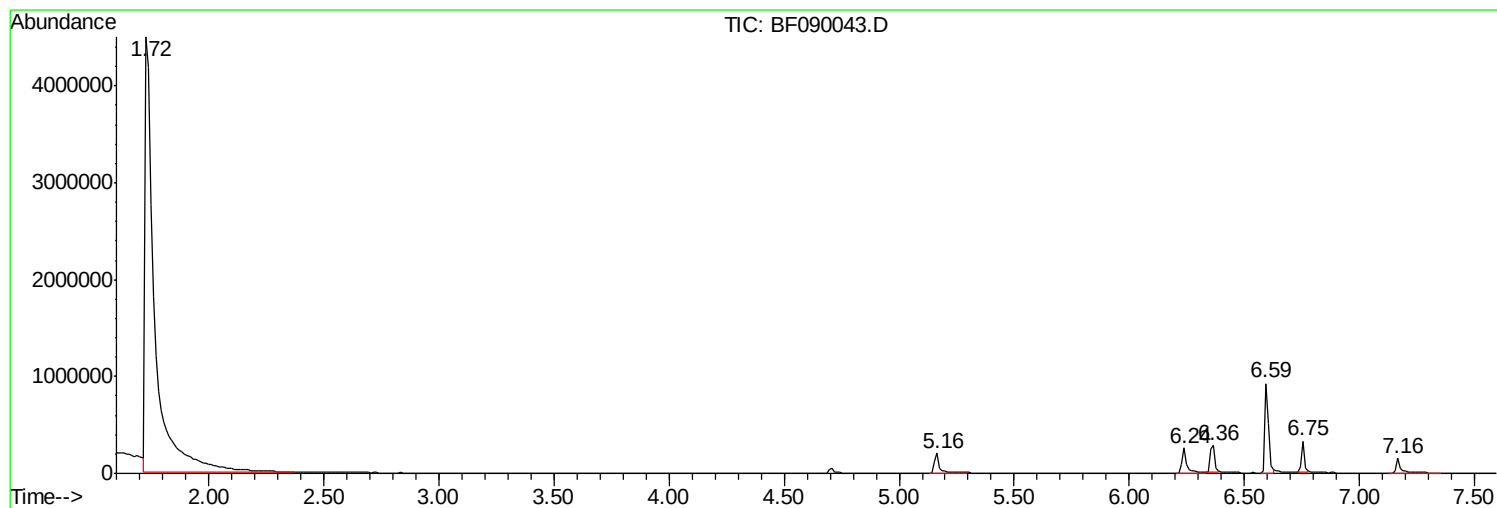

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF090816\
Data File : BF090043.D
Acq On : 9 Sep 2016 00:05
Operator : UM/SJ
Sample : H4688-03 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SS-AST3










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.36 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.36	7.34 ng	393041	1,4-Dichlorobenzene-d4	6.59

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	47
2		5-Aminoindole	132	C8H8N2	005192-03-0	37
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	33
4		1H-Indazole, 7-methyl-	132	C8H8N2	1000316-00-7	32
5		Tranlycypromine-propionyl	189	C12H15NO	1000123-86-3	32

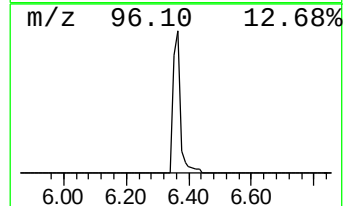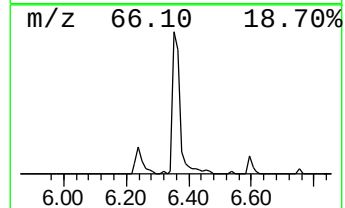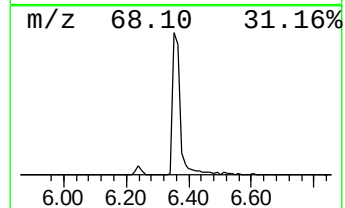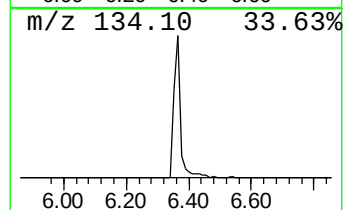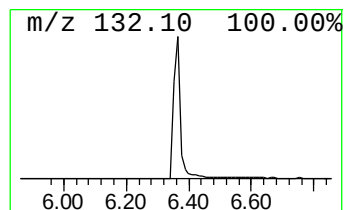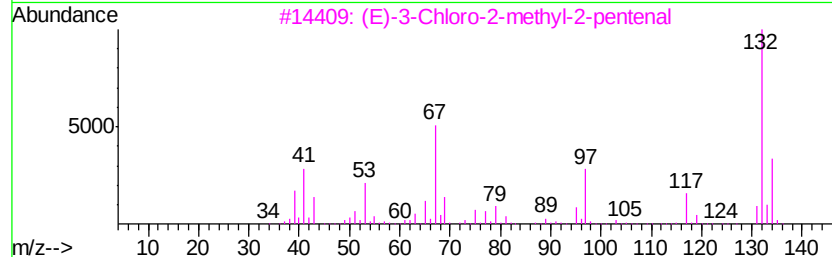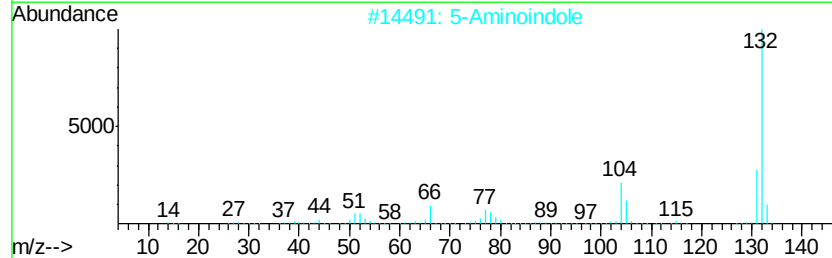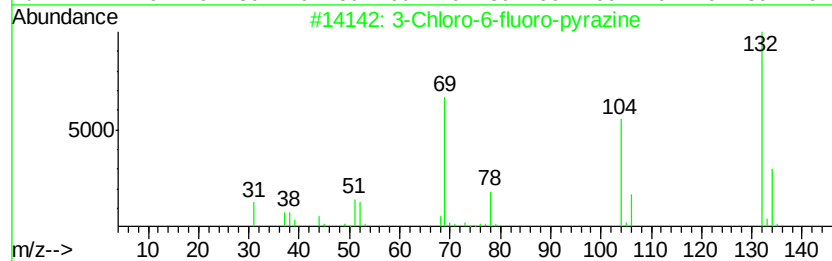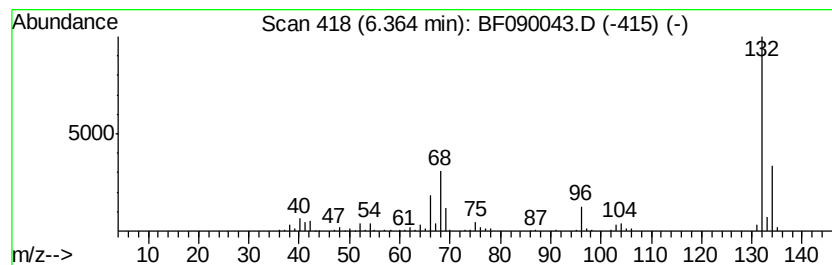

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF090816\
Data File : BF090043.D
Acq On : 9 Sep 2016 00:05
Operator : UM/SJ
Sample : H4688-03 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SS-AST3

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.36	6.36	7.3	ng	393041	1	6.59	1071680	20.0