


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF090817\
 Data File : BF098346.D
 Acq On : 8 Sep 2017 12:16
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 05 17:28:20 2017

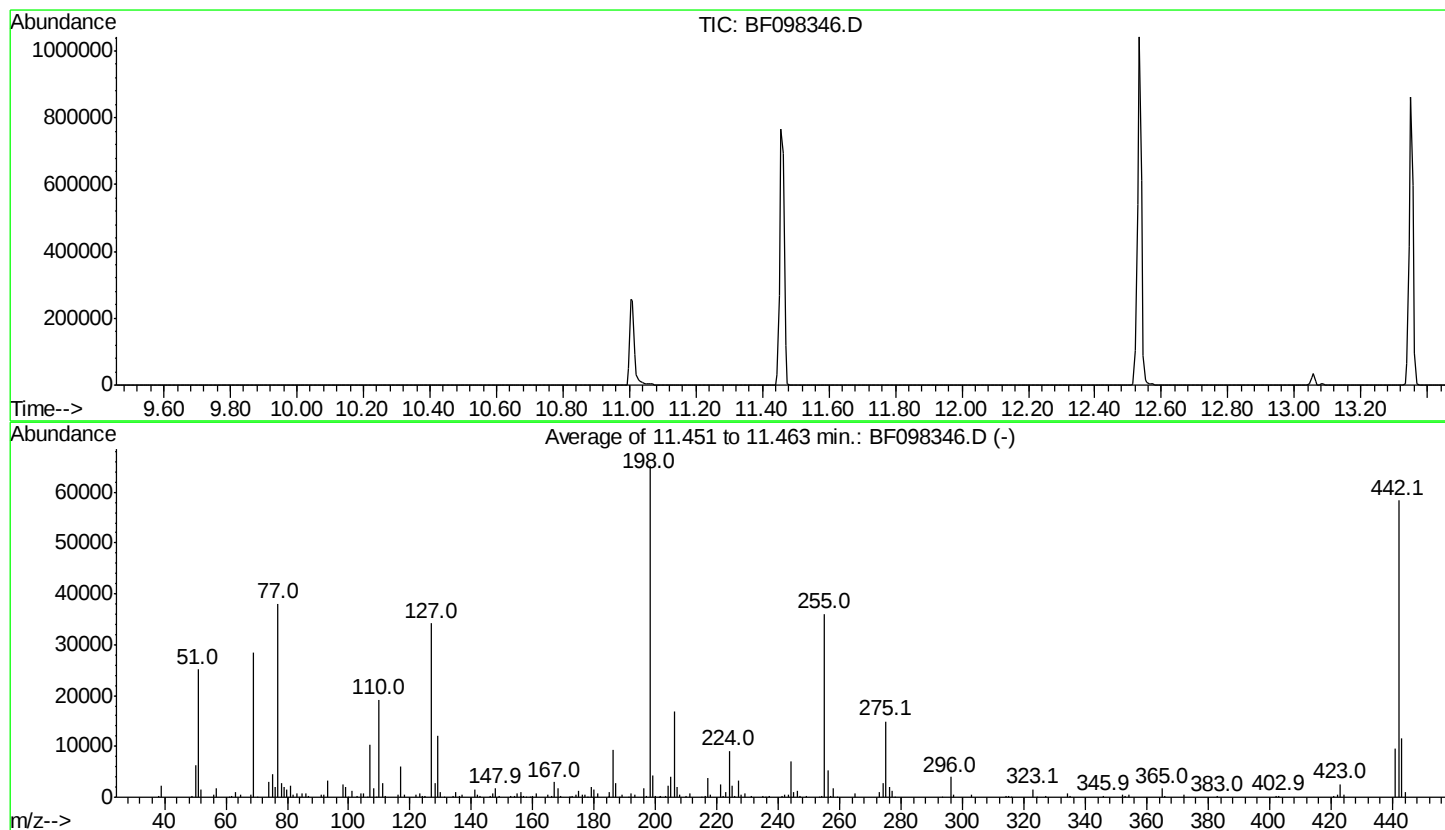

AutoFind: Scans 1592, 1593, 1594; Background Corrected with Scan 1587

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	25176	PASS
68	69	0.00	2	1.5	440	PASS
69	198	0.00	100	43.6	28453	PASS
70	69	0.00	2	0.4	100	PASS
127	198	10	80	52.4	34181	PASS
197	198	0.00	2	0.4	268	PASS
198	198	100	100	100.0	65221	PASS
199	198	5	9	6.6	4303	PASS
275	198	10	60	22.9	14952	PASS
365	198	1	100	2.6	1710	PASS
441	442	0.01	24	16.4	9540	PASS
442	198	50	100	89.4	58317	PASS
443	442	15	24	19.8	11549	PASS