


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF090817\
 Data File : BF098370.D
 Acq On : 9 Sep 2017 00:50
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 05 17:28:20 2017

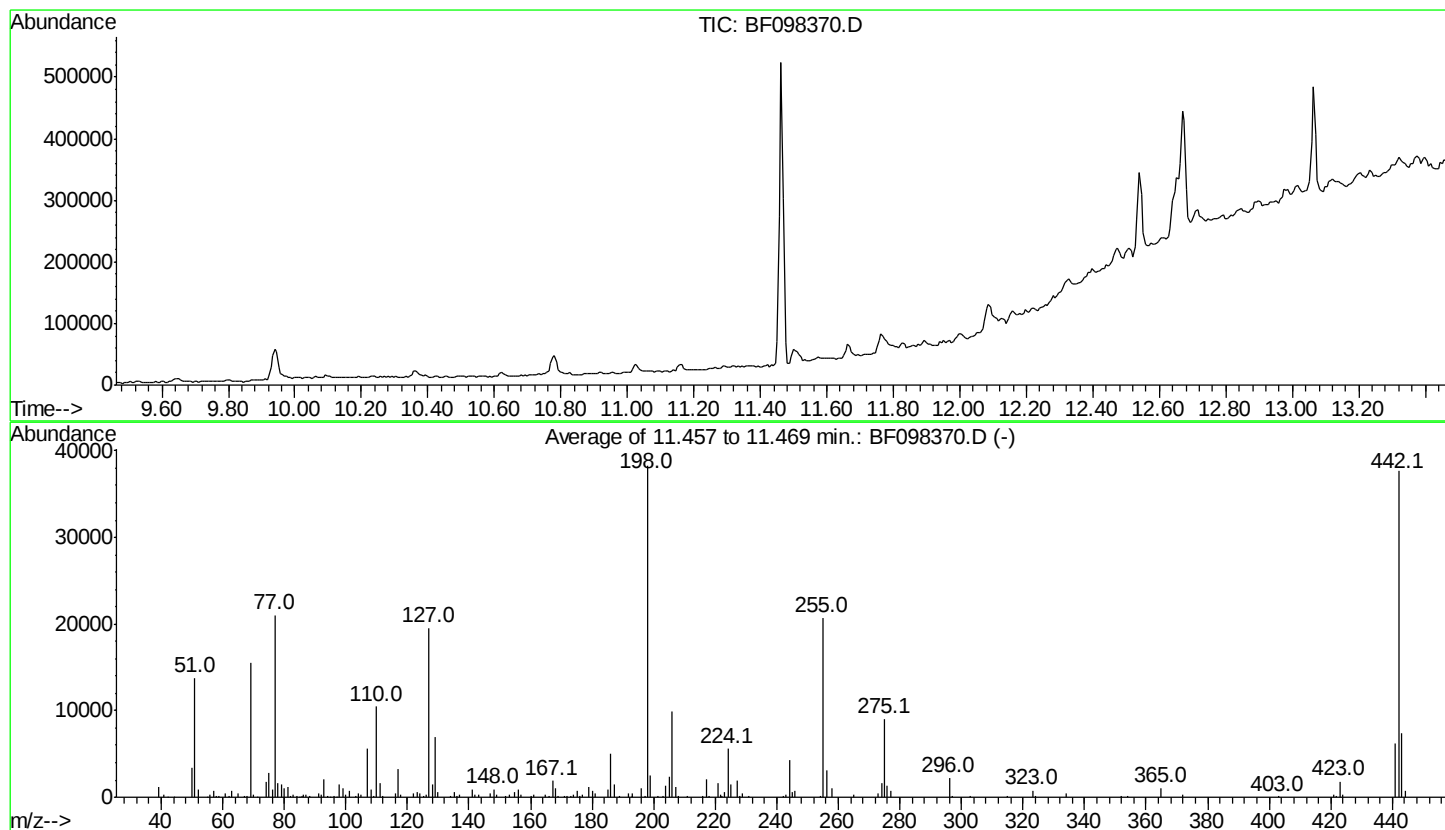

AutoFind: Scans 1593, 1594, 1595; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	13822	PASS
68	69	0.00	2	0.8	126	PASS
69	198	0.00	100	40.5	15515	PASS
70	69	0.00	2	1.6	241	PASS
127	198	10	80	51.1	19575	PASS
197	198	0.00	2	0.3	113	PASS
198	198	100	100	100.0	38293	PASS
199	198	5	9	6.6	2510	PASS
275	198	10	60	23.7	9072	PASS
365	198	1	100	2.9	1098	PASS
441	442	0.01	24	16.6	6251	PASS
442	198	50	100	98.6	37742	PASS
443	442	15	24	19.5	7365	PASS