


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090820\
 Data File : BF121521.D
 Acq On : 8 Sep 2020 14:31
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082720.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 02 17:52:18 2020

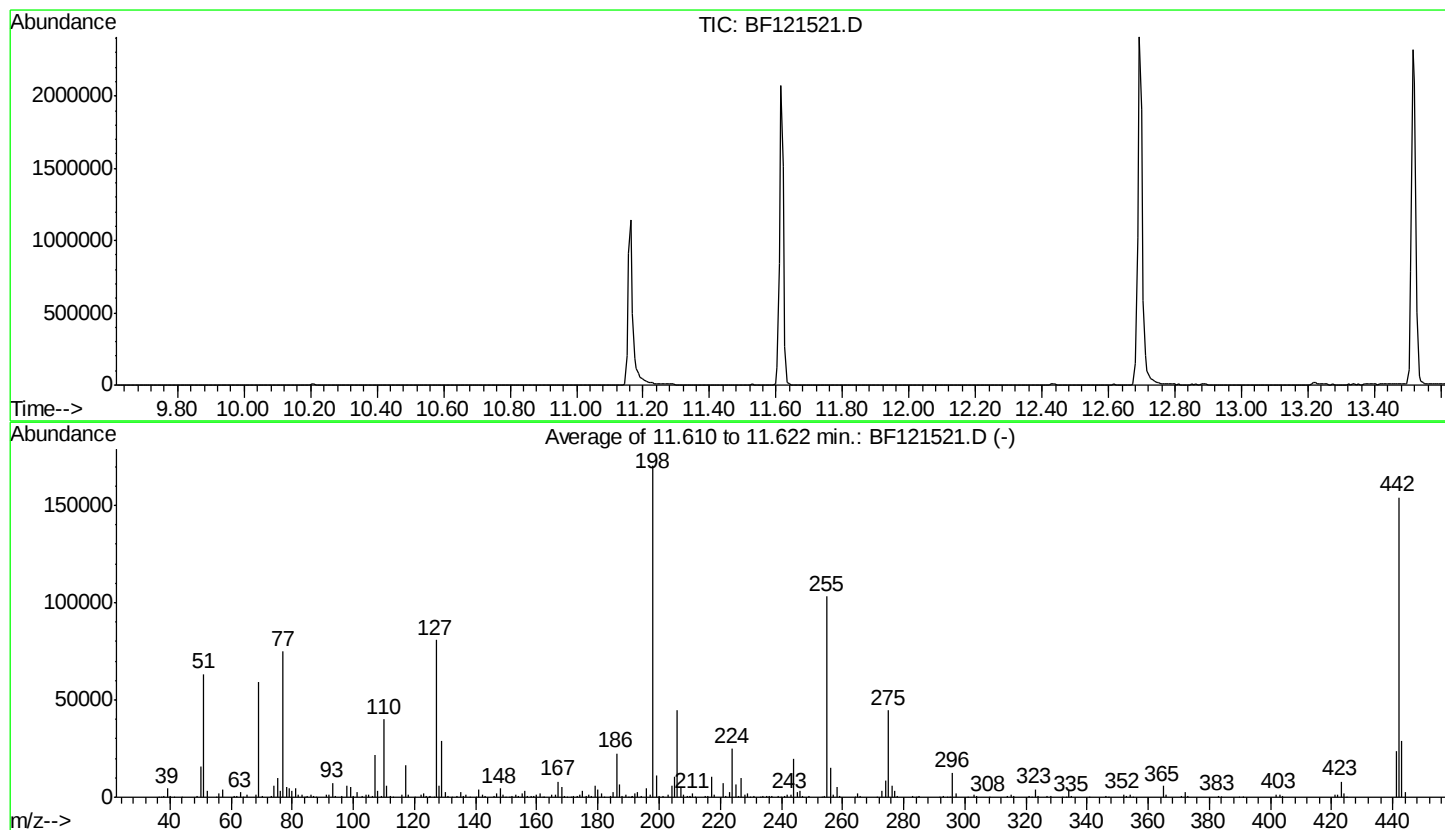

AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	63448	PASS
68	69	0.00	2	1.9	1122	PASS
69	198	0.00	100	34.7	59136	PASS
70	69	0.00	2	0.6	359	PASS
127	198	10	80	47.4	80709	PASS
197	198	0.00	2	0.6	1031	PASS
198	198	100	100	100.0	170349	PASS
199	198	5	9	6.5	11086	PASS
275	198	10	60	26.2	44674	PASS
365	198	1	100	3.4	5757	PASS
441	198	0.01	100	13.8	23511	PASS
442	198	50	100	90.5	154128	PASS
443	442	15	24	18.6	28649	PASS