
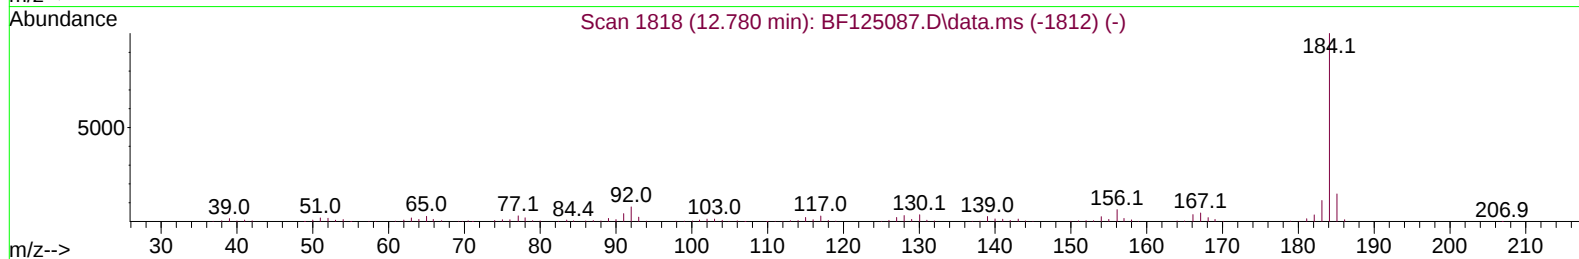
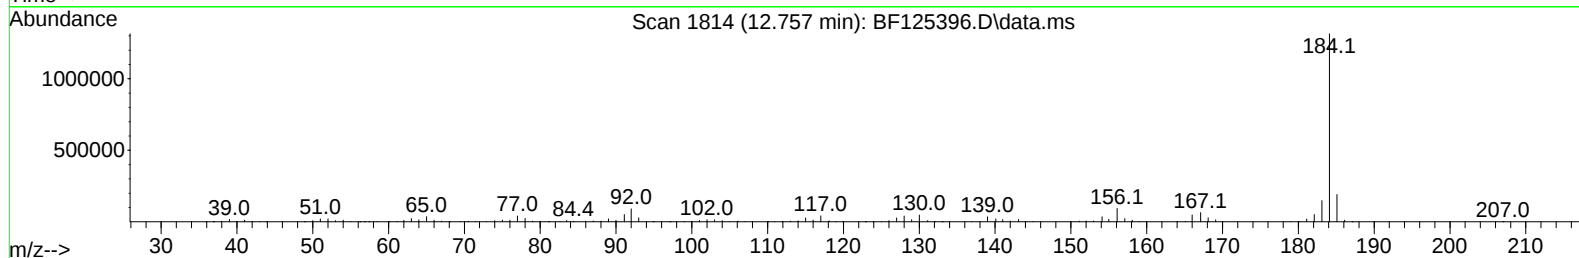


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090821\
Data File : BF125396.D
Acq On : 8 Sep 2021 11:34
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 08 14:08:57 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 03 11:56:34 2021
Response via : Initial Calibration

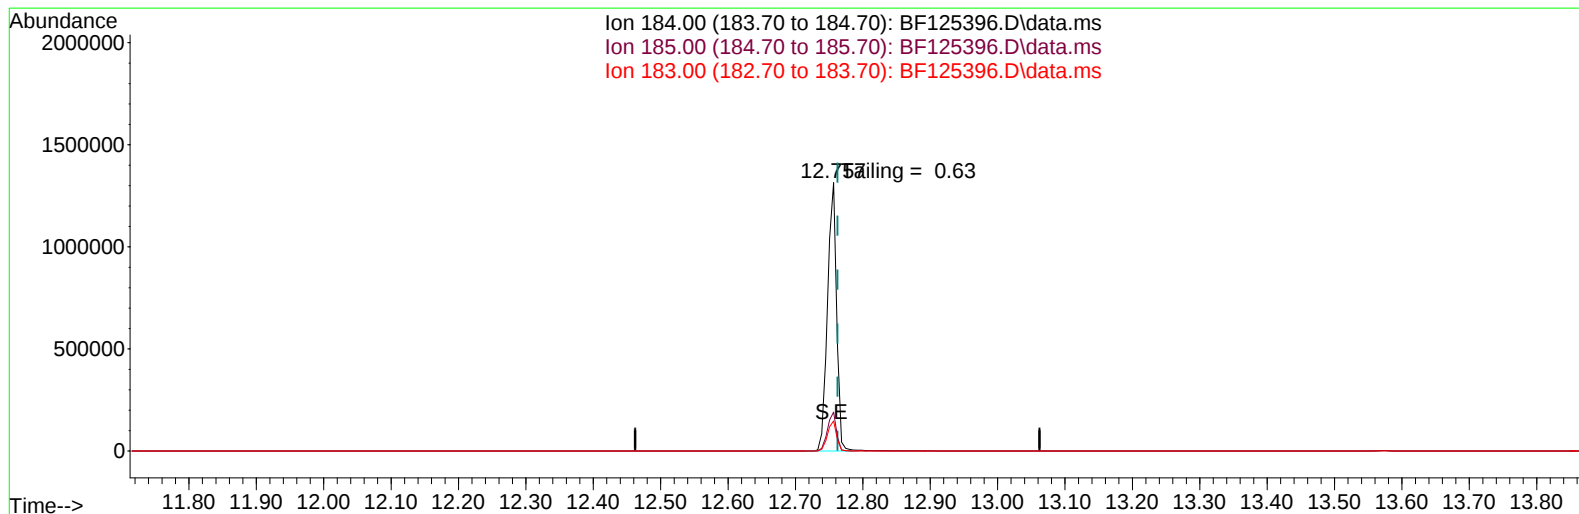

TIC: BF125396.D\data.ms

(77) Benzidine




12.757min (-0.006) 0.00 ng

response 1236711

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.53
183.00	10.10	11.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090821\
Data File : BF125396.D
Acq On : 8 Sep 2021 11:34
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 08 14:08:57 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 03 11:56:34 2021
Response via : Initial Calibration

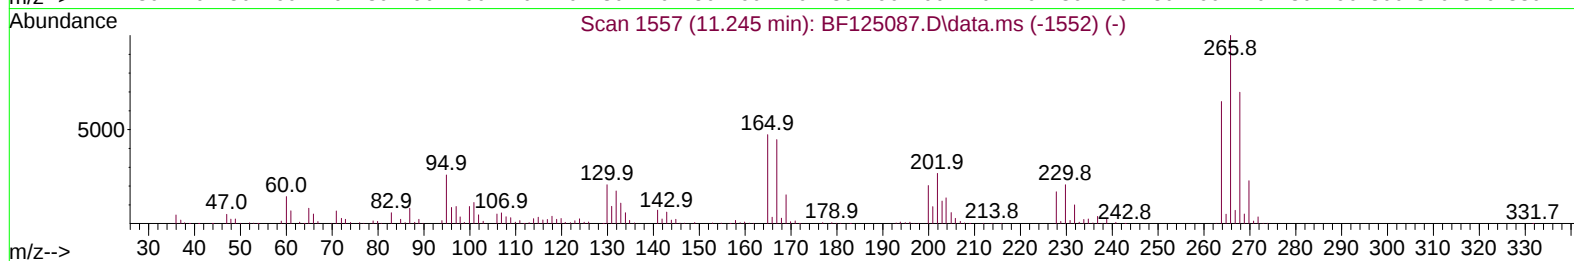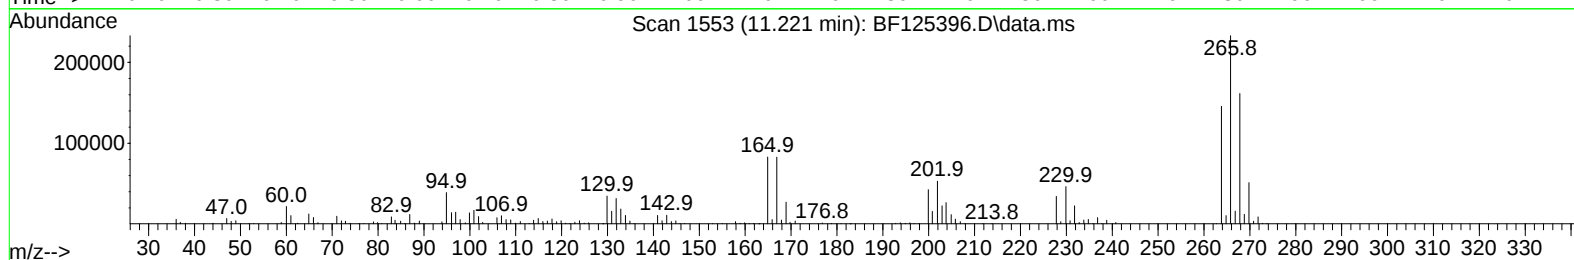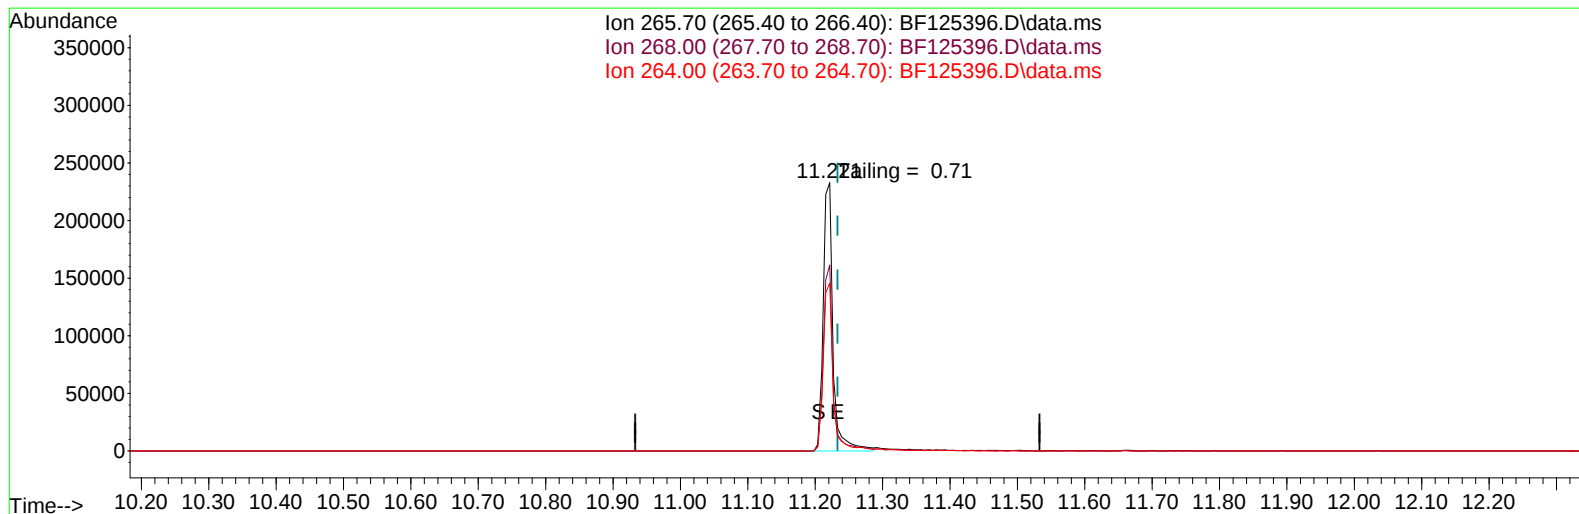

TIC: BF125396.D\data.ms

(70) Pentachlorophenol (C)

11.221min (-0.012) 30467.44 ng

response 240201

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	69.31
264.00	69.90	62.53
0.00	0.00	0.00