
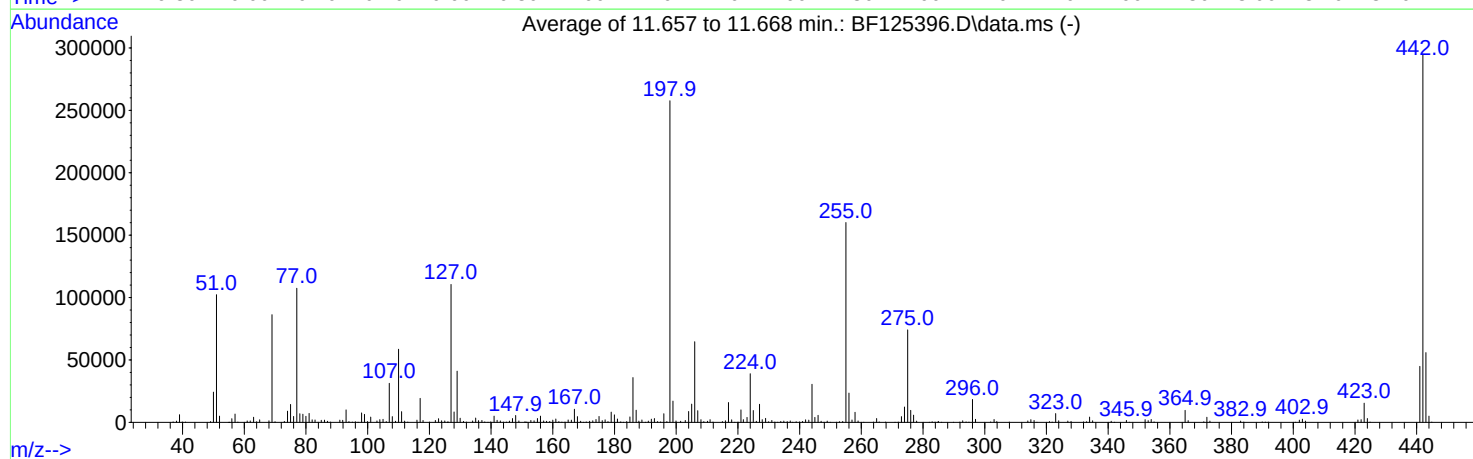


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090821\
 Data File : BF125396.D
 Acq On : 8 Sep 2021 11:34
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 08 14:14:01 2021

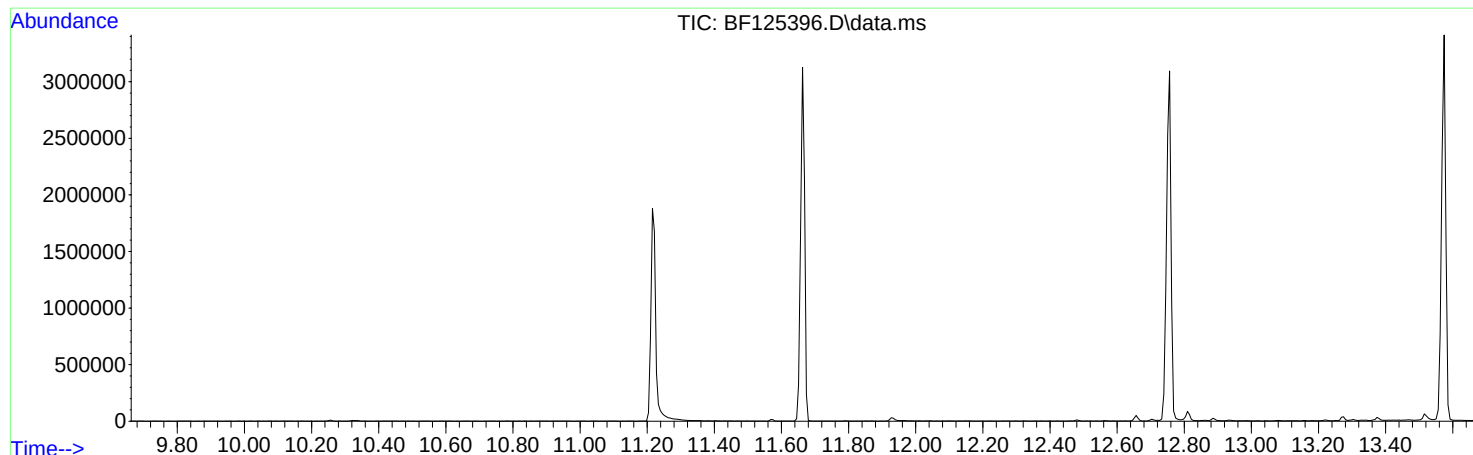




AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.7	102288	PASS
68	69	0.00	2	1.5	1335	PASS
69	198	0.00	100	33.5	86363	PASS
70	69	0.00	2	0.7	576	PASS
127	198	10	80	42.9	110560	PASS
197	198	0.00	2	0.3	655	PASS
198	198	100	100	100.0	257664	PASS
199	198	5	9	6.6	17026	PASS
275	198	10	60	28.8	74091	PASS
365	198	1	100	3.8	9685	PASS
441	198	0.01	100	17.4	44896	PASS
442	442	50	100	100.0	294795	PASS
443	442	15	24	19.0	55949	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090821\
Data File : BF125396.D
Acq On : 8 Sep 2021 11:34
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 08 14:08:57 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 03 11:56:34 2021
Response via : Initial Calibration

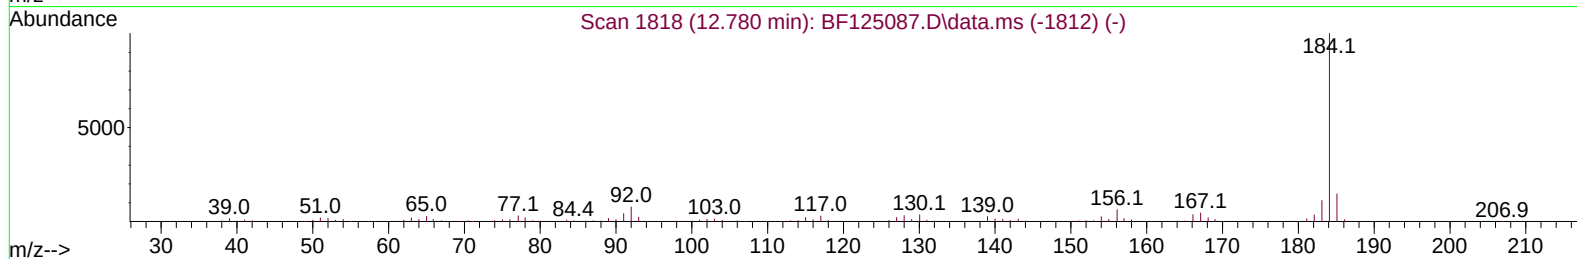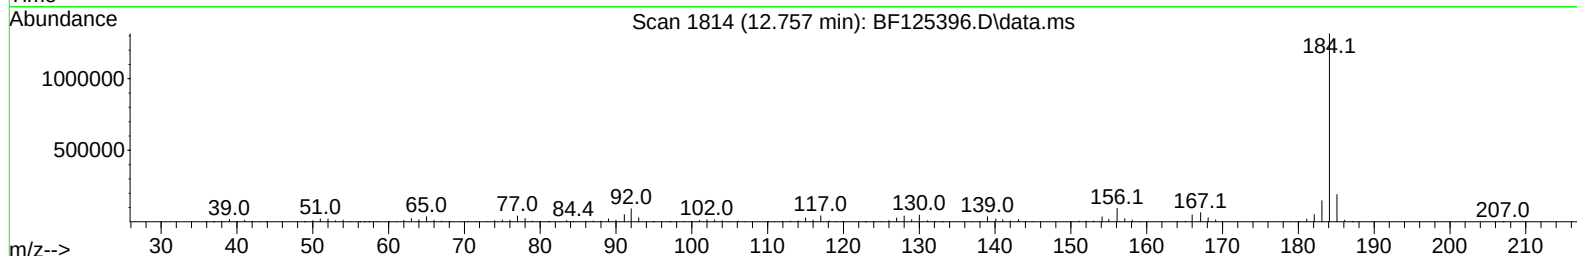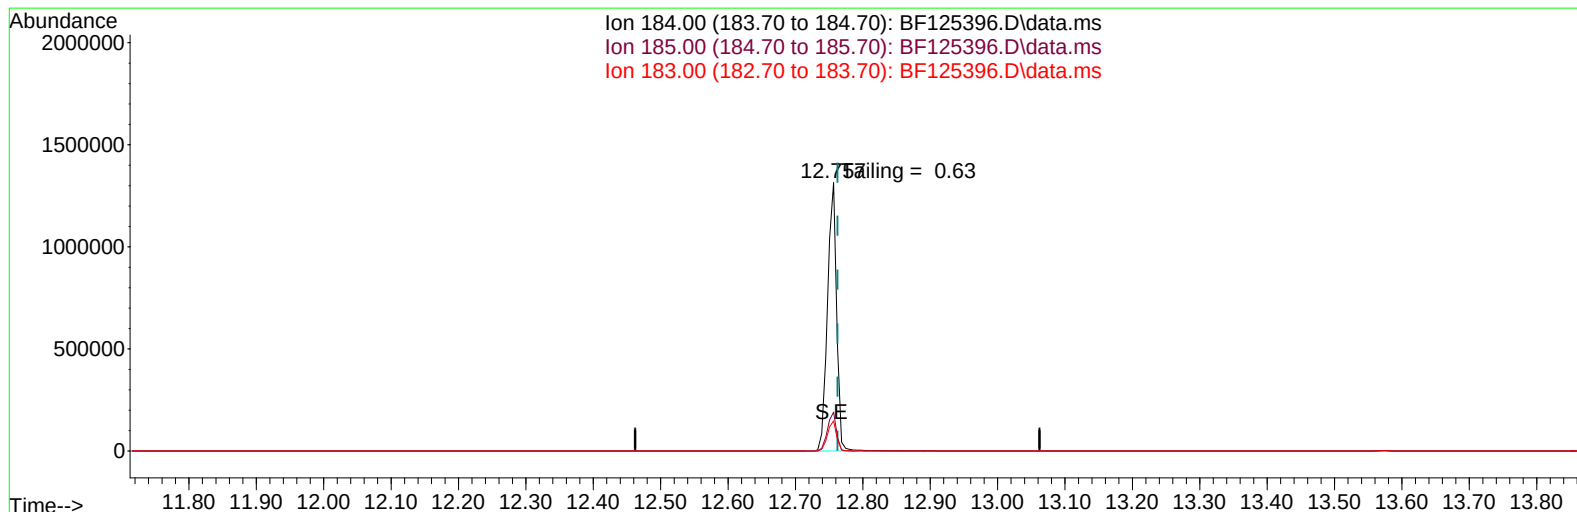

TIC: BF125396.D\data.ms

(77) Benzidine

12.757min (-0.006) 0.00 ng




response 1236711

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.53
183.00	10.10	11.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090821\
 Data File : BF125396.D
 Acq On : 8 Sep 2021 11:34
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 08 14:08:57 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 03 11:56:34 2021
 Response via : Initial Calibration

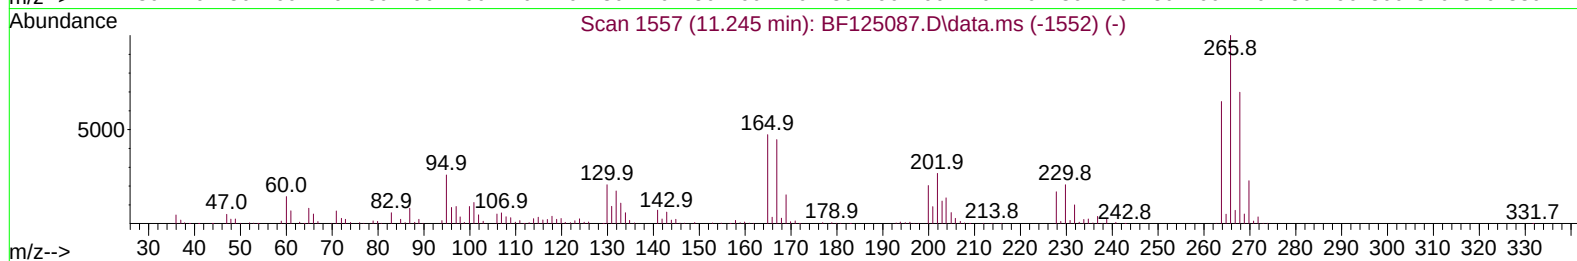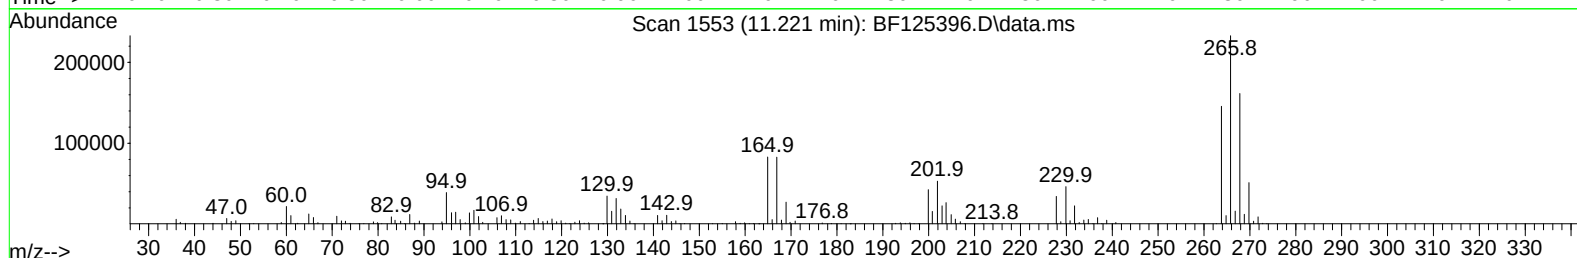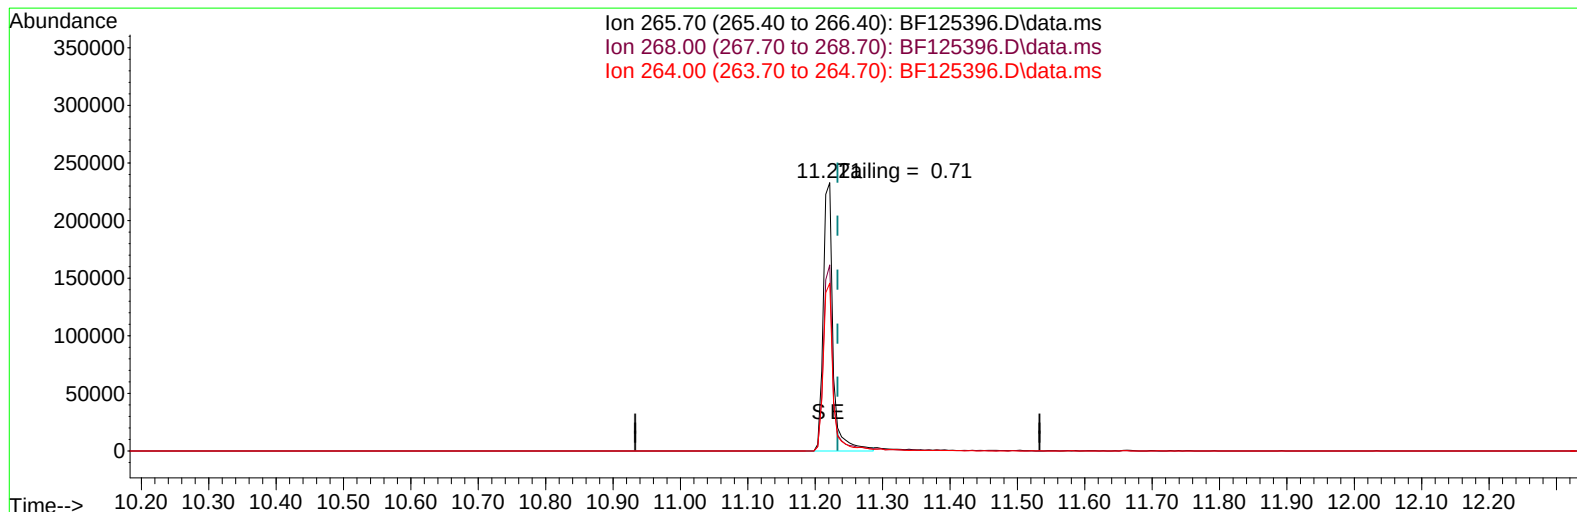

TIC: BF125396.D\data.ms

(70) Pentachlorophenol (C)

11.221min (-0.012) 30467.44 ng

response 240201

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	69.31
264.00	69.90	62.53
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/8/2021	BNA_F	BF125396.D
Compound Name	Response	Retention Time
DDT	607237	13.57
DDD	7868	13.27
DDE	1245	12.93
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9113	616350	1.48

Instrument :
BNA_F
ClientSampleId :
DFTPP