
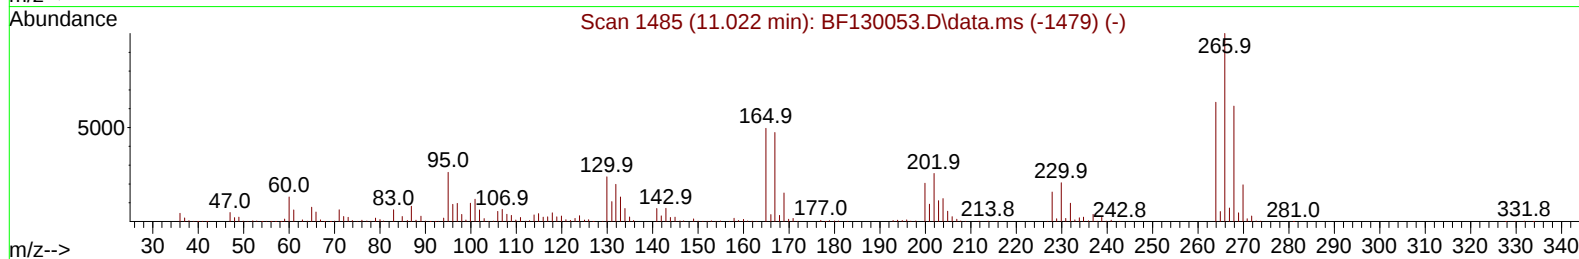
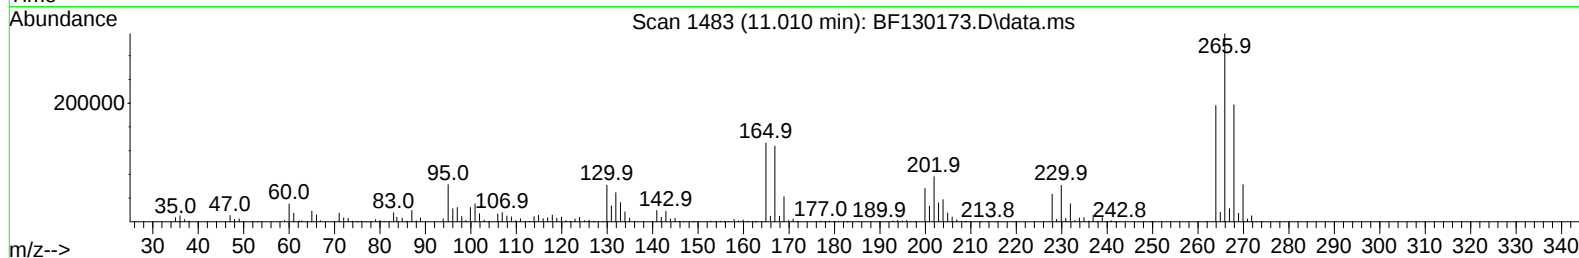


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090822\
Data File : BF130173.D
Acq On : 08 Sep 2022 09:37
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 09 06:10:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 07 02:05:07 2022
Response via : Initial Calibration

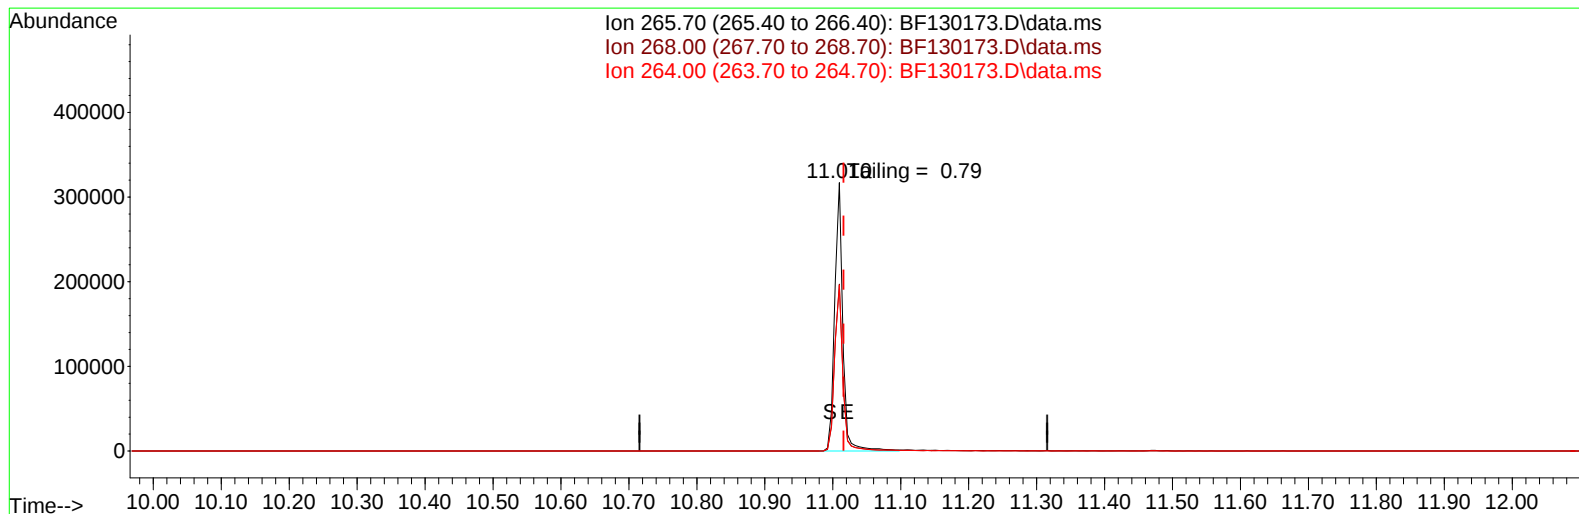

TIC: BF130173.D\data.ms

(70) Pentachlorophenol (C)




11.010min (-0.006) 209625.14 ng

response 262830

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	62.19
264.00	59.90	61.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090822\
Data File : BF130173.D
Acq On : 08 Sep 2022 09:37
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 09 06:10:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 07 02:05:07 2022
Response via : Initial Calibration

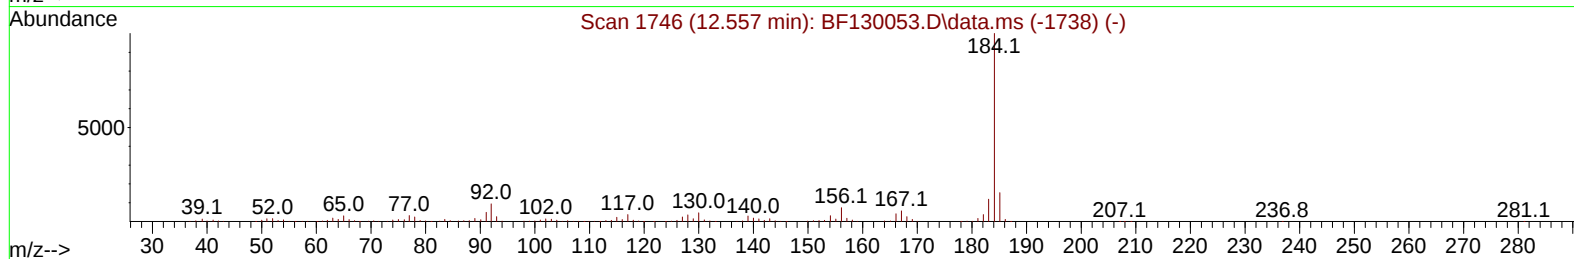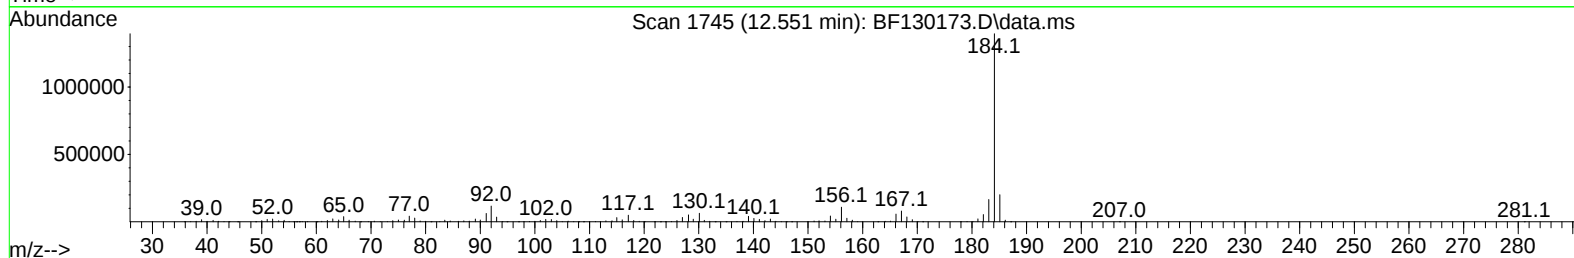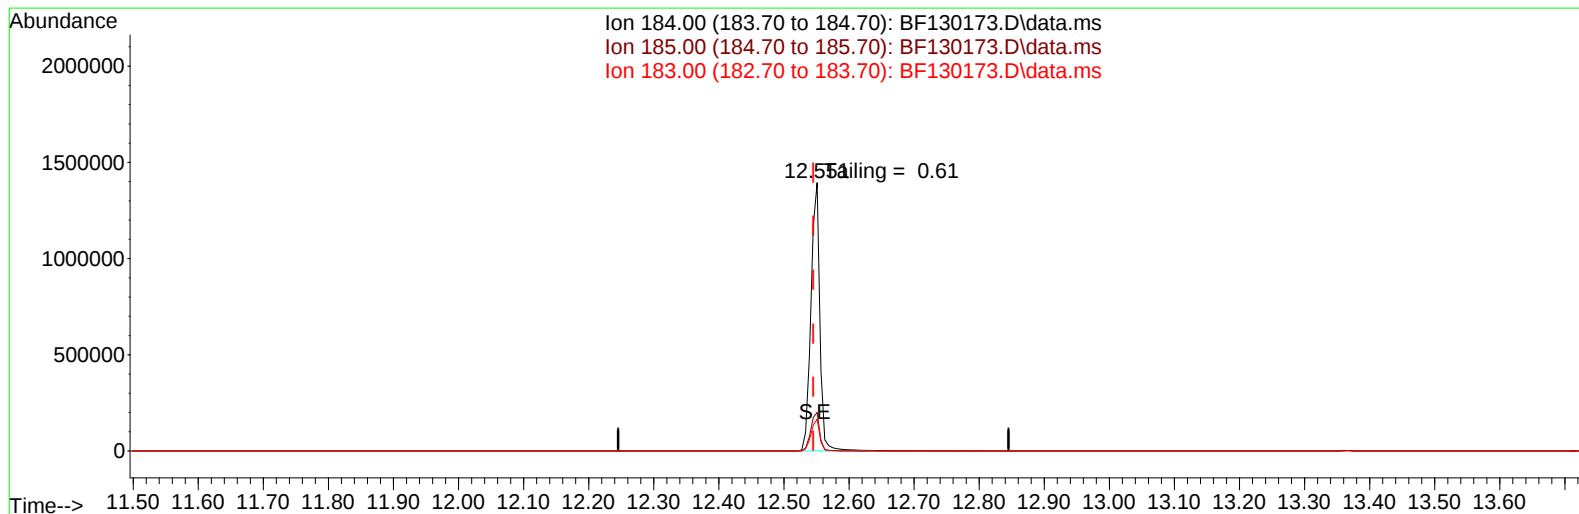

TIC: BF130173.D\data.ms

(77) Benzidine

12.551min (+ 0.006) 209831.06 ng

response 1331328

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.40
183.00	11.80	11.88
0.00	0.00	0.00