

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090822\
 Data File : BF130184.D
 Acq On : 08 Sep 2022 18:14
 Operator : CG\JU
 Sample : N4513-01RE
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 72-11939RE

Quant Time: Sep 09 01:07:22 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 07 02:05:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.692	152	146407	20.000	ng	0.00
21) Naphthalene-d8	7.975	136	551322	20.000	ng	0.00
39) Acenaphthene-d10	9.722	164	250485	20.000	ng	-0.01
64) Phenanthrene-d10	11.204	188	341706	20.000	ng	0.00
76) Chrysene-d12	13.833	240	273686	20.000	ng	-0.01
86) Perylene-d12	15.233	264	340799	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.292	112	870802	100.973	ng	0.00
7) Phenol-d6	6.322	99	1028770	95.684	ng	-0.01
23) Nitrobenzene-d5	7.257	82	612946	71.449	ng	-0.01
42) 2,4,6-Tribromophenol	10.510	330	170002	74.559	ng	-0.01
45) 2-Fluorobiphenyl	9.051	172	809640	53.590	ng	0.00
79) Terphenyl-d14	12.786	244	460646	29.187	ng	-0.01


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090822\
Data File : BF130184.D
Acq On : 08 Sep 2022 18:14
Operator : CG\JU
Sample : N4513-01RE
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
72-11939RE

Quant Time: Sep 09 01:07:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 07 02:05:07 2022
Response via : Initial Calibration




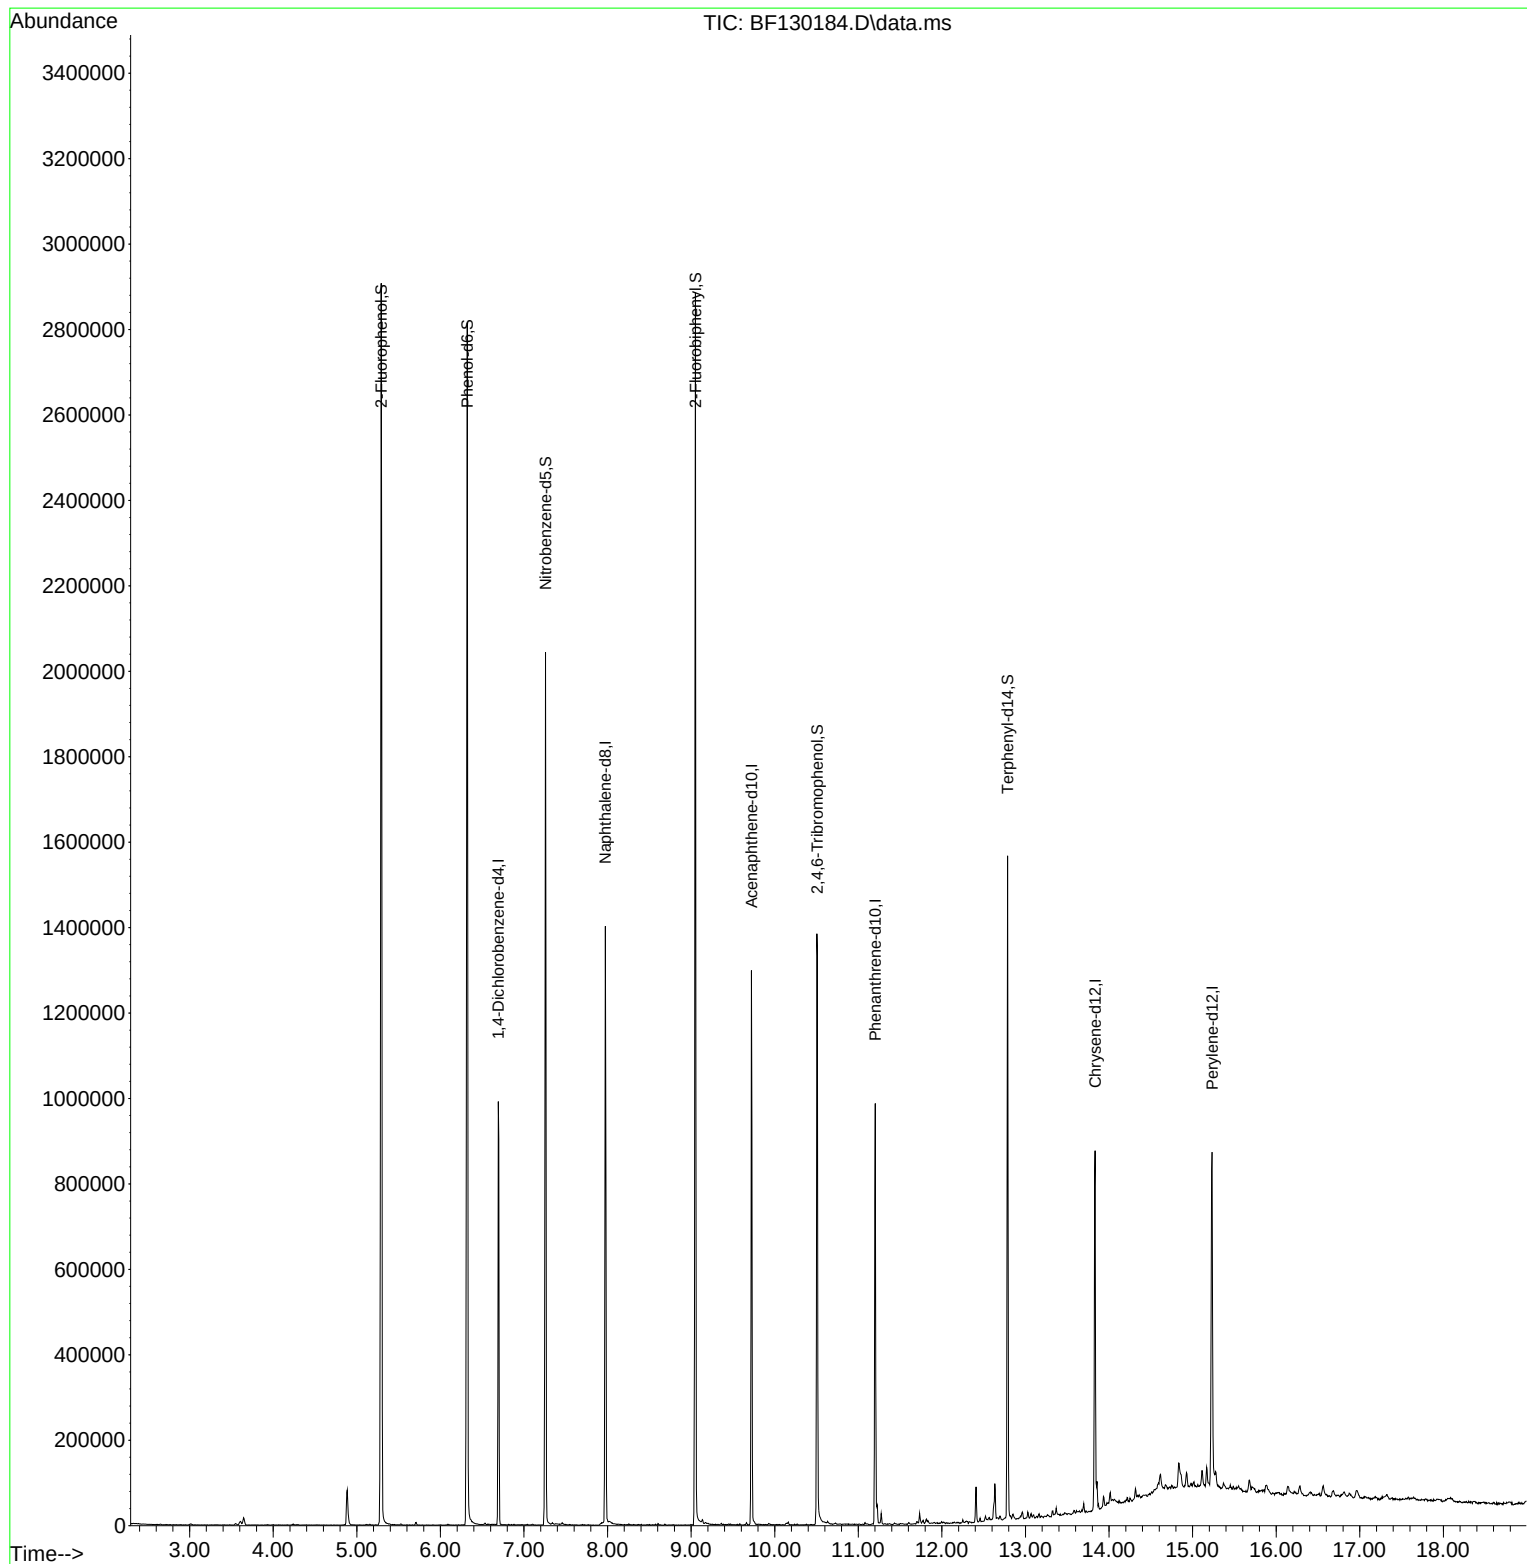


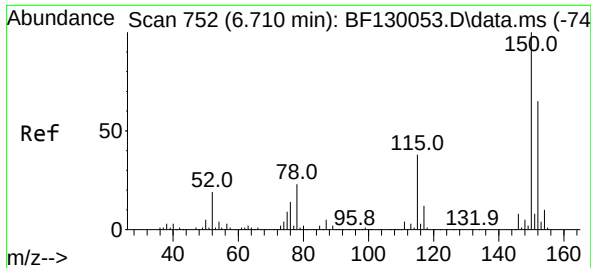

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.692 min Scan# 74
 Delta R.T. -0.006 min
 Lab File: BF130184.D
 Acq: 08 Sep 2022 18:14




Instrument :
 BNA_F
 ClientSampleId :
 72-11939RE


Tgt Ion:152 Resp: 146407
 Ion Ratio Lower Upper
 152 100
 150 157.5 126.9 190.3
 115 64.8 53.4 80.0

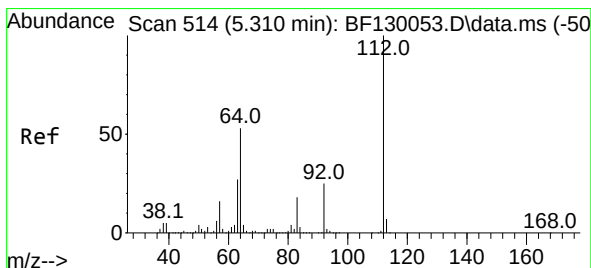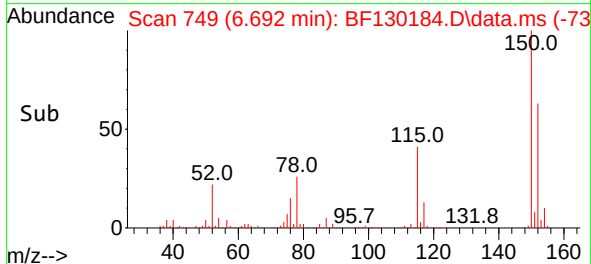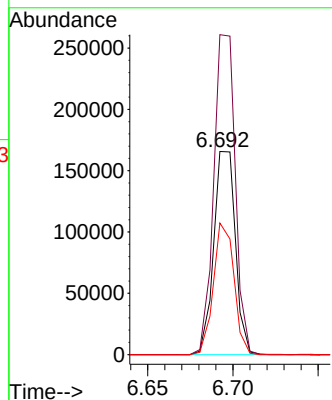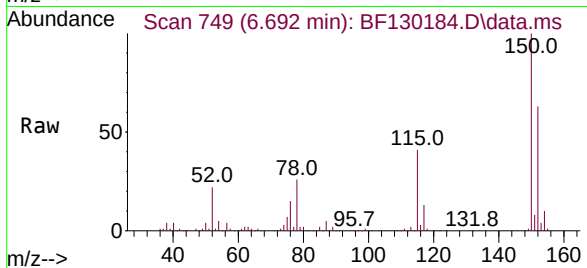

#5
 2-Fluorophenol
 Concen: 100.973 ng
 RT: 5.292 min Scan# 511
 Delta R.T. -0.006 min
 Lab File: BF130184.D
 Acq: 08 Sep 2022 18:14

Tgt Ion:112 Resp: 870802
 Ion Ratio Lower Upper
 112 100
 64 56.9 47.6 71.4
 63 28.7 24.6 37.0


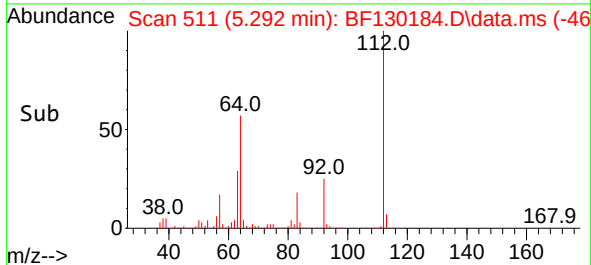
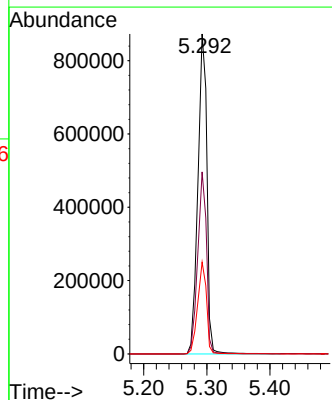
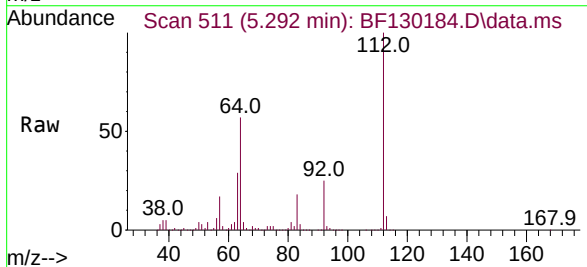


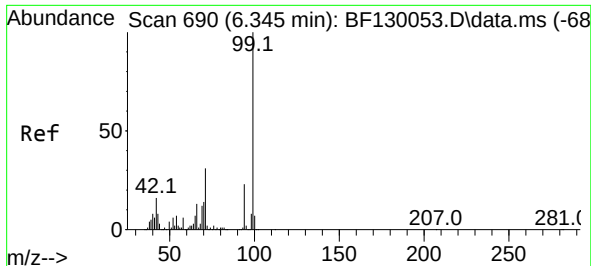

#7
Phenol-d6
Concen: 95.684 ng
RT: 6.322 min Scan# 68
Delta R.T. -0.012 min
Lab File: BF130184.D
Acq: 08 Sep 2022 18:14




Instrument :
BNA_F
ClientSampleId :
72-11939RE


Tgt Ion: 99 Resp: 1028770
Ion Ratio Lower Upper
99 100
42 15.9 15.0 22.4
71 32.2 28.8 43.2

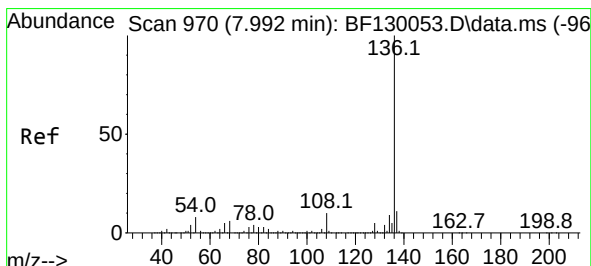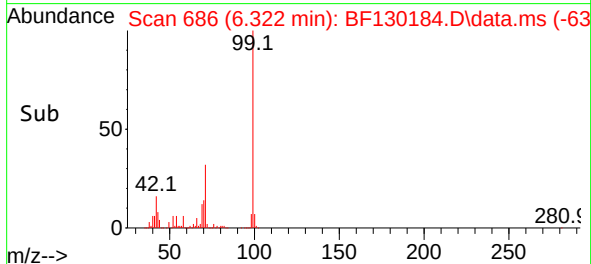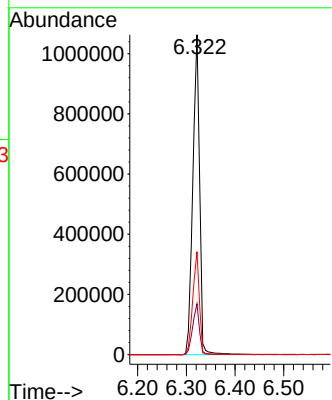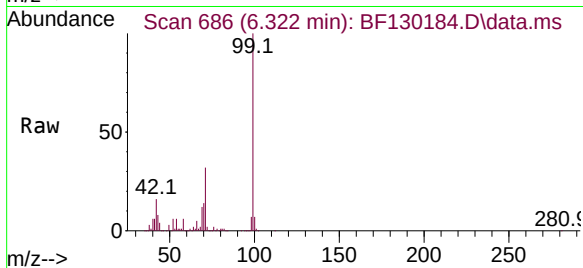

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 7.975 min Scan# 967
Delta R.T. -0.006 min
Lab File: BF130184.D
Acq: 08 Sep 2022 18:14

Tgt Ion: 136 Resp: 551322
Ion Ratio Lower Upper
136 100
137 11.0 8.4 12.6
54 7.2 6.2 9.2
68 6.0 4.2 6.4


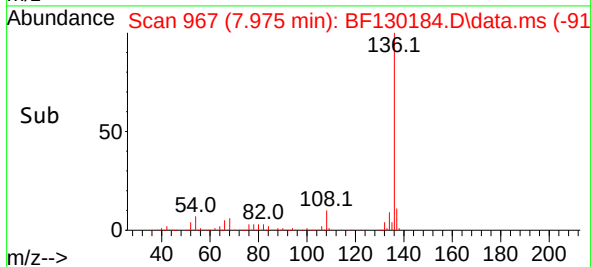
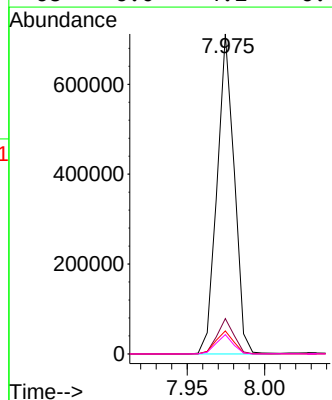
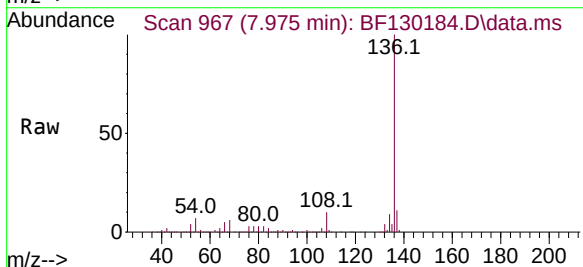


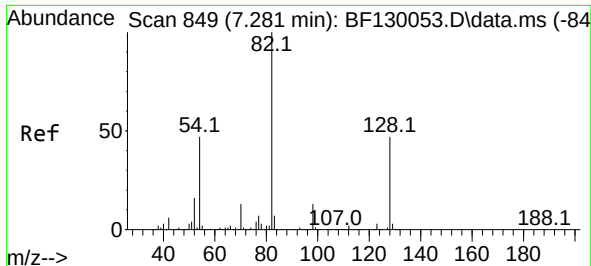

#23
Nitrobenzene-d5
Concen: 71.449 ng
RT: 7.257 min Scan# 84
Delta R.T. -0.012 min
Lab File: BF130184.D
Acq: 08 Sep 2022 18:14




Instrument :
BNA_F
ClientSampleId :
72-11939RE


Tgt Ion: 82 Resp: 612946
Ion Ratio Lower Upper
82 100
128 44.9 36.1 54.1
54 47.0 40.0 60.0

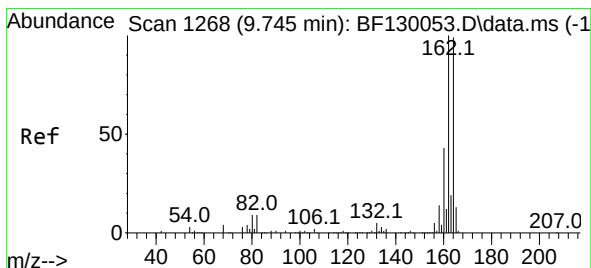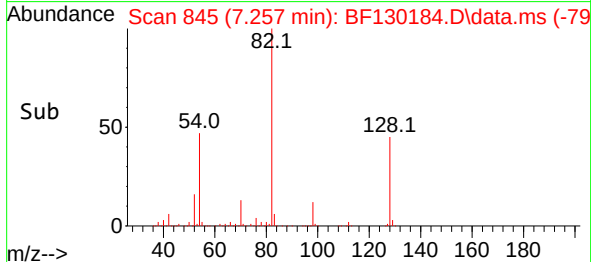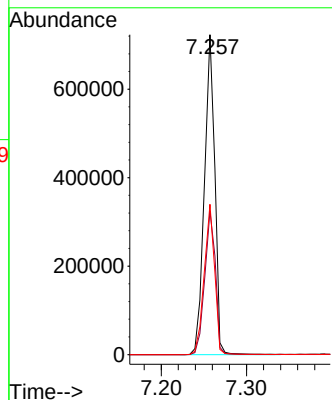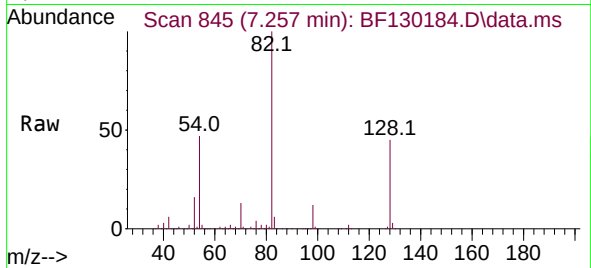

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.722 min Scan# 1264
Delta R.T. -0.012 min
Lab File: BF130184.D
Acq: 08 Sep 2022 18:14

Tgt Ion:164 Resp: 250485
Ion Ratio Lower Upper
164 100
162 99.4 82.0 123.0
160 43.2 35.4 53.0

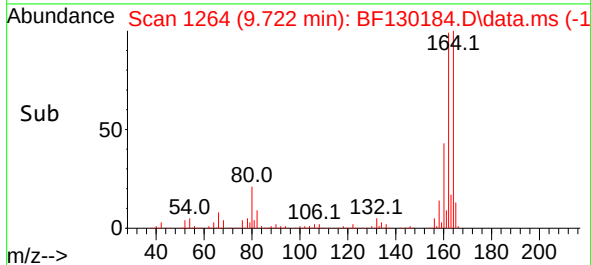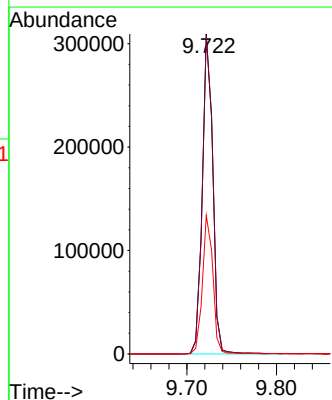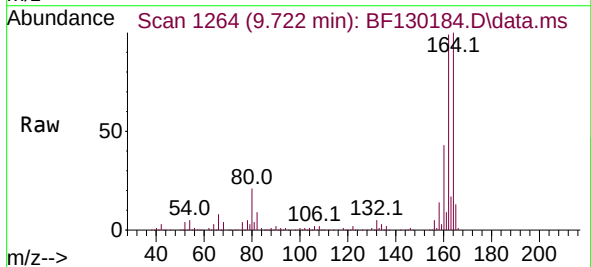

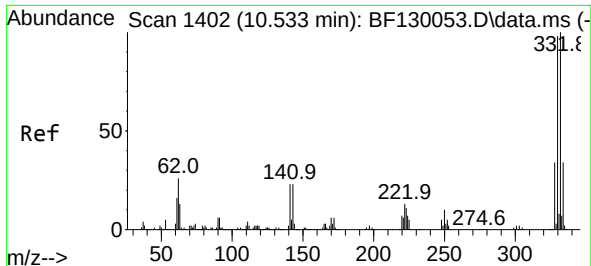

#42

2,4,6-Tribromophenol

Concen: 74.559 ng

RT: 10.510 min Scan# 1398

Delta R.T. -0.012 min

Lab File: BF130184.D

Acq: 08 Sep 2022 18:14

Instrument :

BNA_F

ClientSampleId :

72-11939RE





Tgt Ion:330 Resp: 170002

Ion Ratio Lower Upper

330 100

332 105.4 82.6 124.0

141 35.4 27.6 41.4

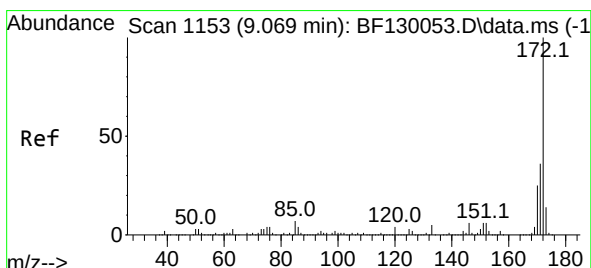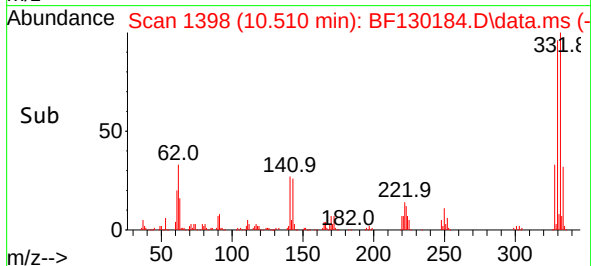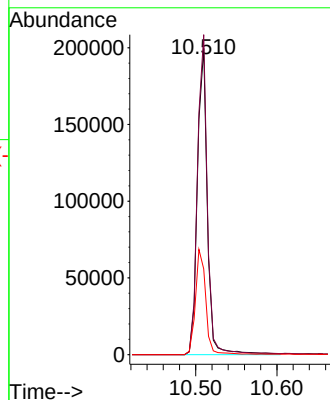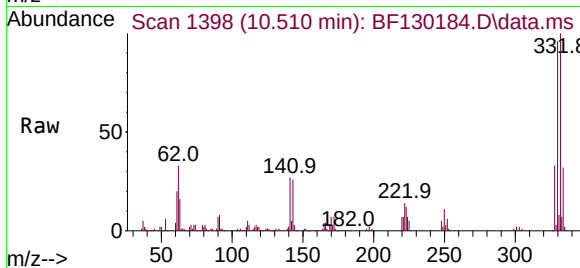

#45

2-Fluorobiphenyl

Concen: 53.590 ng

RT: 9.051 min Scan# 1150

Delta R.T. -0.006 min

Lab File: BF130184.D

Acq: 08 Sep 2022 18:14




Tgt Ion:172 Resp: 809640


Ion Ratio Lower Upper

172 100

171 34.7 28.4 42.6

170 23.1 19.1 28.7


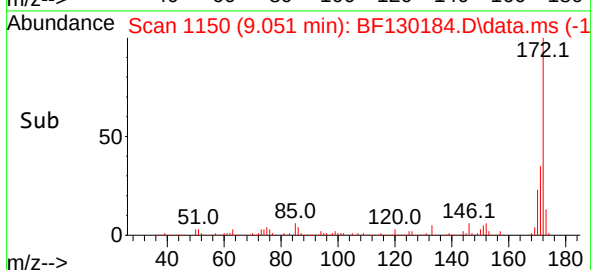
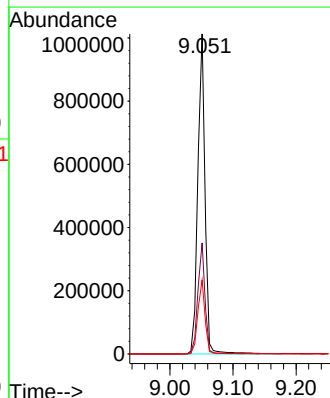
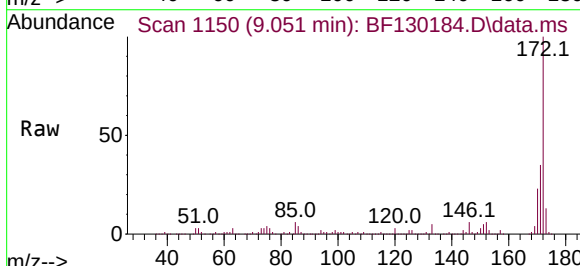


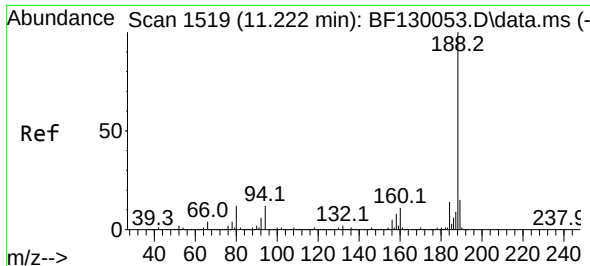

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.204 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF130184.D
Acq: 08 Sep 2022 18:14




Instrument :
BNA_F
ClientSampleId :
72-11939RE


Tgt Ion:188 Resp: 341706
Ion Ratio Lower Upper
188 100
94 9.8 7.4 11.2
80 10.0 7.9 11.9

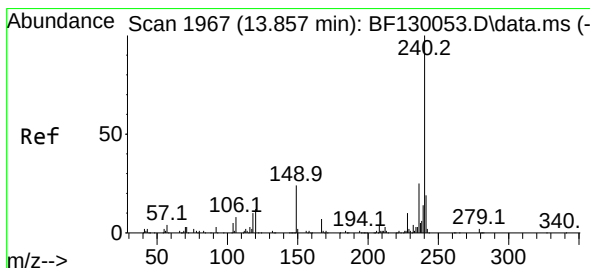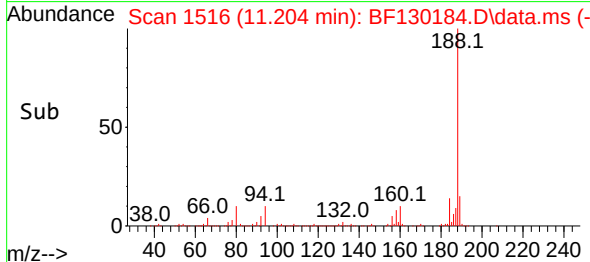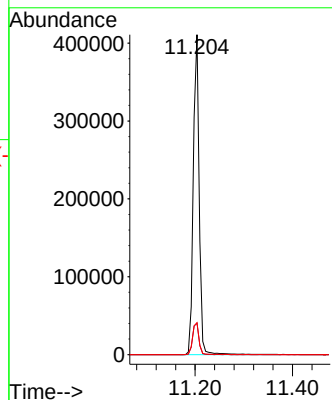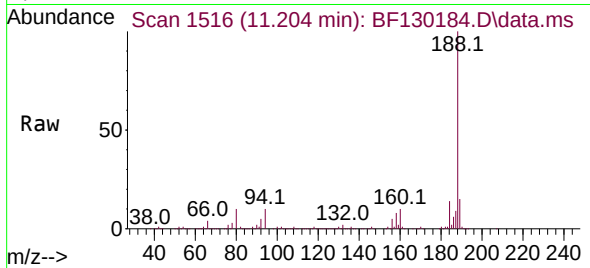

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.833 min Scan# 1963
Delta R.T. -0.012 min
Lab File: BF130184.D
Acq: 08 Sep 2022 18:14

Tgt Ion:240 Resp: 273686
Ion Ratio Lower Upper
240 100
120 11.5 9.2 13.8
236 25.4 20.7 31.1


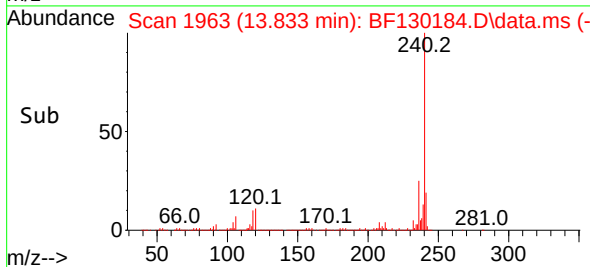
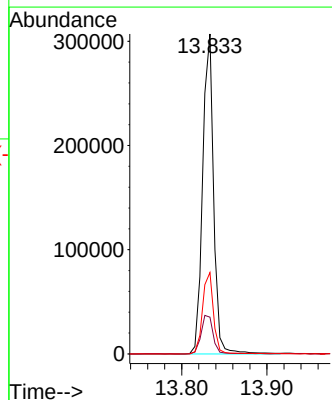
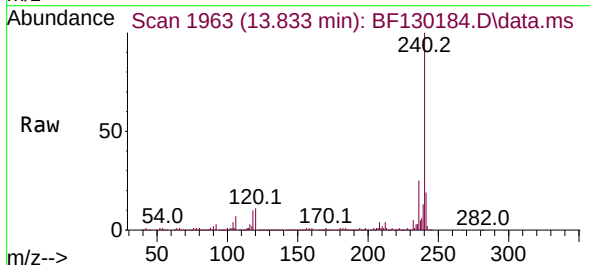


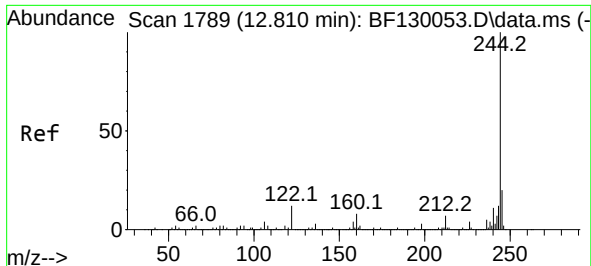

#79
Terphenyl-d14
Concen: 29.187 ng
RT: 12.786 min Scan# 11
Delta R.T. -0.012 min
Lab File: BF130184.D
Acq: 08 Sep 2022 18:14

Instrument :
BNA_F
ClientSampleId :
72-11939RE

Tgt Ion:244 Resp: 460646
Ion Ratio Lower Upper
244 100
212 6.8 5.9 8.9
122 12.7 9.9 14.9

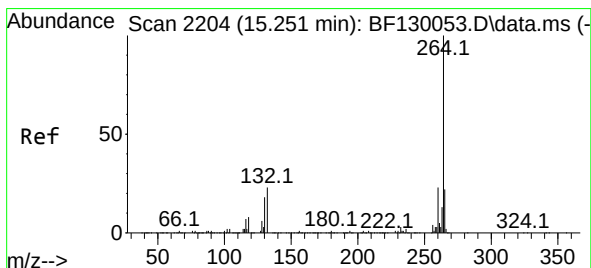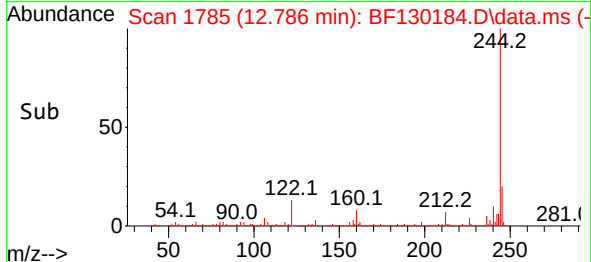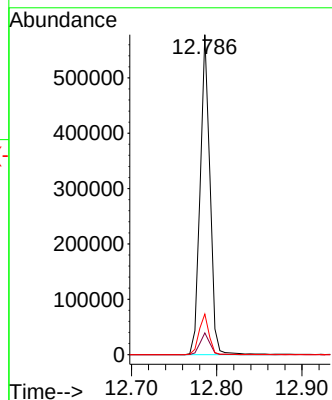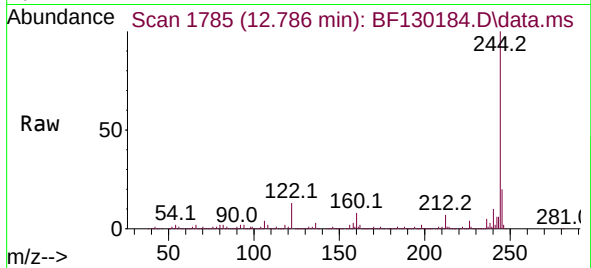

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.233 min Scan# 2201
Delta R.T. -0.006 min
Lab File: BF130184.D
Acq: 08 Sep 2022 18:14

Tgt Ion:264 Resp: 340799
Ion Ratio Lower Upper
264 100
260 23.5 19.1 28.7
265 20.9 16.7 25.1

